

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040425\
 Data File : P0110241.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Apr 2025 15:51
 Operator : YP/AJ
 Sample : Q1720-01 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 GAS-CAM-03

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/07/2025
 Supervised By :mohammad ahmed 04/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 01:16:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.688	3.686	13511611	7900053	1.485m	1.506m
2) SA Decachlor...	8.739	8.690	11370282	2885909	1.479	1.190

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040425\
Data File : PO110241.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Apr 2025 15:51
Operator : YP/AJ
Sample : Q1720-01 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
GAS-CAM-03


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/07/2025
Supervised By :mohammad ahmed 04/09/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 01:16:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

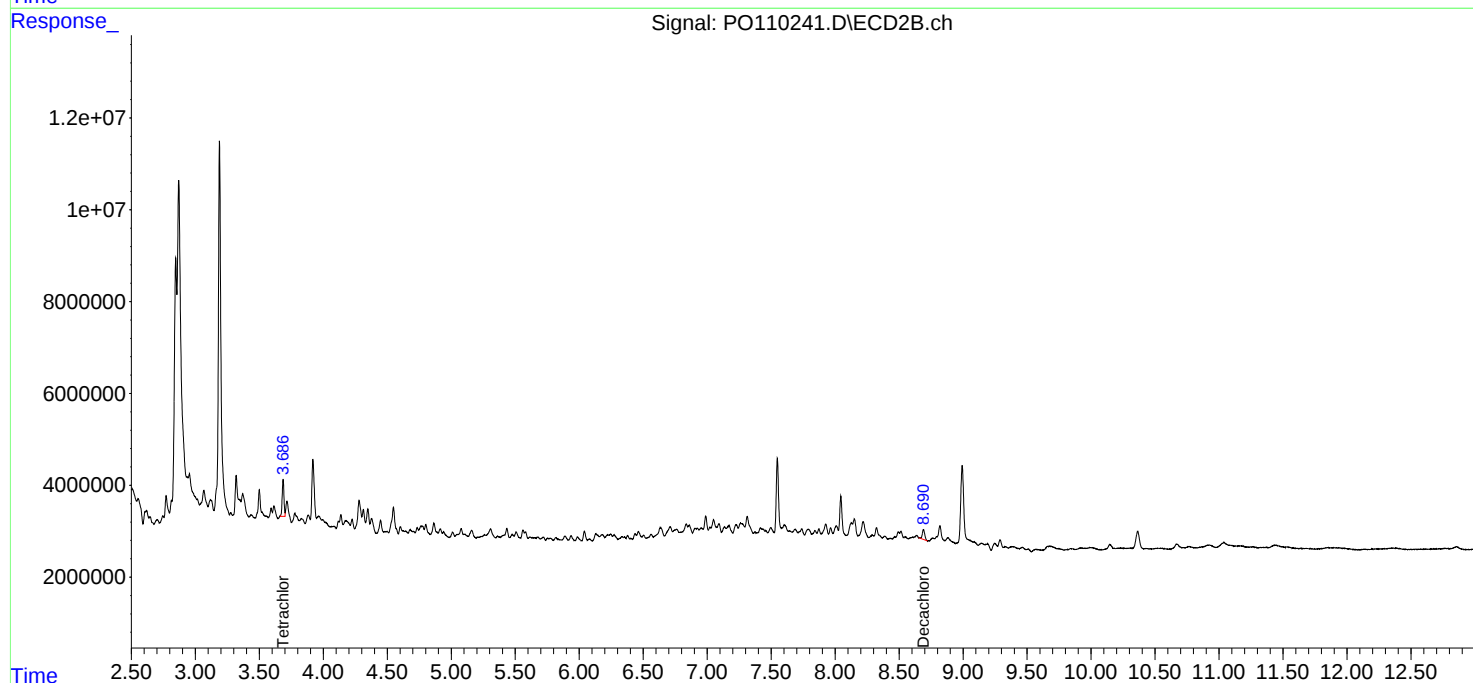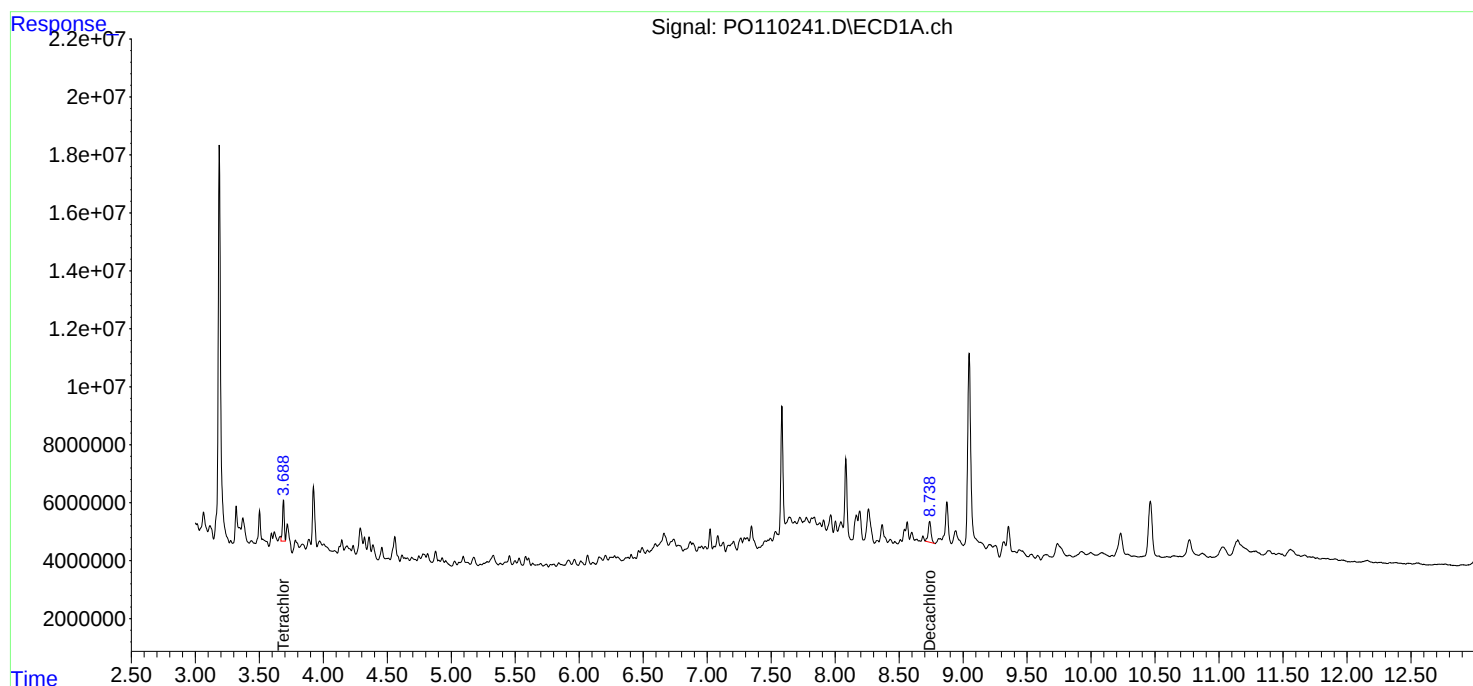

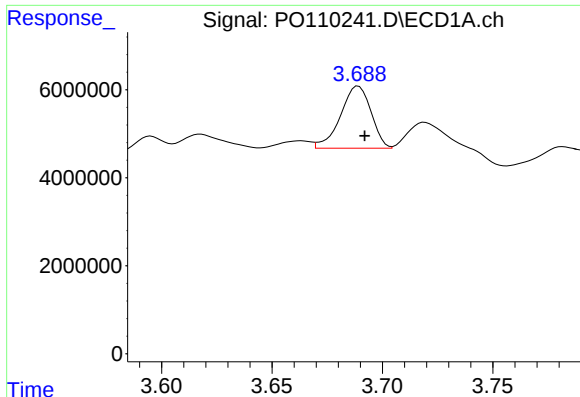


#1 Tetrachloro-m-xylene

R.T.: 3.688 min
Delta R.T.: -0.004 min
Response: 13511611
Conc: 1.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
GAS-CAM-03


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/07/2025
Supervised By :mohammad ahmed 04/09/2025

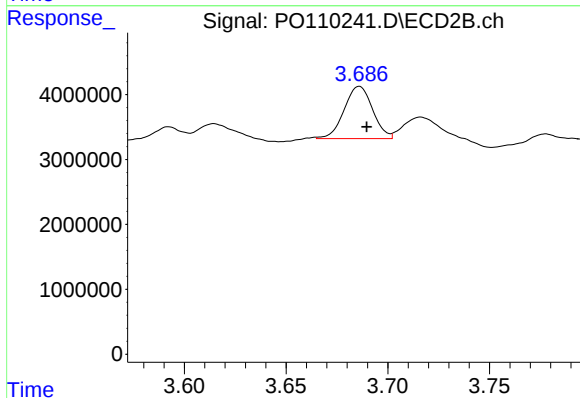


#1 Tetrachloro-m-xylene

R.T.: 3.686 min
Delta R.T.: -0.004 min
Response: 7900053
Conc: 1.51 ng/ml m

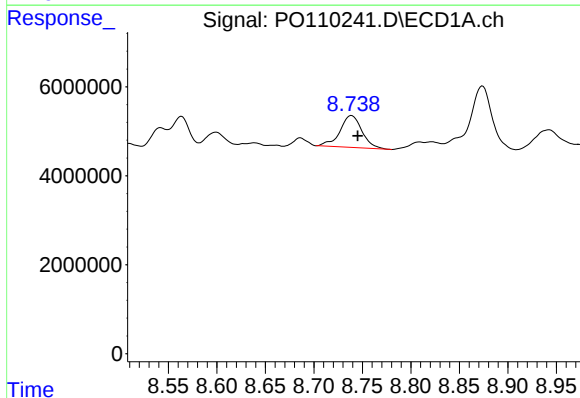

#2 Decachlorobiphenyl

R.T.: 8.739 min
Delta R.T.: -0.007 min
Response: 11370282
Conc: 1.48 ng/ml

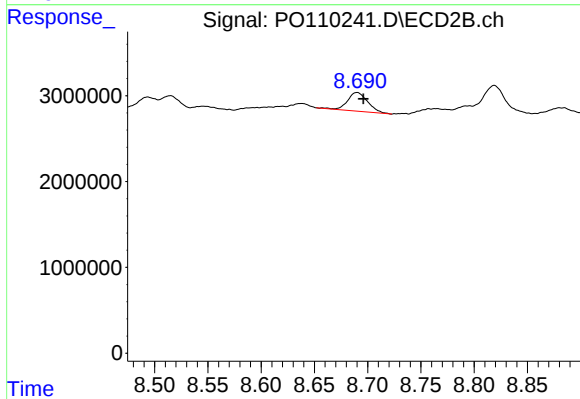

#2 Decachlorobiphenyl

R.T.: 8.690 min
Delta R.T.: -0.006 min
Response: 2885909
Conc: 1.19 ng/ml