

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040522\
 Data File : P0085901.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Apr 2022 16:03
 Operator : YP\AJ
 Sample : N2250-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 040122TB03-PCB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 02:43:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 30 16:55:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.489	3.587	3862112	953874	19.819	20.169
2) SA Decachlor...	10.391	8.602	3583059	779810	27.923	22.210

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040522\
Data File : P0085901.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Apr 2022 16:03
Operator : YP\AJ
Sample : N2250-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
040122TB03-PCB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 02:43:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 30 16:55:12 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

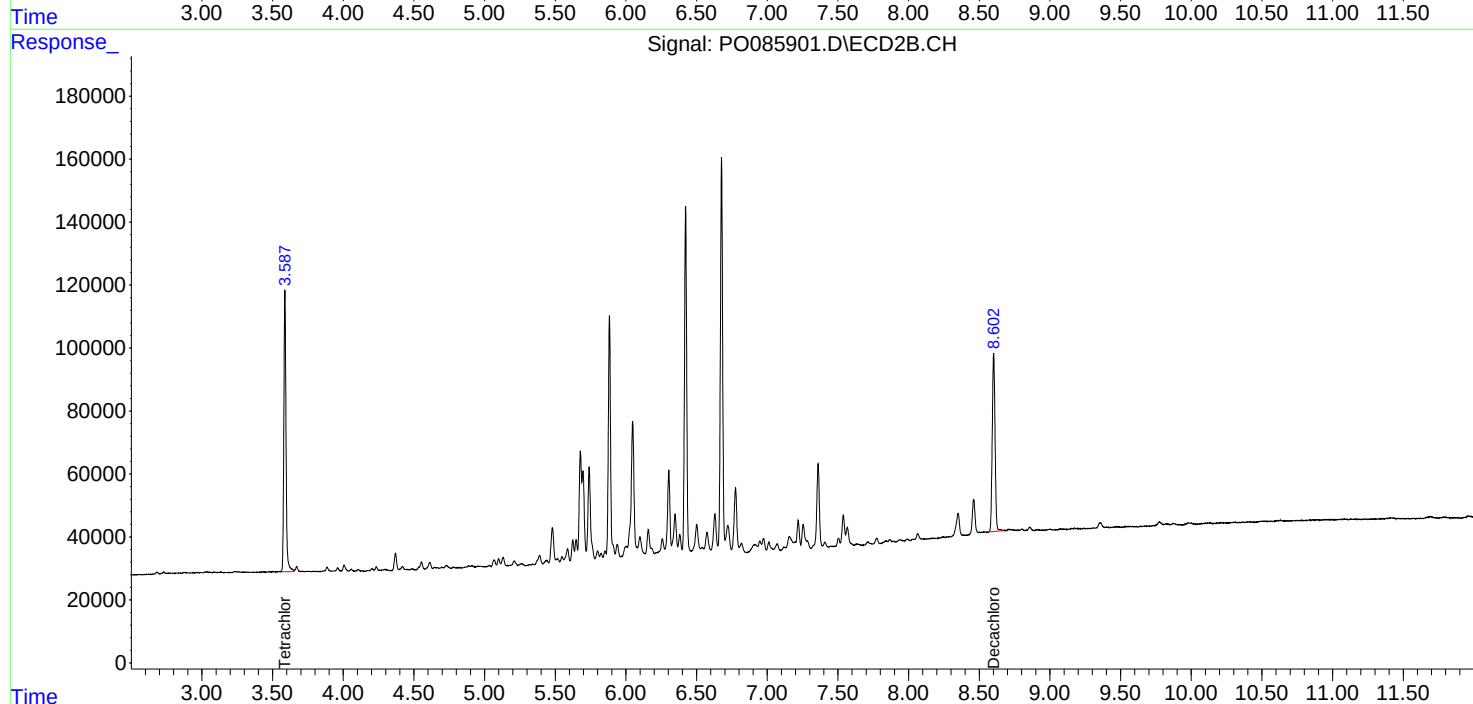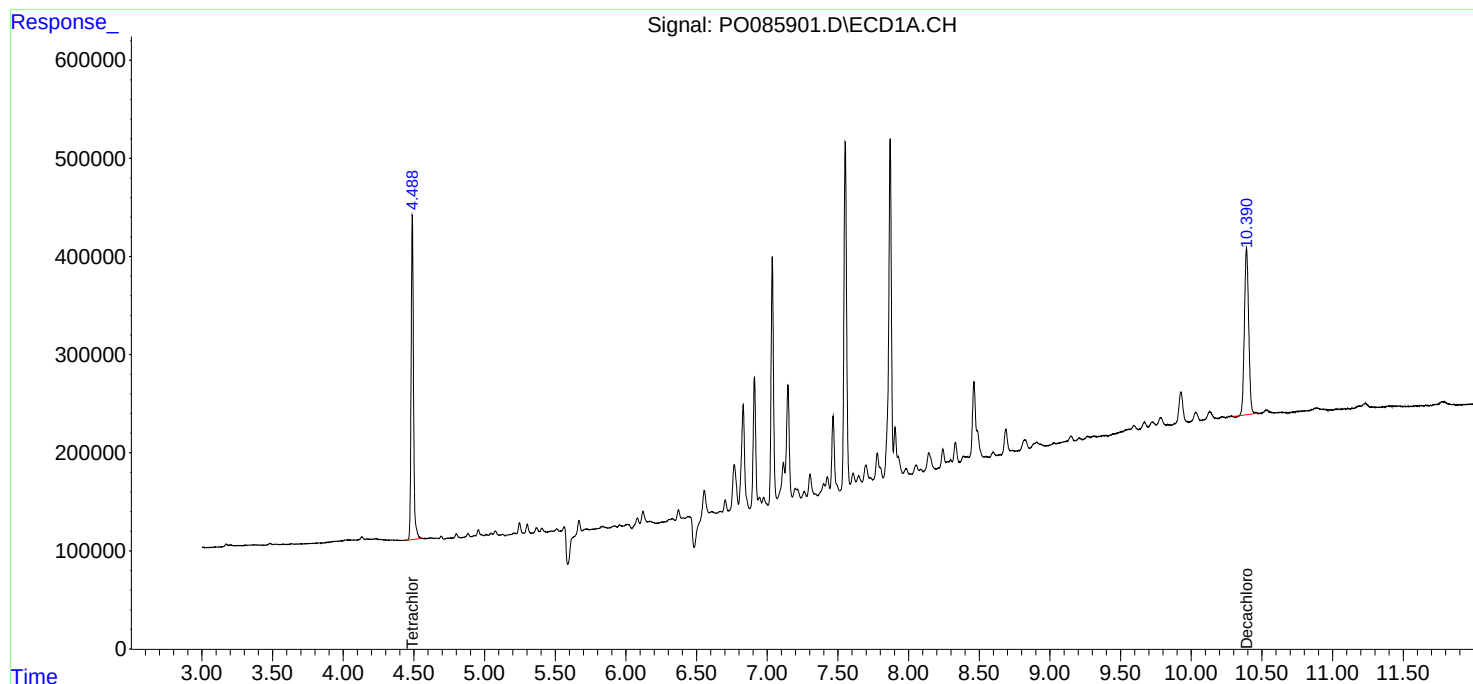


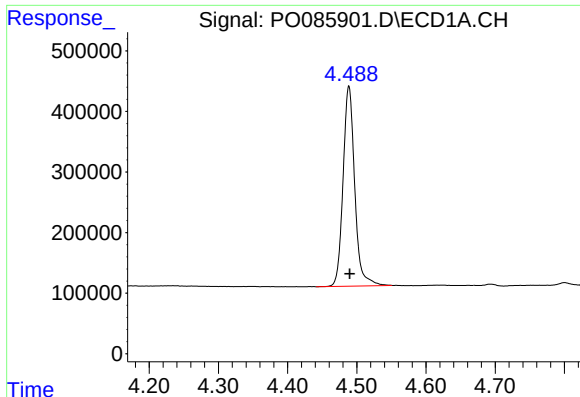

#1 Tetrachloro-m-xylene


R.T.: 4.489 min
Delta R.T.: -0.001 min
Response: 3862112
Conc: 19.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
040122TB03-PCB

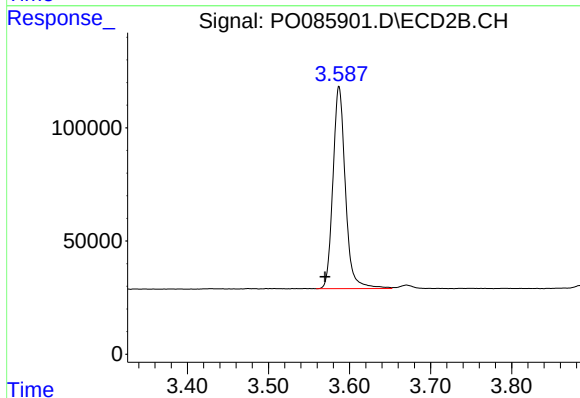


#1 Tetrachloro-m-xylene

R.T.: 3.587 min
Delta R.T.: 0.017 min
Response: 953874
Conc: 20.17 ng/ml

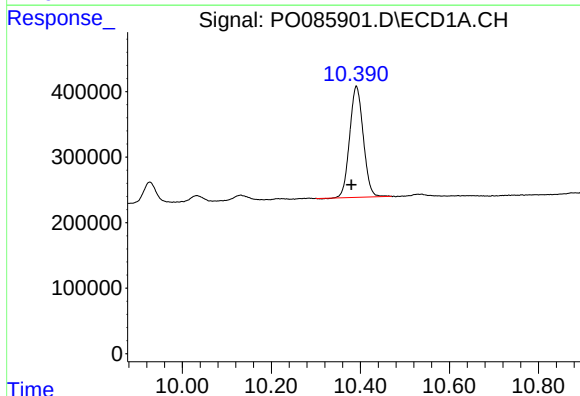

#2 Decachlorobiphenyl

R.T.: 10.391 min
Delta R.T.: 0.011 min
Response: 3583059
Conc: 27.92 ng/ml

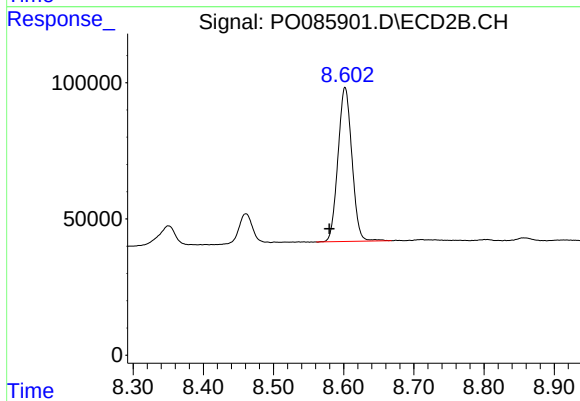

#2 Decachlorobiphenyl

R.T.: 8.602 min
Delta R.T.: 0.022 min
Response: 779810
Conc: 22.21 ng/ml