

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040522\
 Data File : P0085902.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Apr 2022 16:19
 Operator : YP\AJ
 Sample : N2250-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 040122TB02-PCB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 02:43:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 30 16:55:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.489	3.588	3657300	935792	18.768	19.786
2) SA Decachlor...	10.390	8.601	3031297	740525	23.623	21.091

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040522\
Data File : PO085902.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Apr 2022 16:19
Operator : YP\AJ
Sample : N2250-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
040122TB02-PCB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 02:43:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 30 16:55:12 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

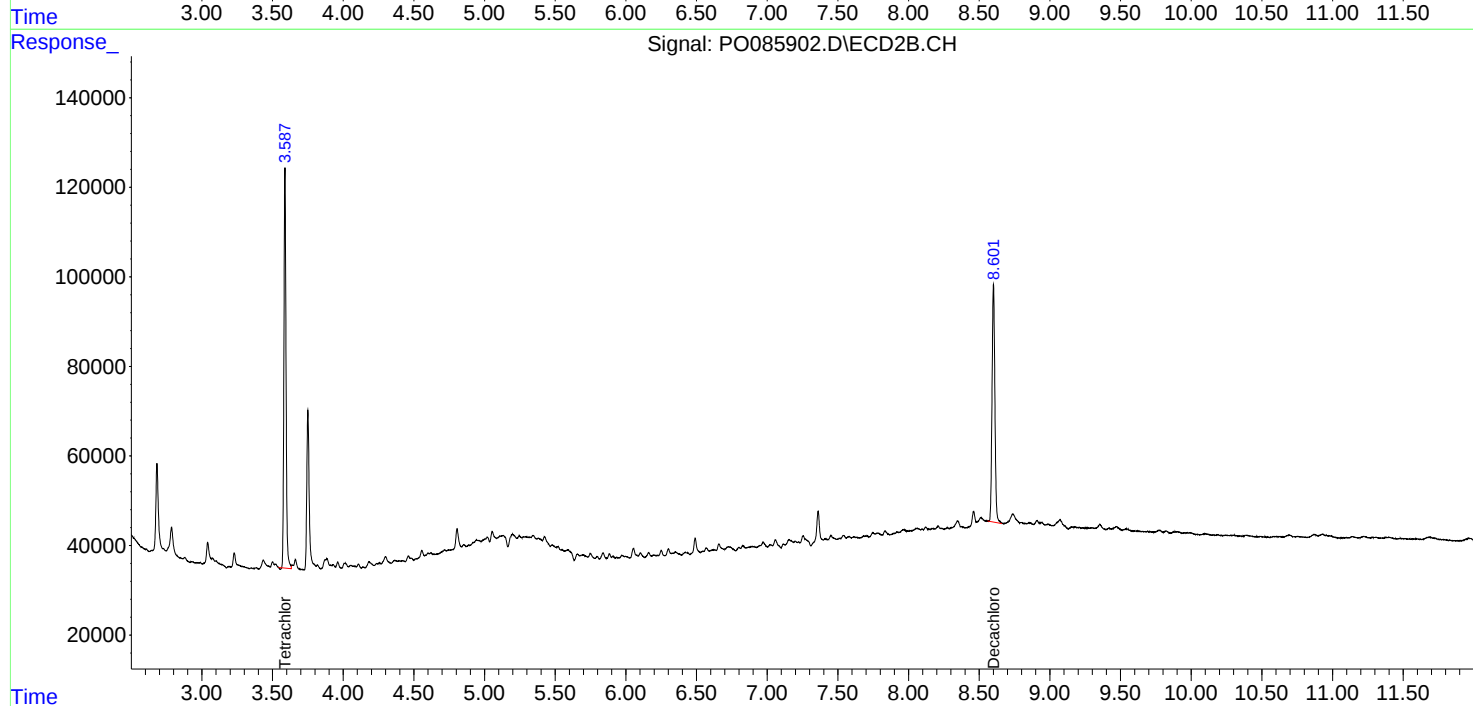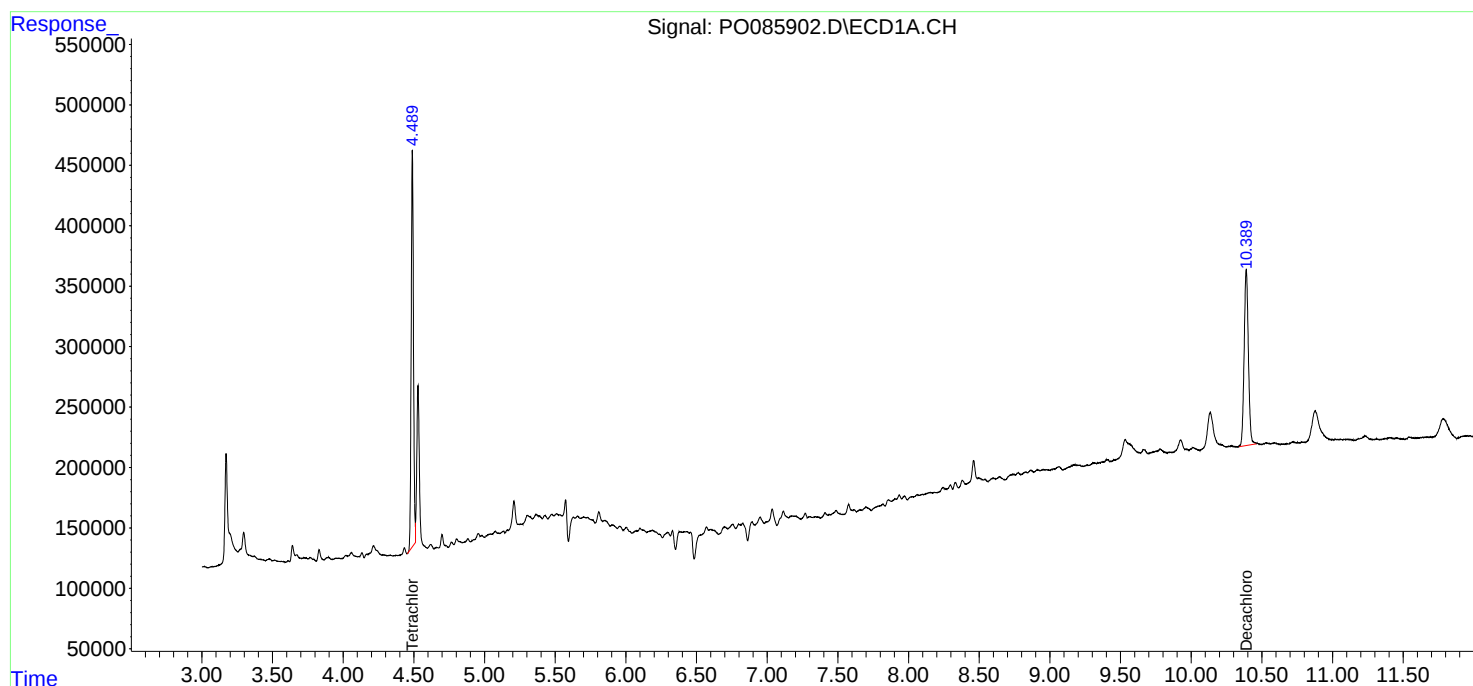


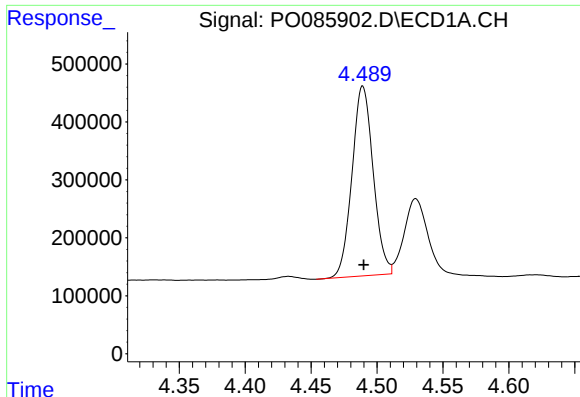

#1 Tetrachloro-m-xylene


R.T.: 4.489 min
Delta R.T.: 0.000 min
Response: 3657300
Conc: 18.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
040122TB02-PCB

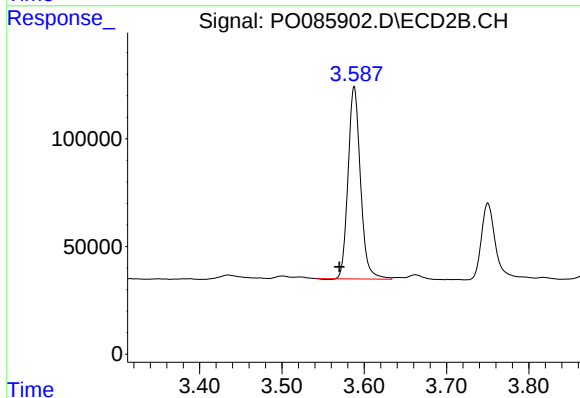


#1 Tetrachloro-m-xylene

R.T.: 3.588 min
Delta R.T.: 0.018 min
Response: 935792
Conc: 19.79 ng/ml

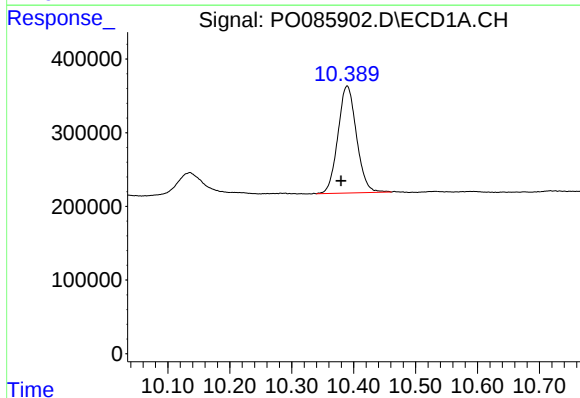

#2 Decachlorobiphenyl

R.T.: 10.390 min
Delta R.T.: 0.009 min
Response: 3031297
Conc: 23.62 ng/ml

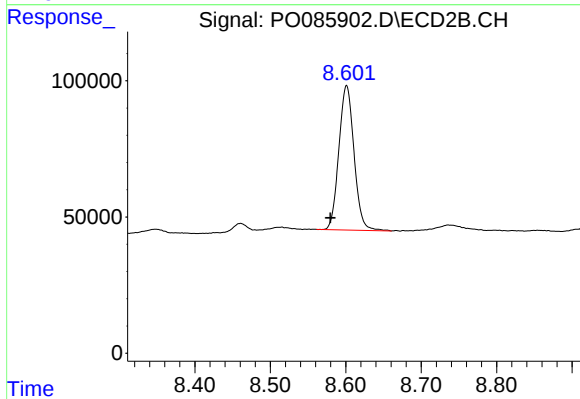

#2 Decachlorobiphenyl

R.T.: 8.601 min
Delta R.T.: 0.021 min
Response: 740525
Conc: 21.09 ng/ml