

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040522\
 Data File : P0085907.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Apr 2022 17:38
 Operator : YP\AJ
 Sample : N2234-03 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SOM-2022-11A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/06/2022
 Supervised By :mohammad ahmed 04/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 02:45:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 30 16:55:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.490	3.587	358665	105494	1.841	2.231
2) SA Decachlor...	10.395	8.600	251392	52933	1.959	1.508m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040522\
Data File : P0085907.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Apr 2022 17:38
Operator : YP\AJ
Sample : N2234-03 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SOM-2022-11A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/06/2022
Supervised By :mohammad ahmed 04/06/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 02:45:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 30 16:55:12 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

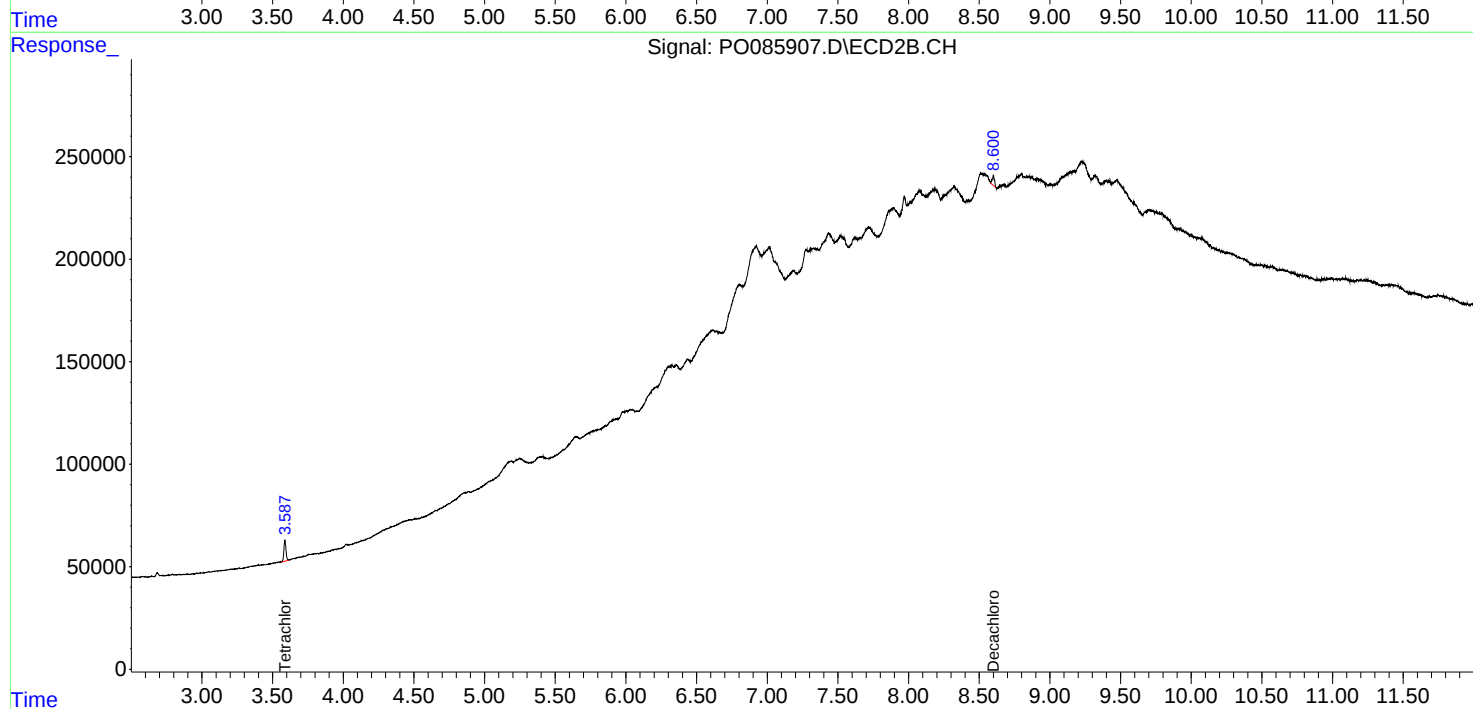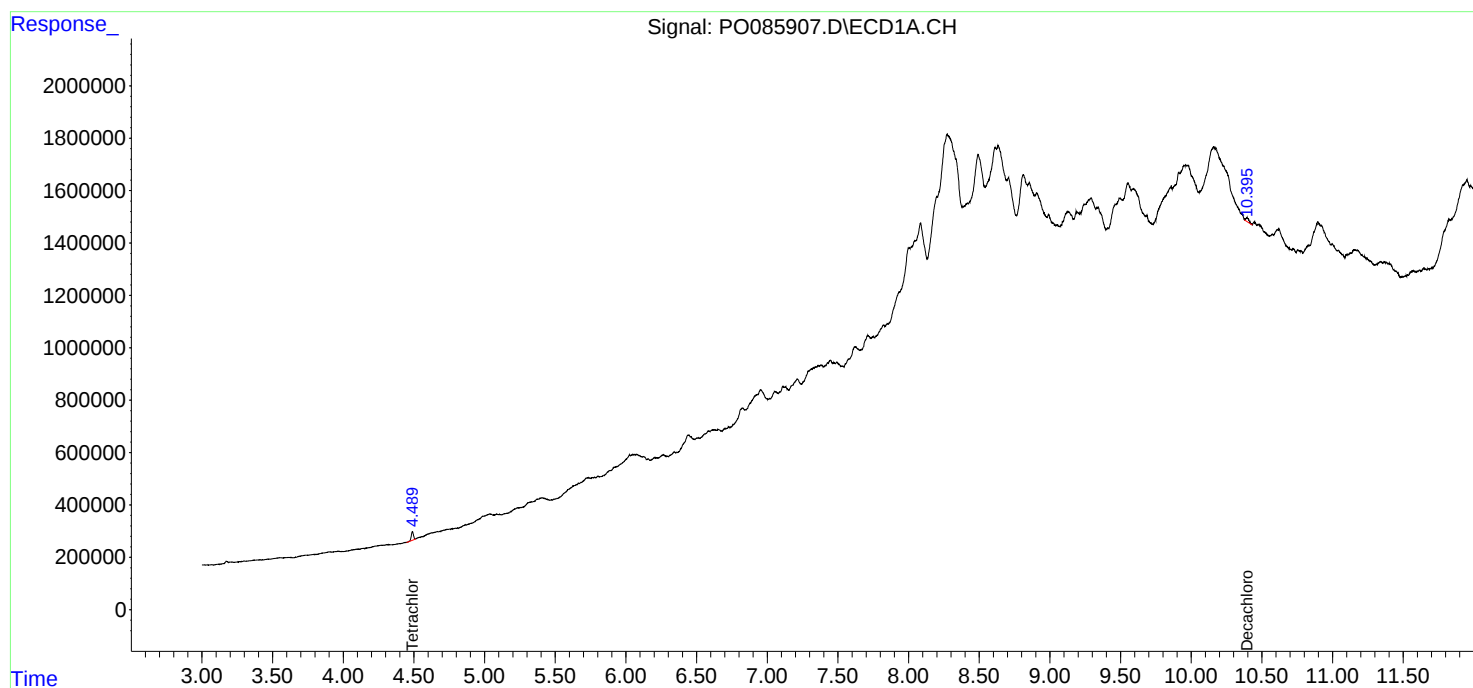

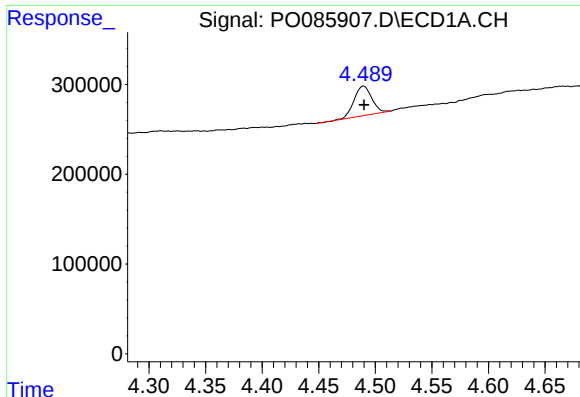


#1 Tetrachloro-m-xylene

R.T.: 4.490 min
Delta R.T.: 0.000 min
Response: 358665
Conc: 1.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
SOM-2022-11A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/06/2022
Supervised By :mohammad ahmed 04/06/2022

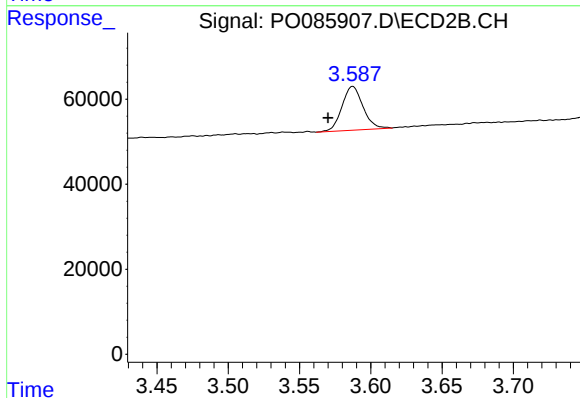


#1 Tetrachloro-m-xylene

R.T.: 3.587 min
Delta R.T.: 0.017 min
Response: 105494
Conc: 2.23 ng/ml

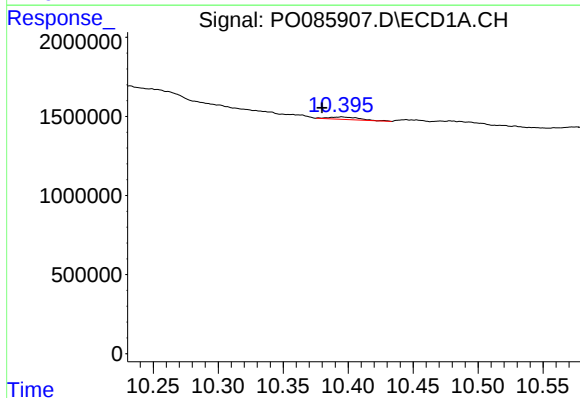

#2 Decachlorobiphenyl

R.T.: 10.395 min
Delta R.T.: 0.015 min
Response: 251392
Conc: 1.96 ng/ml

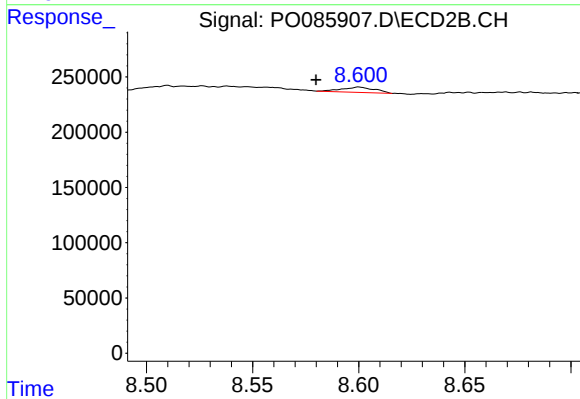

#2 Decachlorobiphenyl

R.T.: 8.600 min
Delta R.T.: 0.020 min
Response: 52933
Conc: 1.51 ng/ml m