

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040522\
 Data File : P0085922.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Apr 2022 23:36
 Operator : YP\AJ
 Sample : N2236-04
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 17140

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/06/2022
 Supervised By :mohammad ahmed 04/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 02:55:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 30 16:55:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.488	3.587	581657	213721	2.985	4.519m#
2) SA Decachlor...	10.393	8.601	448524	144333	3.495	4.111

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040522\
Data File : PO085922.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Apr 2022 23:36
Operator : YP\AJ
Sample : N2236-04
Misc :
ALS Vial : 25 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
17140


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/06/2022
Supervised By :mohammad ahmed 04/06/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 02:55:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 30 16:55:12 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

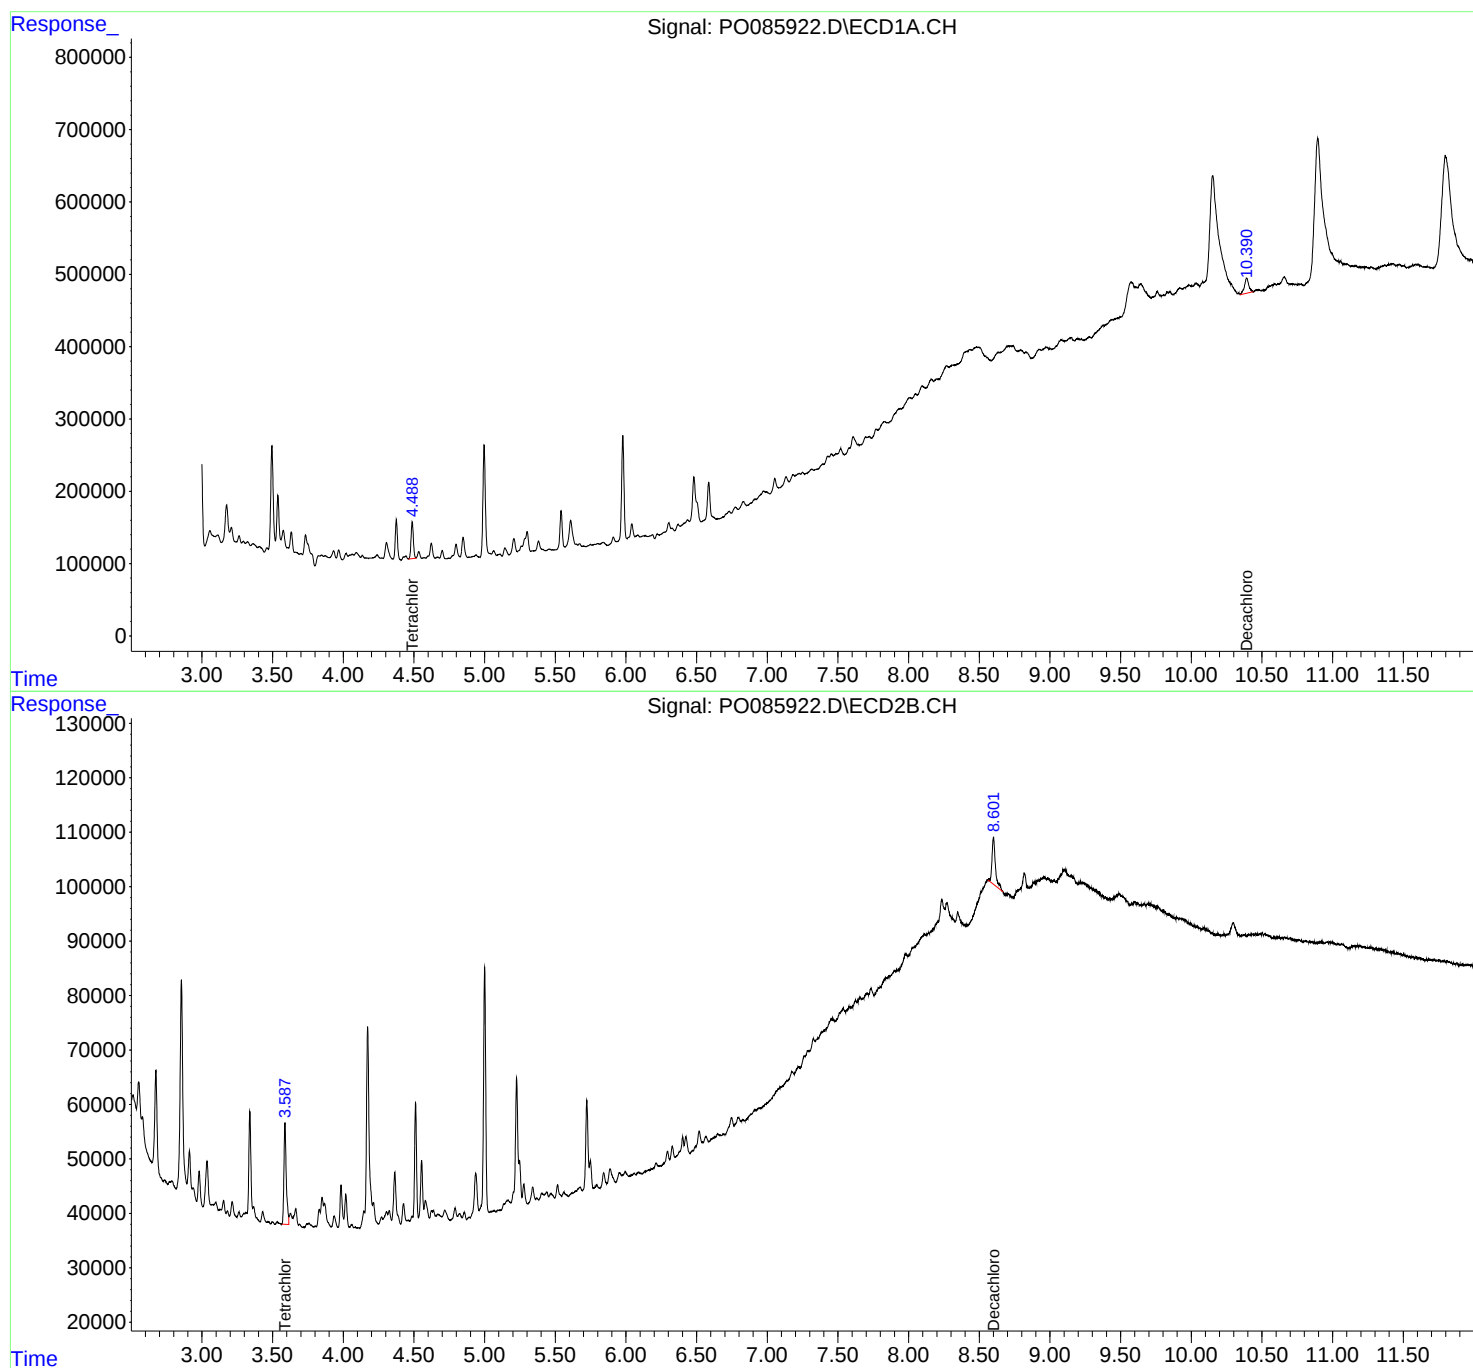

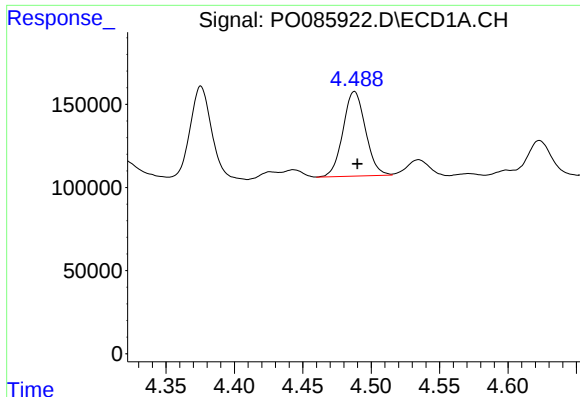


#1 Tetrachloro-m-xylene

R.T.: 4.488 min
Delta R.T.: -0.002 min
Response: 581657
Conc: 2.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
17140


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/06/2022
Supervised By :mohammad ahmed 04/06/2022

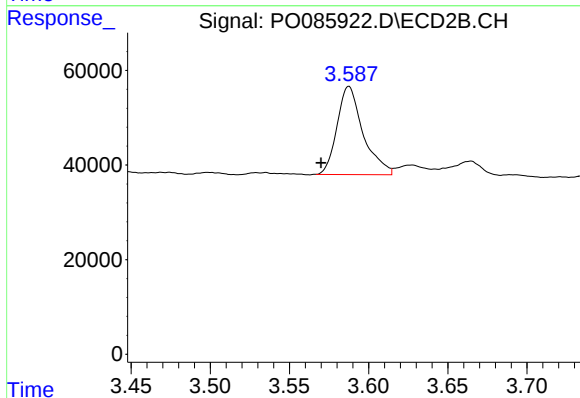


#1 Tetrachloro-m-xylene

R.T.: 3.587 min
Delta R.T.: 0.017 min
Response: 213721
Conc: 4.52 ng/ml m

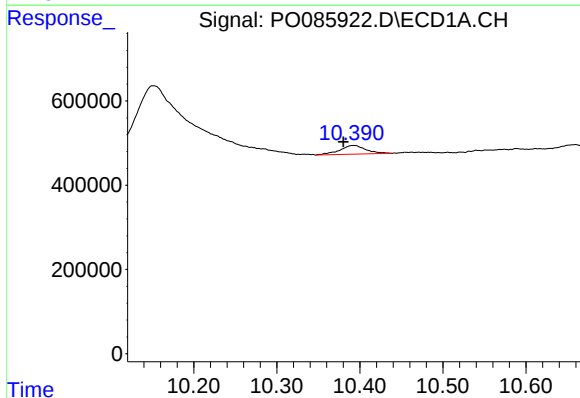

#2 Decachlorobiphenyl

R.T.: 10.393 min
Delta R.T.: 0.013 min
Response: 448524
Conc: 3.50 ng/ml

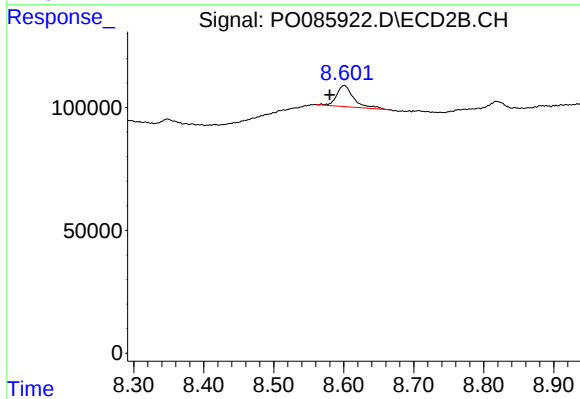

#2 Decachlorobiphenyl

R.T.: 8.601 min
Delta R.T.: 0.021 min
Response: 144333
Conc: 4.11 ng/ml