

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040522\
 Data File : P0085930.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Apr 2022 3:42
 Operator : YP\AJ
 Sample : N2253-05
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 41044

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/06/2022
 Supervised By :mohammad ahmed 04/06/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 06:09:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 30 16:55:12 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.489	3.587	1968376	682397	10.101	14.429m#
2) SA Decachlor...	10.377	8.604	36527	249571	0.285m	7.108m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040522\
Data File : P0085930.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Apr 2022 3:42
Operator : YP\AJ
Sample : N2253-05
Misc :
ALS Vial : 28 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
41044


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/06/2022
Supervised By :mohammad ahmed 04/06/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 06:09:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 30 16:55:12 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

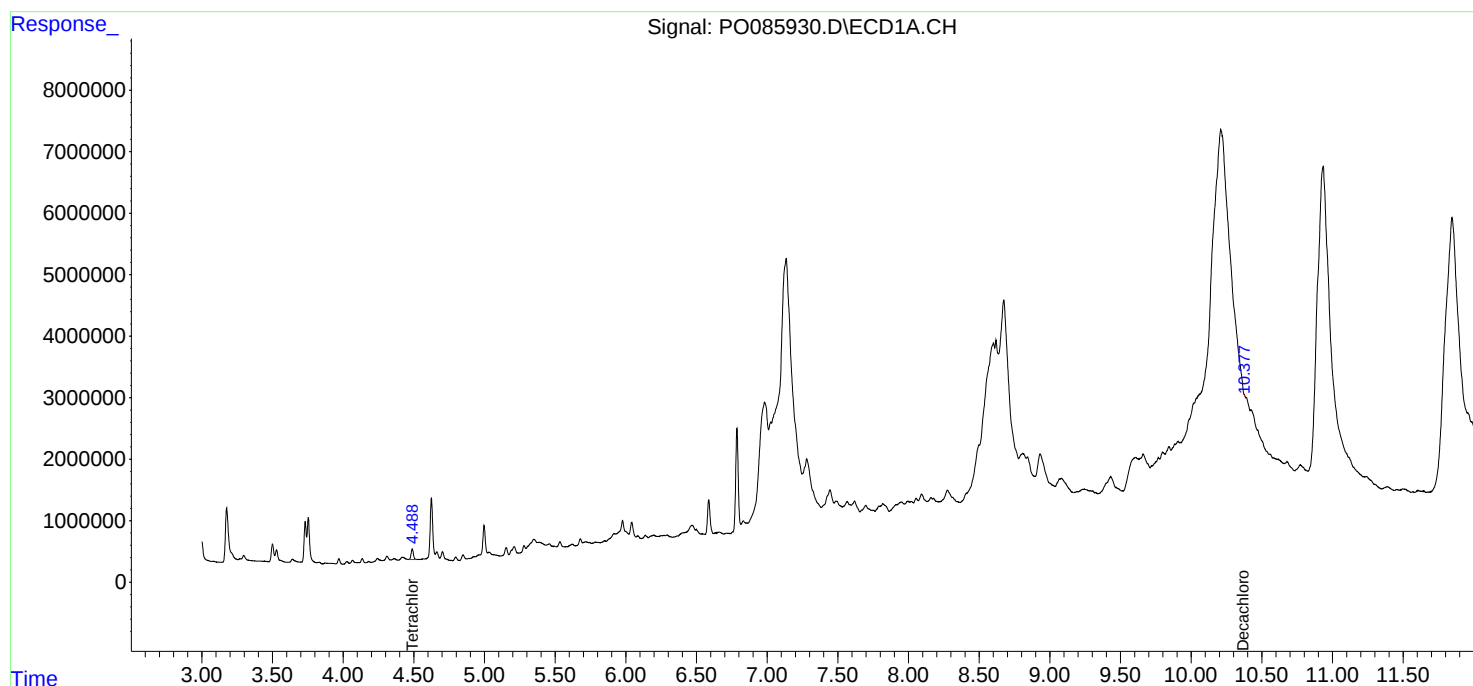

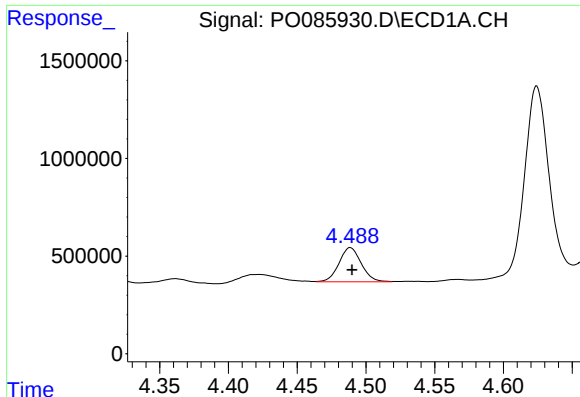


#1 Tetrachloro-m-xylene

R.T.: 4.489 min
Delta R.T.: -0.001 min
Response: 1968376
Conc: 10.10 ng/ml

Instrument :
ECD_O
ClientSampleId :
41044


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/06/2022
Supervised By :mohammad ahmed 04/06/2022

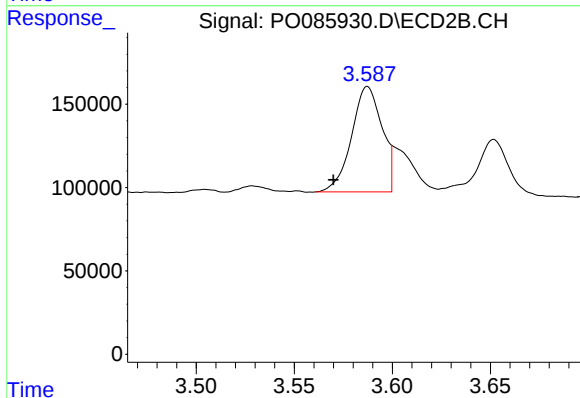


#1 Tetrachloro-m-xylene

R.T.: 3.587 min
Delta R.T.: 0.017 min
Response: 682397
Conc: 14.43 ng/ml m

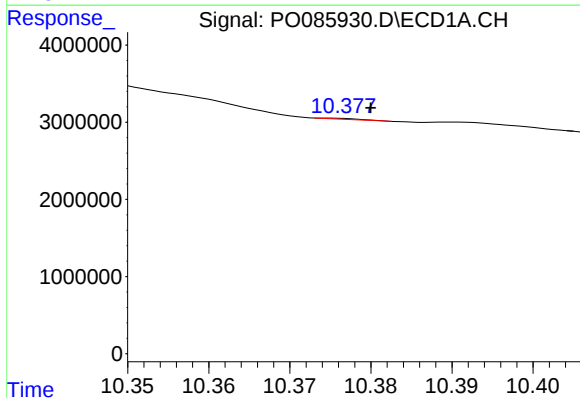

#2 Decachlorobiphenyl

R.T.: 10.377 min
Delta R.T.: -0.003 min
Response: 36527
Conc: 0.28 ng/ml m

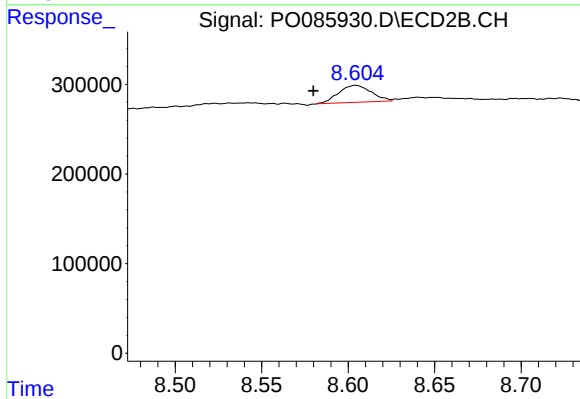

#2 Decachlorobiphenyl

R.T.: 8.604 min
Delta R.T.: 0.024 min
Response: 249571
Conc: 7.11 ng/ml m