

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040523\
 Data File : P0093822.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2023 12:37
 Operator : YP/AJ
 Sample : 02175-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AUD-1956

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/06/2023
 Supervised By :Ankita Jodhani 04/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 22:22:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.420	3.627	52325628	12775281	13.997	10.032m#
2) SA Decachlor...	10.243	8.646	21707597	7635722	9.704	7.637
Target Compounds						
31) L7 AR-1260-1	7.212	6.194	108.8E6	40875440	745.531m	626.816m
32) L7 AR-1260-2	7.473	6.383	125.3E6	48341956	782.722	665.647m
33) L7 AR-1260-3	7.836	6.537	84235081	36743617	634.406	506.297m
34) L7 AR-1260-4	8.065	7.010	119.9E6	25105375	870.776	452.082 #
35) L7 AR-1260-5	8.389	7.253	196.3E6	71091031	901.362	685.058

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040523\
Data File : PO093822.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2023 12:37
Operator : YP/AJ
Sample : 02175-02
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AUD-1956


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/06/2023
Supervised By :Ankita Jodhani 04/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 22:22:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

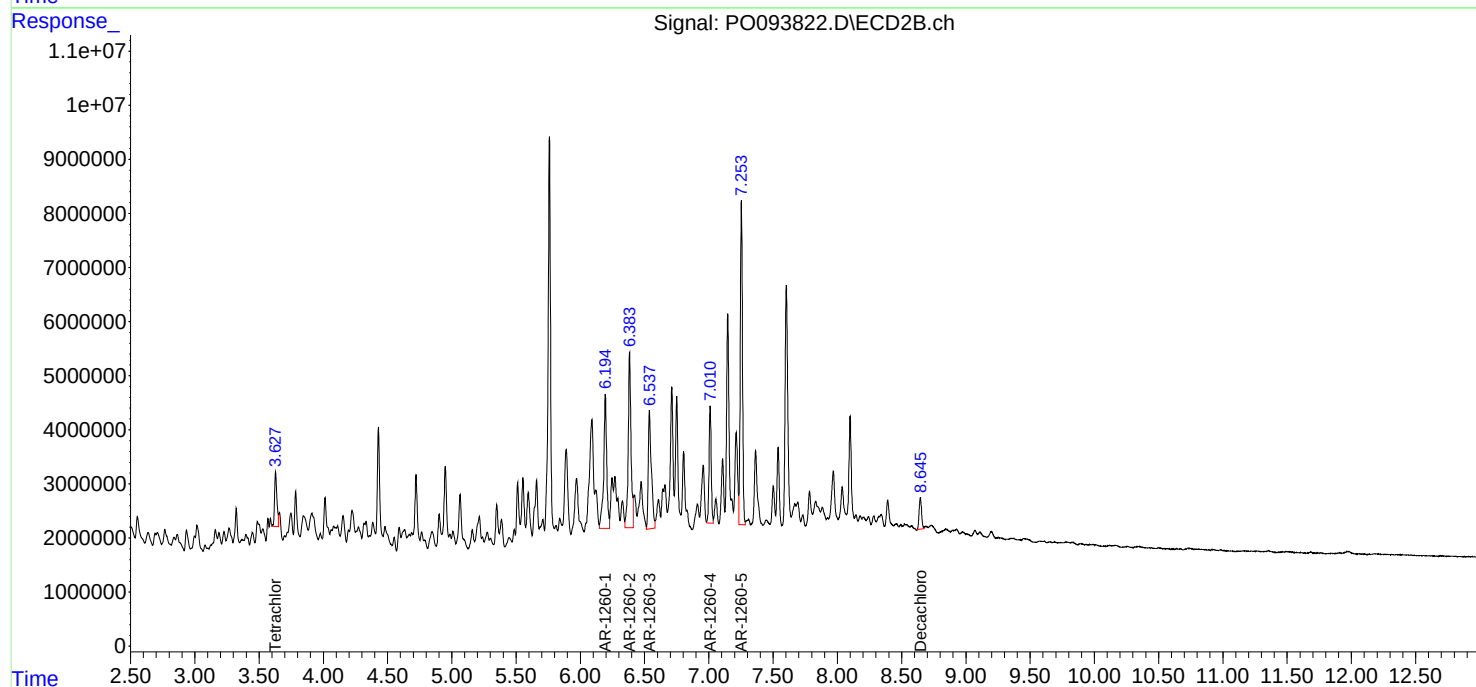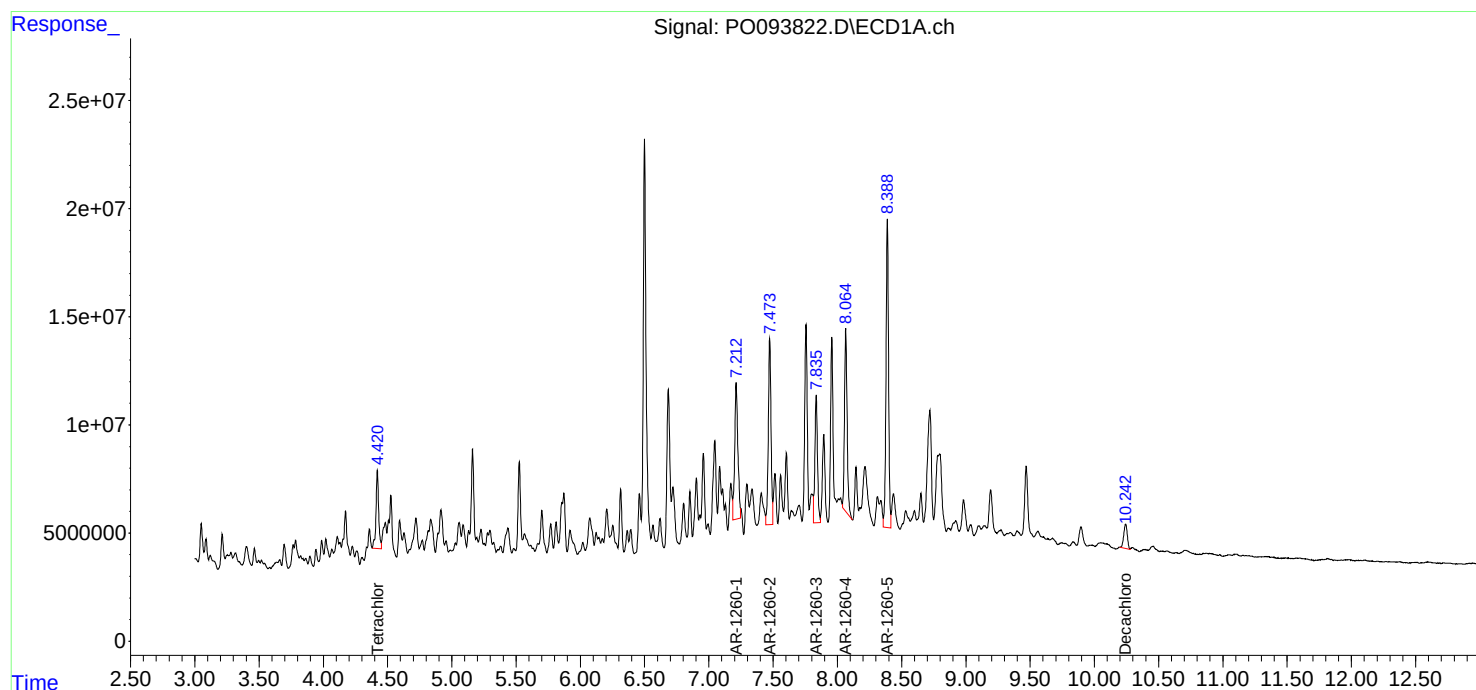

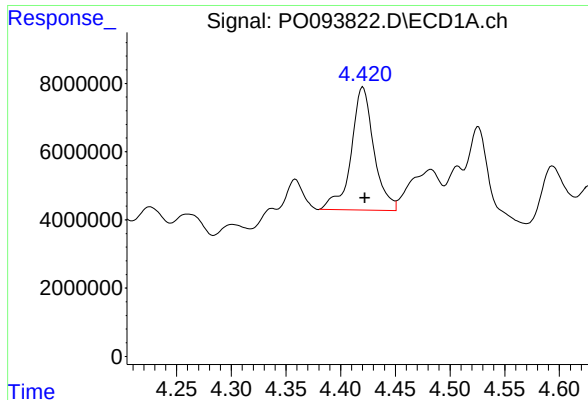


#1 Tetrachloro-m-xylene

R.T.: 4.420 min
Delta R.T.: -0.002 min
Response: 52325628
Conc: 14.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1956


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/06/2023
Supervised By :Ankita Jodhani 04/06/2023

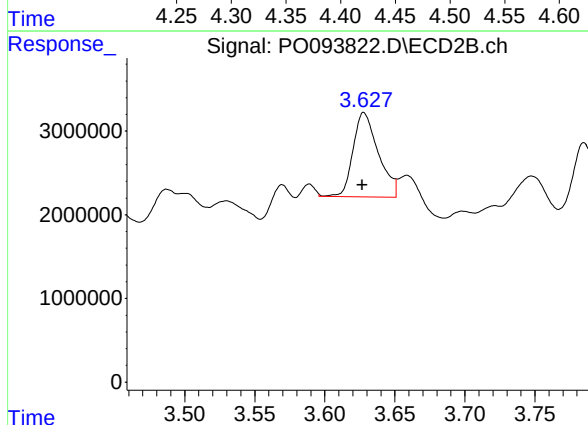


#1 Tetrachloro-m-xylene

R.T.: 3.627 min
Delta R.T.: 0.000 min
Response: 12775281
Conc: 10.03 ng/ml

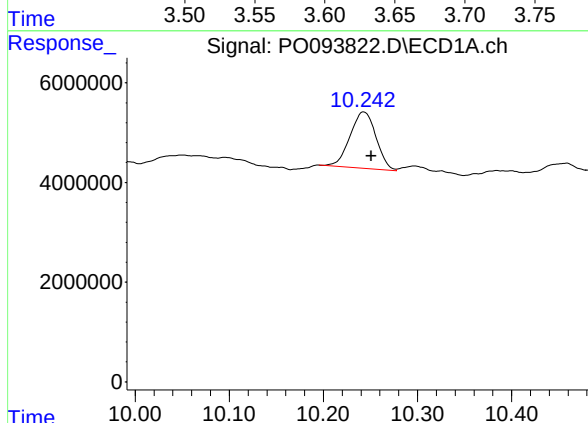


#2 Decachlorobiphenyl

R.T.: 10.243 min
Delta R.T.: -0.008 min
Response: 21707597
Conc: 9.70 ng/ml

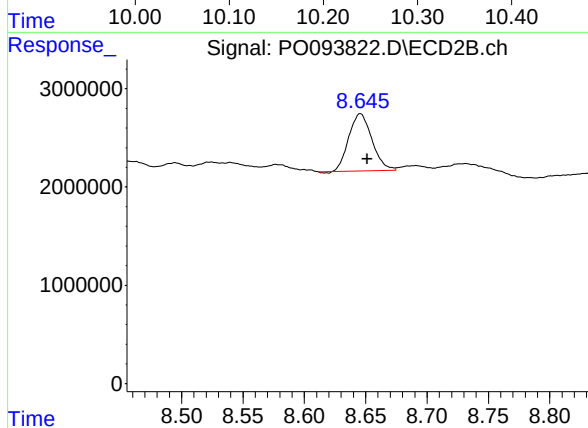

#2 Decachlorobiphenyl

R.T.: 8.646 min
Delta R.T.: -0.006 min
Response: 7635722
Conc: 7.64 ng/ml

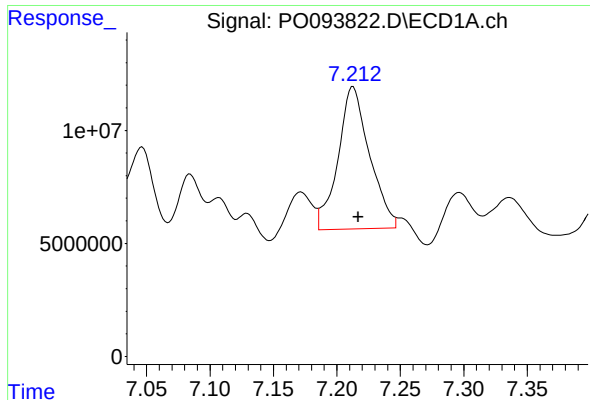


#31 AR-1260-1

R.T.: 7.212 min
Delta R.T.: -0.005 min
Response: 108822976
Conc: 745.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1956


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/06/2023
Supervised By :Ankita Jodhani 04/06/2023

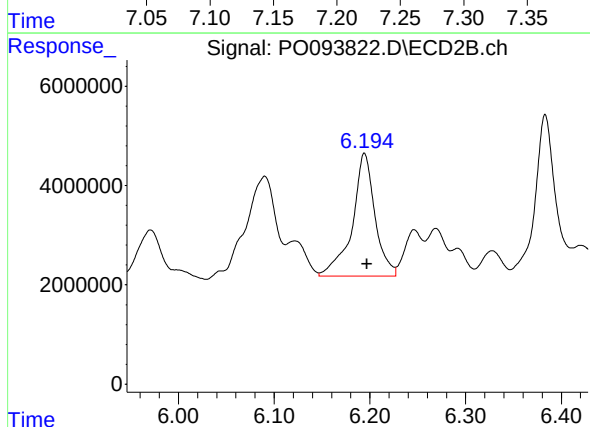


#31 AR-1260-1

R.T.: 6.194 min
Delta R.T.: -0.003 min
Response: 40875440
Conc: 626.82 ng/ml

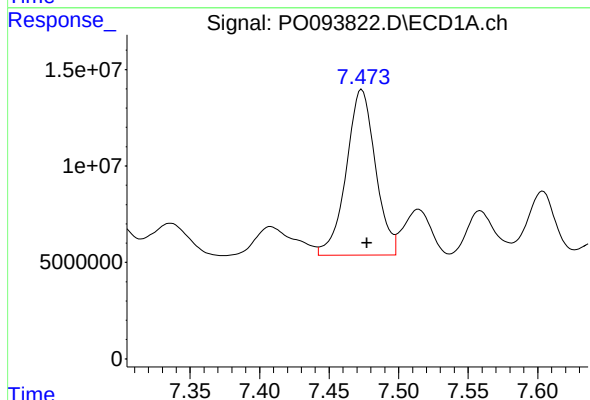


#32 AR-1260-2

R.T.: 7.473 min
Delta R.T.: -0.004 min
Response: 125277787
Conc: 782.72 ng/ml

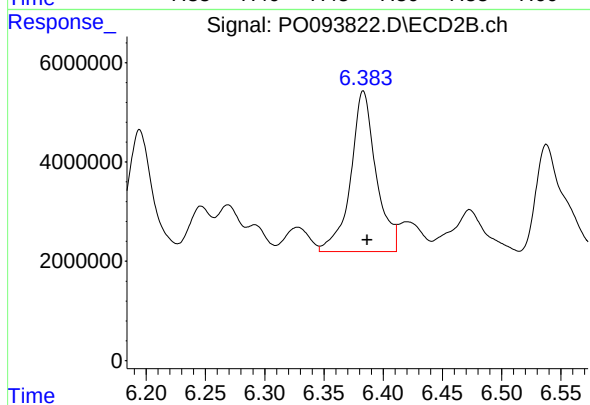

#32 AR-1260-2

R.T.: 6.383 min
Delta R.T.: -0.004 min
Response: 48341956
Conc: 665.65 ng/ml

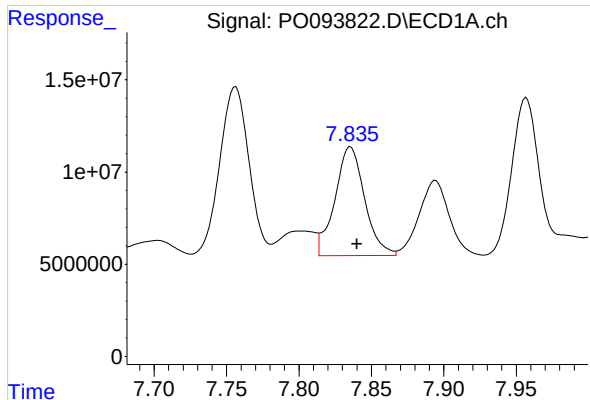


#33 AR-1260-3

R.T.: 7.836 min
Delta R.T.: -0.004 min
Response: 84235081
Conc: 634.41 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1956


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/06/2023
Supervised By :Ankita Jodhani 04/06/2023

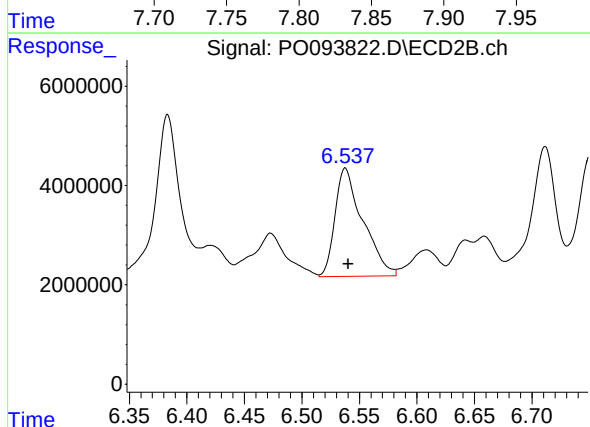


#33 AR-1260-3

R.T.: 6.537 min
Delta R.T.: -0.003 min
Response: 36743617
Conc: 506.30 ng/ml

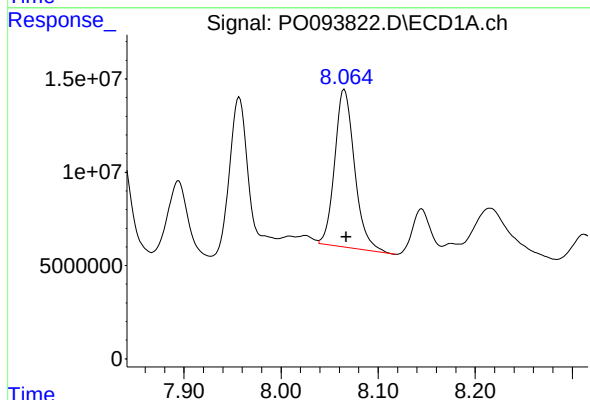


#34 AR-1260-4

R.T.: 8.065 min
Delta R.T.: -0.002 min
Response: 119943610
Conc: 870.78 ng/ml

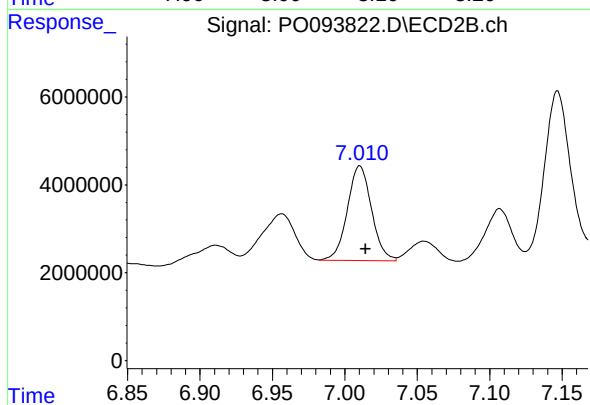

#34 AR-1260-4

R.T.: 7.010 min
Delta R.T.: -0.004 min
Response: 25105375
Conc: 452.08 ng/ml

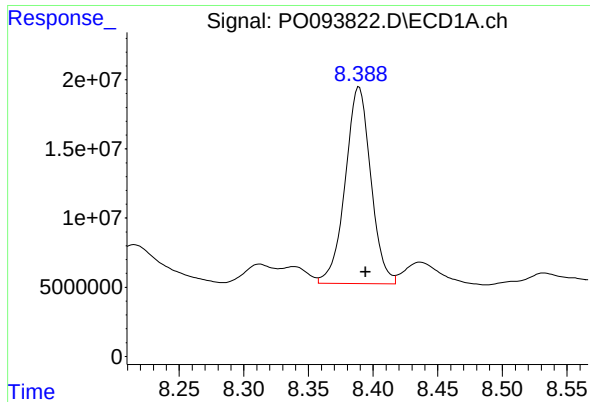


#35 AR-1260-5

R.T.: 8.389 min
Delta R.T.: -0.005 min
Response: 196307023
Conc: 901.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
AUD-1956

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/06/2023
Supervised By :Ankita Jodhani 04/06/2023

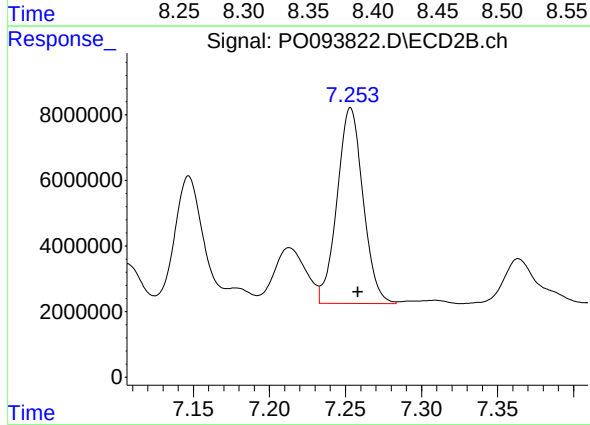

#35 AR-1260-5

R.T.: 7.253 min
Delta R.T.: -0.005 min
Response: 71091031
Conc: 685.06 ng/ml