

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040523\
 Data File : P0093833.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Apr 2023 16:00
 Operator : YP/AJ
 Sample : 02180-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 34132

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/06/2023
 Supervised By :Ankita Jodhani 04/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 05 22:32:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.420	3.625	72098822	21671696	19.287	17.019
2) SA Decachlor...	10.245	8.648	50976960	16487396	22.789m	16.491m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040523\
Data File : PO093833.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Apr 2023 16:00
Operator : YP/AJ
Sample : 02180-02
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
34132


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/06/2023
Supervised By :Ankita Jodhani 04/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 05 22:32:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

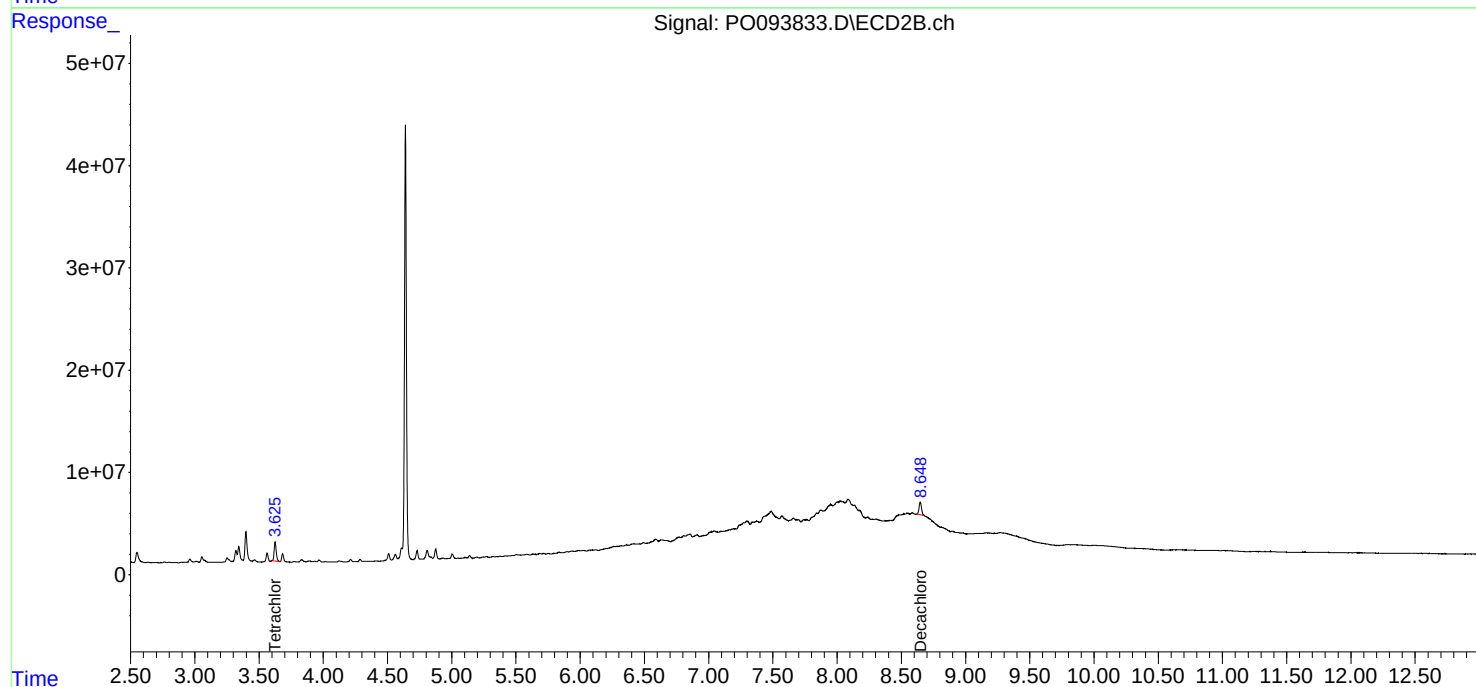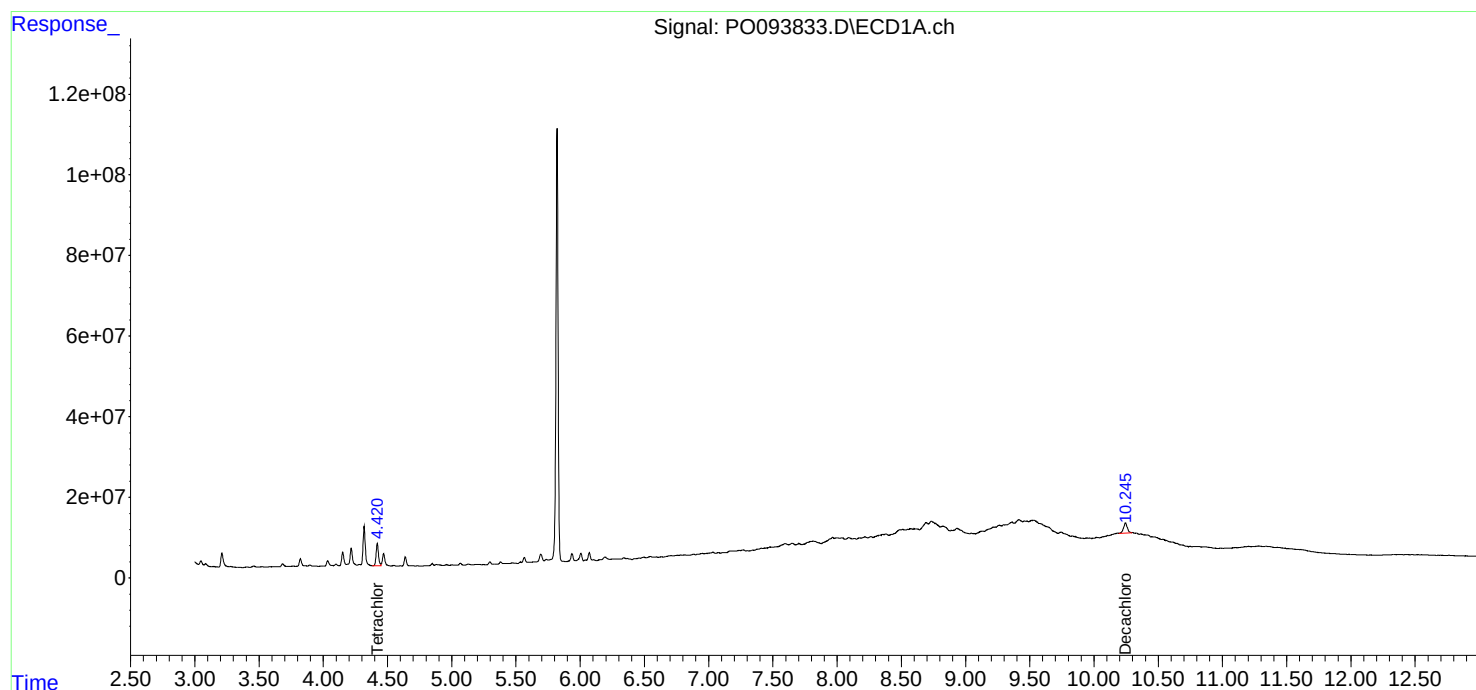

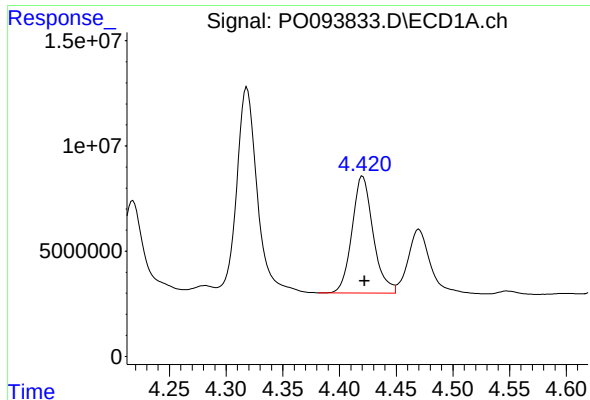

#1 Tetrachloro-m-xylene

R.T.: 4.420 min
Delta R.T.: -0.002 min
Response: 72098822
Conc: 19.29 ng/ml


Instrument :

ECD_O

ClientSampleId :
34132


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/06/2023
Supervised By :Ankita Jodhani 04/06/2023

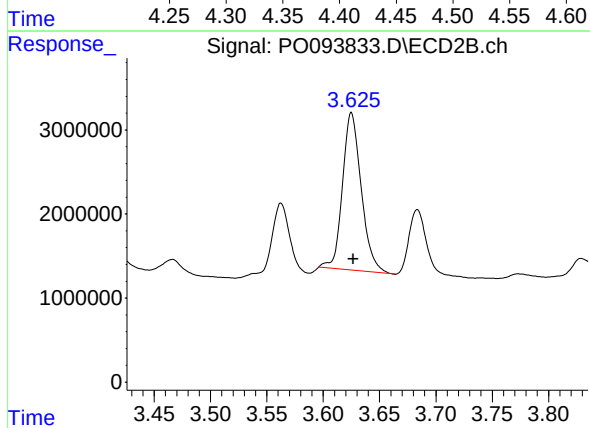


#1 Tetrachloro-m-xylene

R.T.: 3.625 min
Delta R.T.: -0.002 min
Response: 21671696
Conc: 17.02 ng/ml

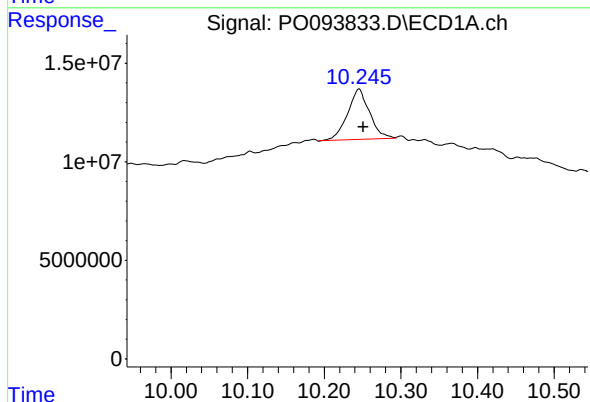

#2 Decachlorobiphenyl

R.T.: 10.245 min
Delta R.T.: -0.006 min
Response: 50976960
Conc: 22.79 ng/ml m

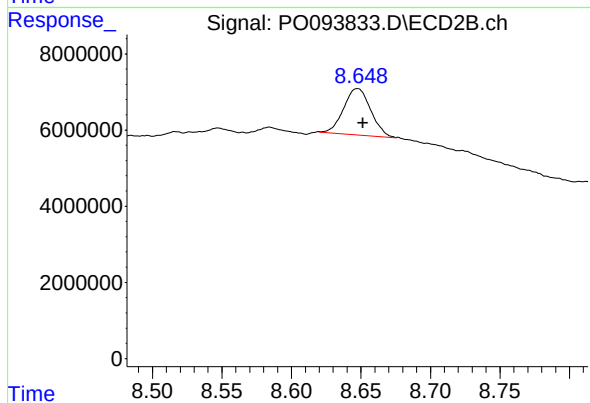

#2 Decachlorobiphenyl

R.T.: 8.648 min
Delta R.T.: -0.003 min
Response: 16487396
Conc: 16.49 ng/ml m