

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040621\
 Data File : P0076838.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Apr 2021 21:49
 Operator : DD\AJ
 Sample : M1933-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 02:23:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.898	3.895	2005144	1040597	21.558	20.736
2)	SA Decachlor...	10.872	9.140	1792009	813758	19.348	16.769
Target Compounds							
7)	L1 AR-1016-5	0.000	5.628	0	29800	N.D.	22.123 #
8)	L2 AR-1221-1	5.162	0.000	86048	0	95.105	N.D. #
15)	L3 AR-1232-5	0.000	5.628	0	29800	N.D.	60.002 #
24)	L5 AR-1248-4	0.000	5.628	0	29800	N.D.	17.454 #
30)	L6 AR-1254-5	8.472	7.242	281284	29510	63.955	9.052 #
31)	L7 AR-1260-1	0.000	6.724	0	21721	N.D.	8.313 #
32)	L7 AR-1260-2	0.000	6.930	0	27171	N.D.	8.605 #
36)	L8 AR-1262-1	0.000	7.242	0	29510	N.D.	16.671 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040621\
Data File : P0076838.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Apr 2021 21:49
Operator : DD\AJ
Sample : M1933-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 02:23:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

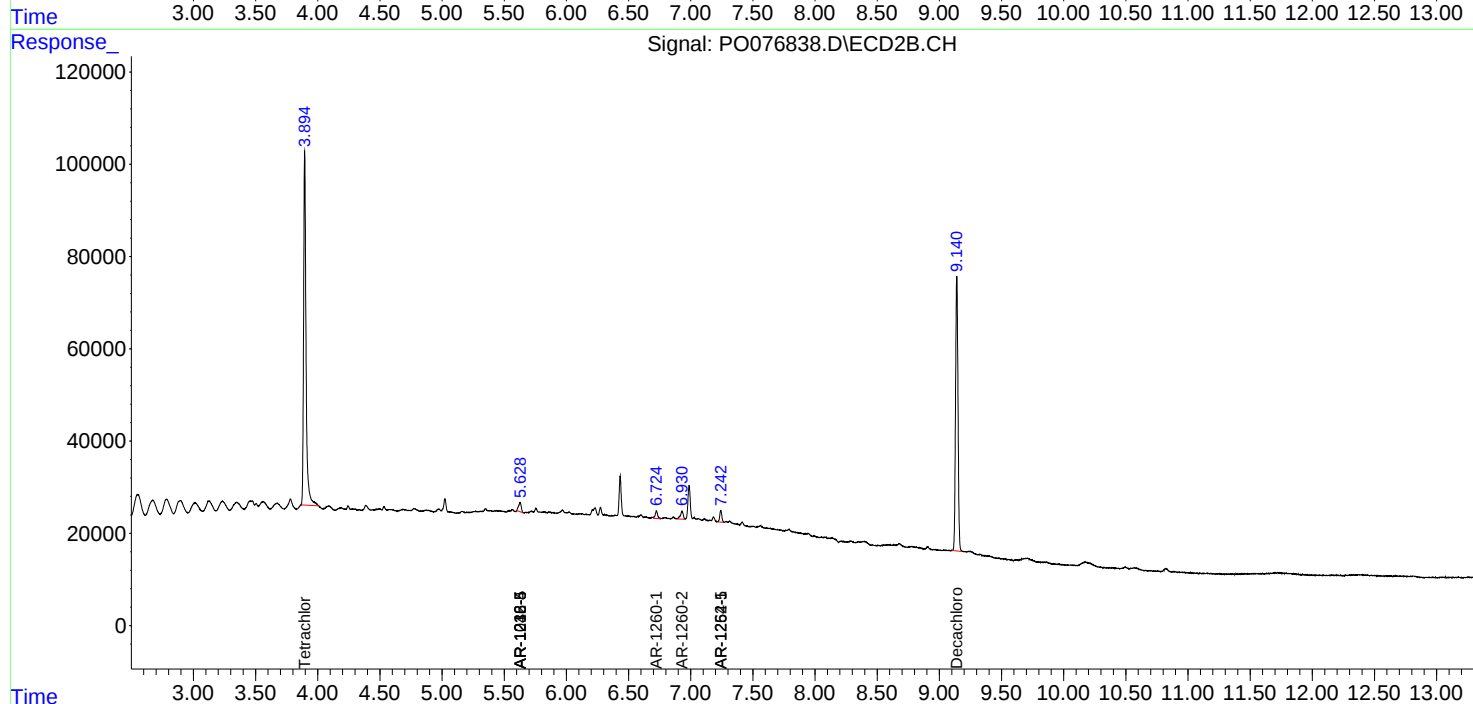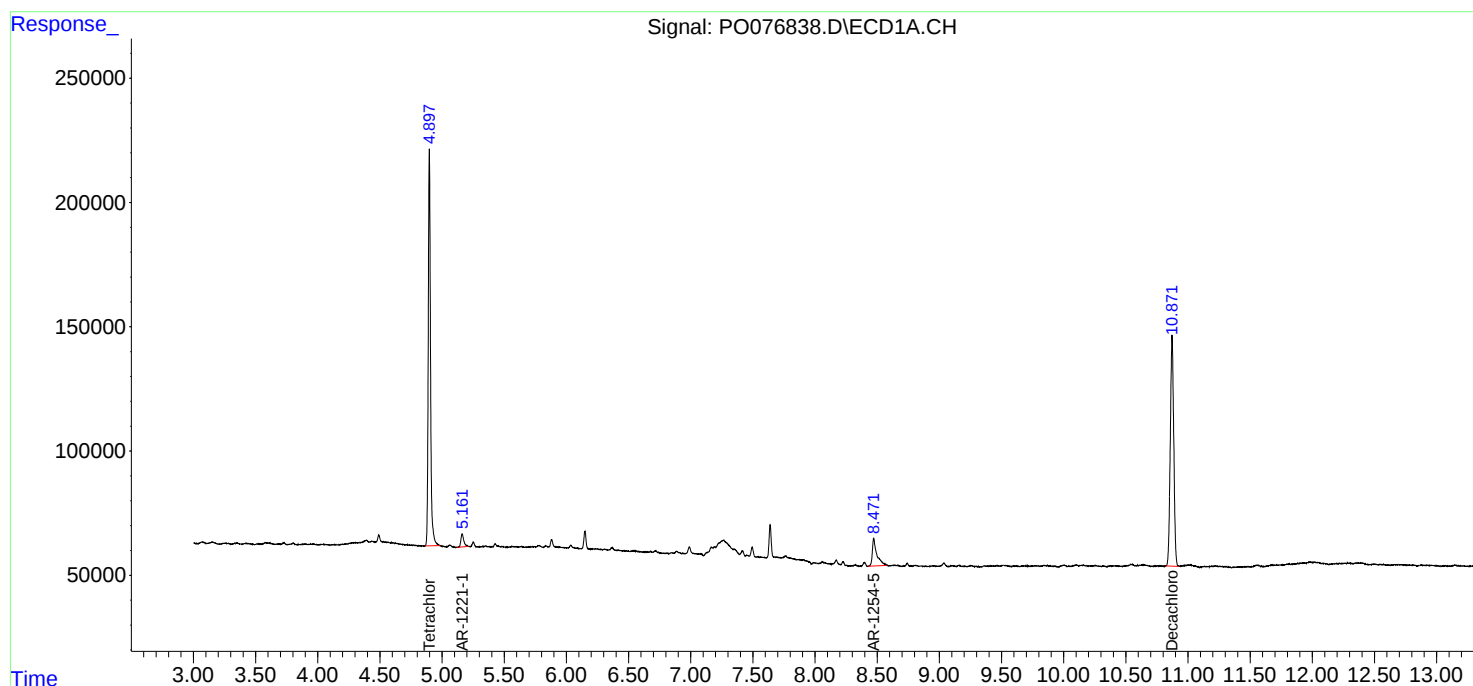


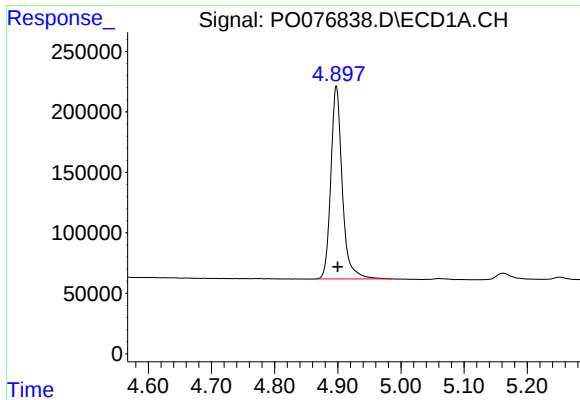

#1 Tetrachloro-m-xylene


R.T.: 4.898 min
Delta R.T.: -0.002 min
Response: 2005144
Conc: 21.56 ng/ml

Instrument :
ECD_O
ClientSampleId :

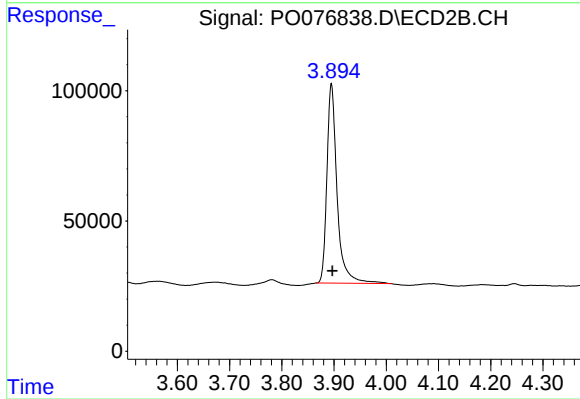


#1 Tetrachloro-m-xylene

R.T.: 3.895 min
Delta R.T.: -0.002 min
Response: 1040597
Conc: 20.74 ng/ml

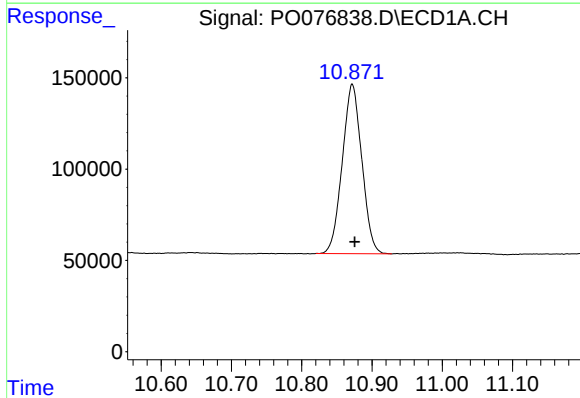


#2 Decachlorobiphenyl

R.T.: 10.872 min
Delta R.T.: -0.004 min
Response: 1792009
Conc: 19.35 ng/ml

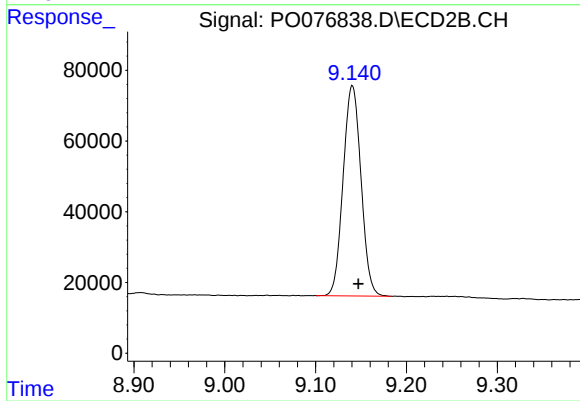

#2 Decachlorobiphenyl


R.T.: 9.140 min
Delta R.T.: -0.007 min
Response: 813758
Conc: 16.77 ng/ml

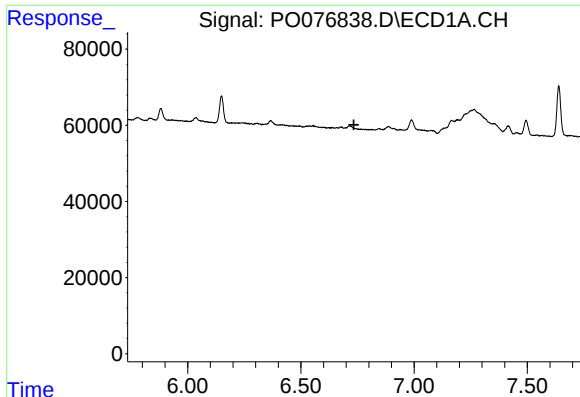

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.734 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

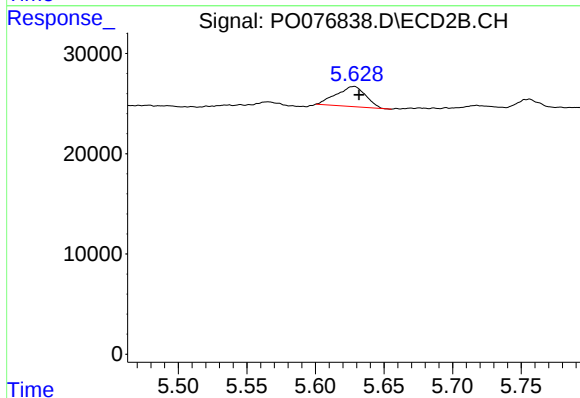


#7 AR-1016-5

R.T.: 5.628 min
Delta R.T.: -0.003 min
Response: 29800
Conc: 22.12 ng/ml

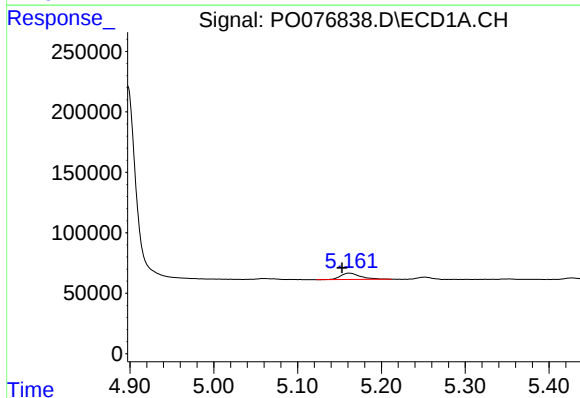


#8 AR-1221-1

R.T.: 5.162 min
Delta R.T.: 0.008 min
Response: 86048
Conc: 95.10 ng/ml

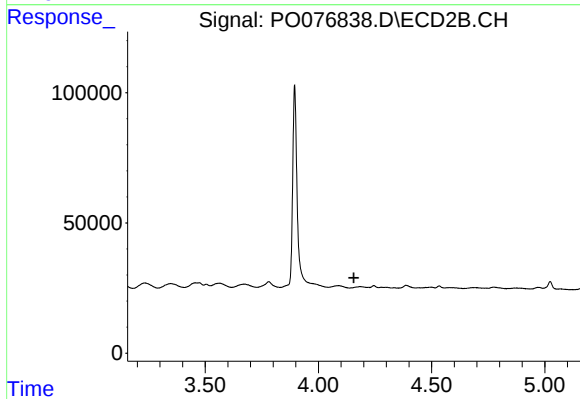

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 4.157 min
Response: 0
Conc: N.D.

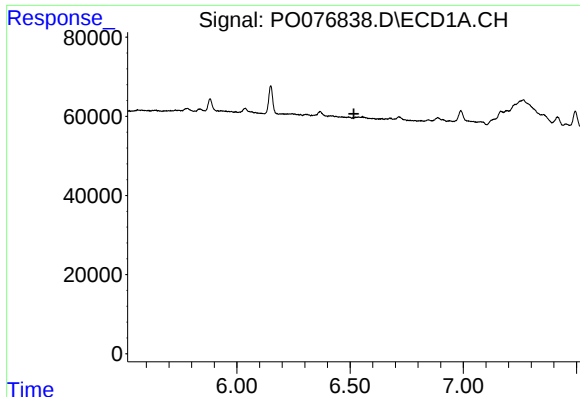

#15 AR-1232-5


R.T.: 0.000 min
Exp R.T.: 6.517 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

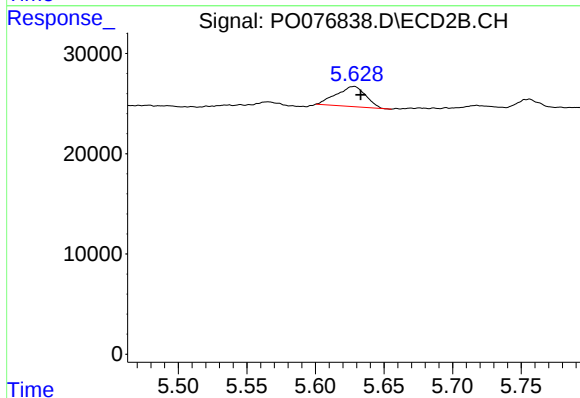


#15 AR-1232-5

R.T.: 5.628 min
Delta R.T.: -0.004 min
Response: 29800
Conc: 60.00 ng/ml

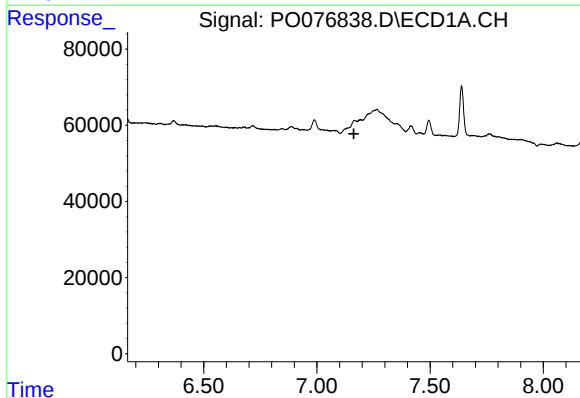


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 7.164 min
Response: 0
Conc: N.D.

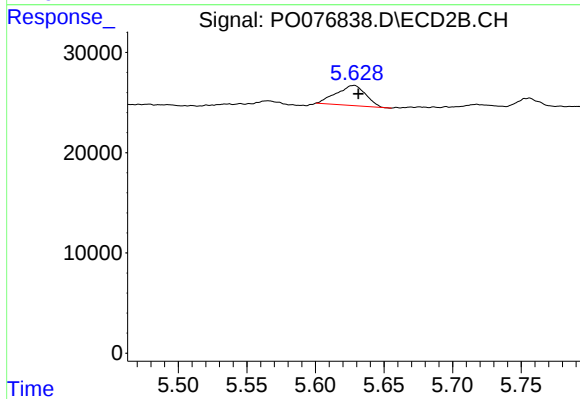

#24 AR-1248-4


R.T.: 5.628 min
Delta R.T.: -0.003 min
Response: 29800
Conc: 17.45 ng/ml

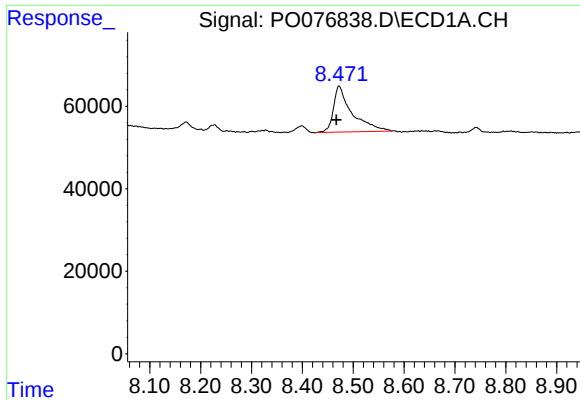

#30 AR-1254-5


R.T.: 8.472 min
Delta R.T.: 0.005 min
Response: 281284
Conc: 63.96 ng/ml

Instrument :
ECD_O
ClientSampleId :

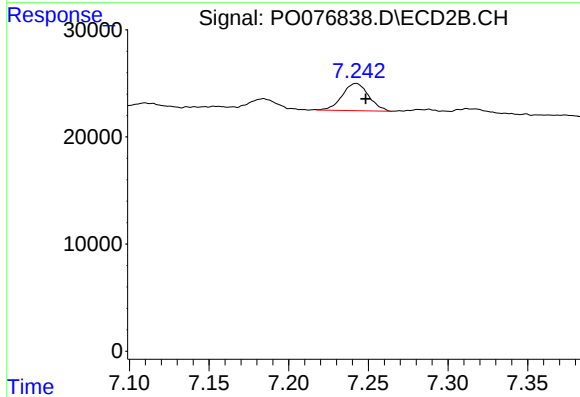


#30 AR-1254-5

R.T.: 7.242 min
Delta R.T.: -0.006 min
Response: 29510
Conc: 9.05 ng/ml

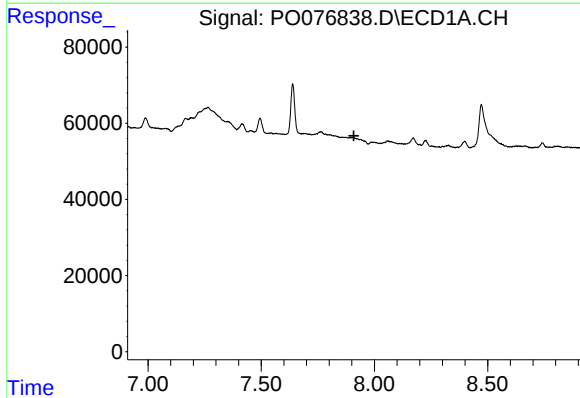


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 7.909 min
Response: 0
Conc: N.D.

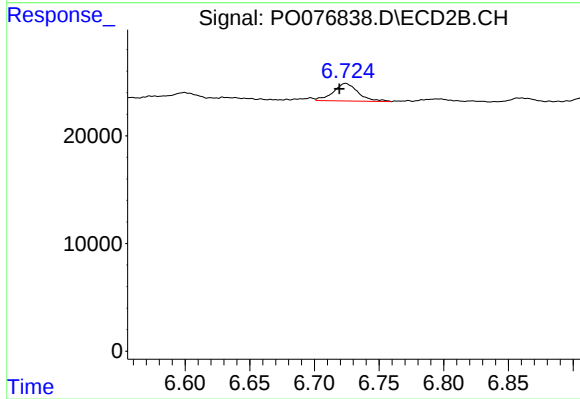

#31 AR-1260-1


R.T.: 6.724 min
Delta R.T.: 0.005 min
Response: 21721
Conc: 8.31 ng/ml

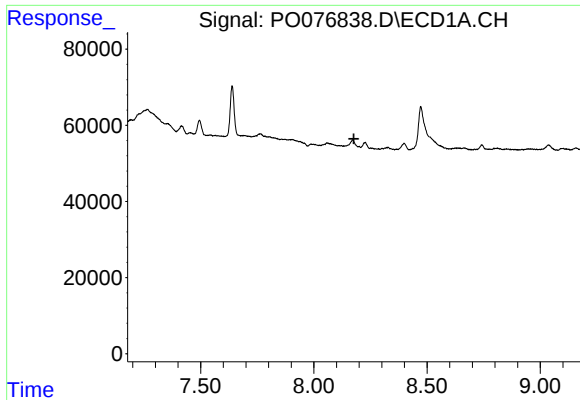

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 8.176 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

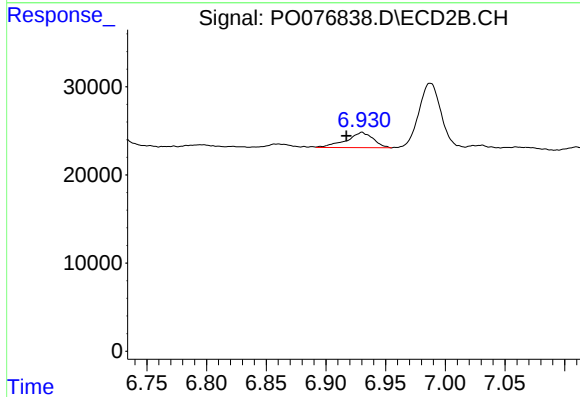


#32 AR-1260-2

R.T.: 6.930 min
Delta R.T.: 0.013 min
Response: 27171
Conc: 8.60 ng/ml

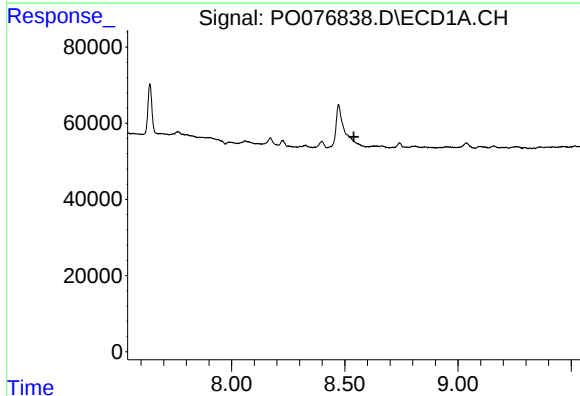

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 8.540 min
Response: 0
Conc: N.D.

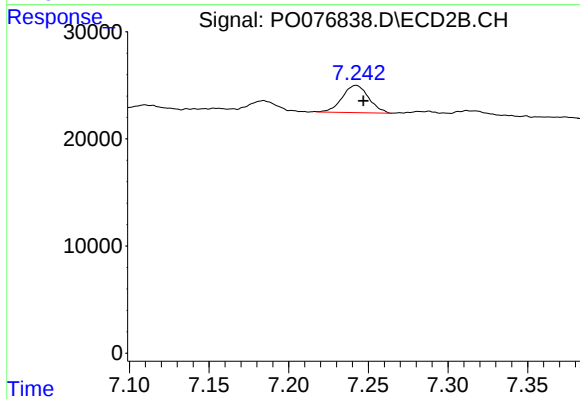

#36 AR-1262-1

R.T.: 7.242 min
Delta R.T.: -0.004 min
Response: 29510
Conc: 16.67 ng/ml