

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040621\
 Data File : P0076838.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Apr 2021 21:49
 Operator : DD\AJ
 Sample : M1933-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BENNETT_BH_01_2-2.5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 02:23:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.898	3.895	2005144	1040597	21.558	20.736
2)	SA Decachlor...	10.872	9.140	1792009	813758	19.348	16.769

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040621\
Data File : P0076838.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Apr 2021 21:49
Operator : DD\AJ
Sample : M1933-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BENNETT_BH_01_2-2.5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 02:23:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

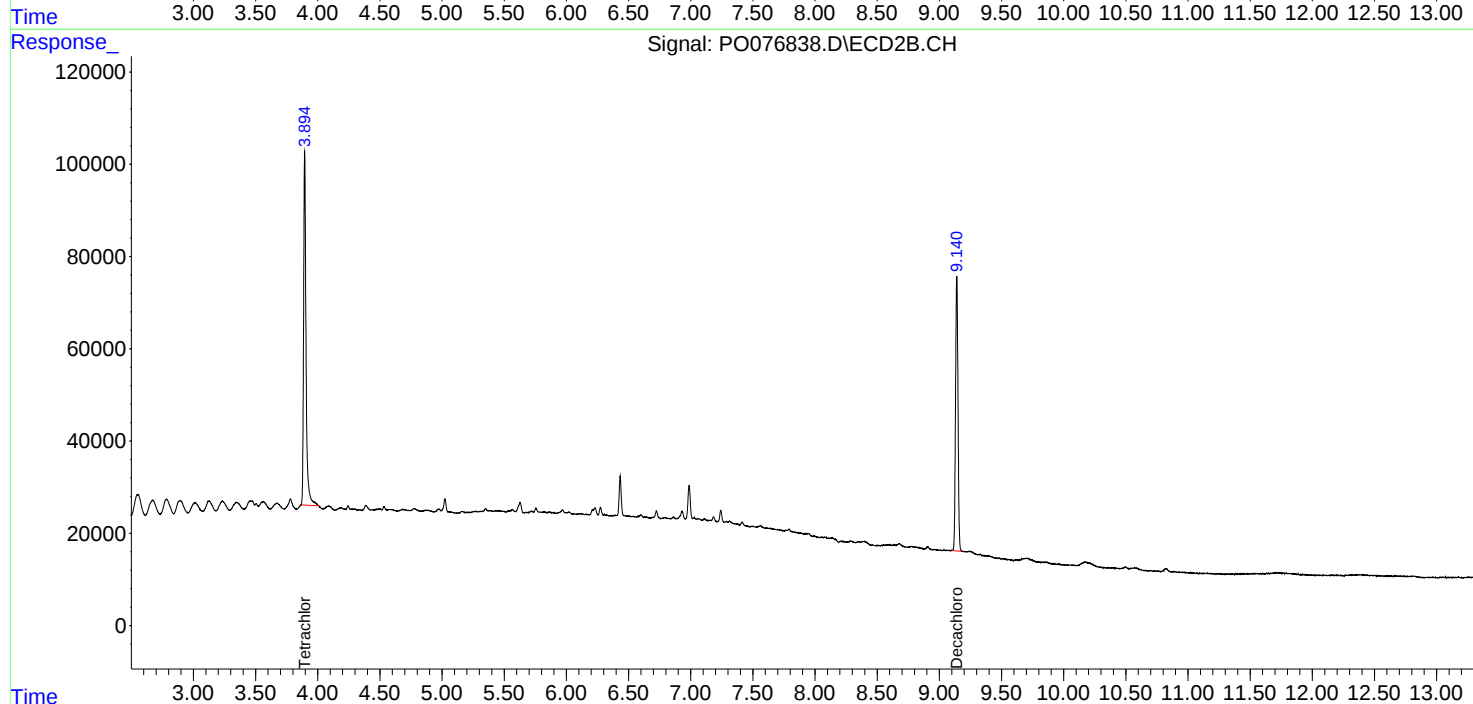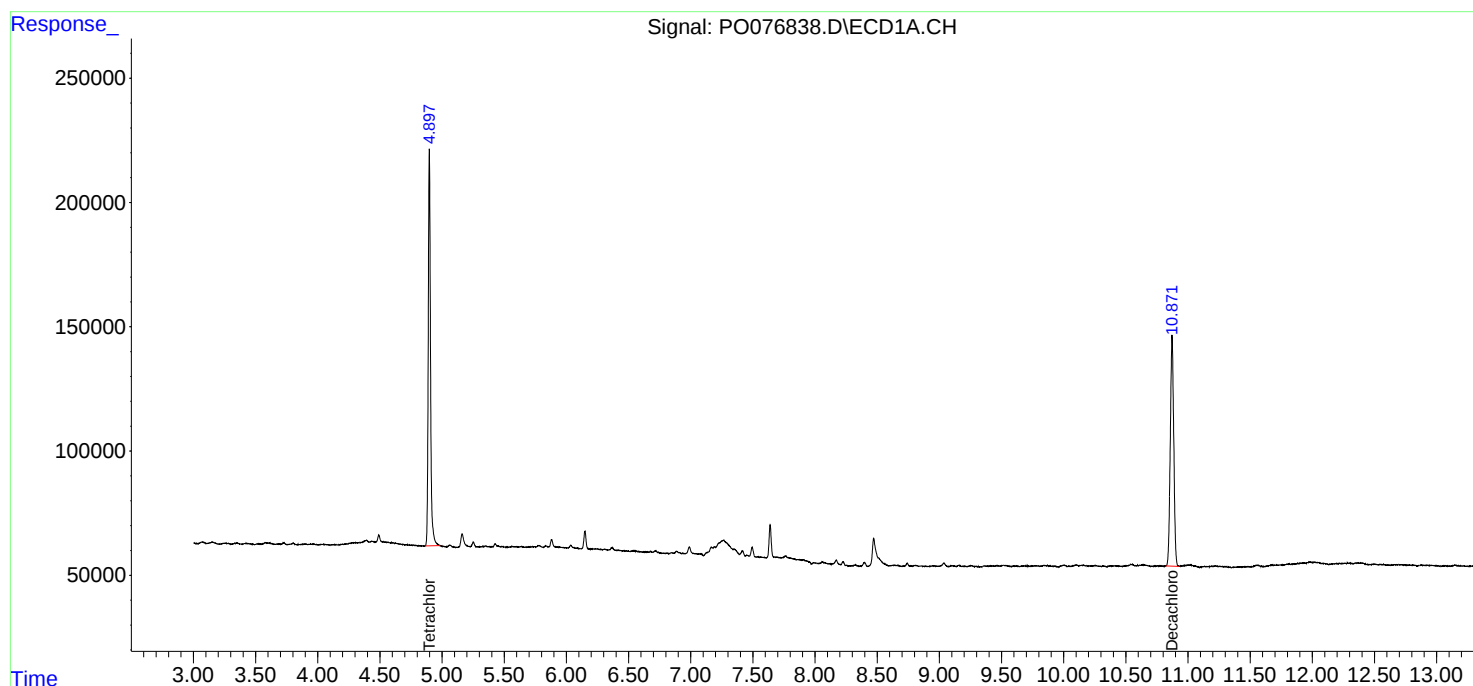


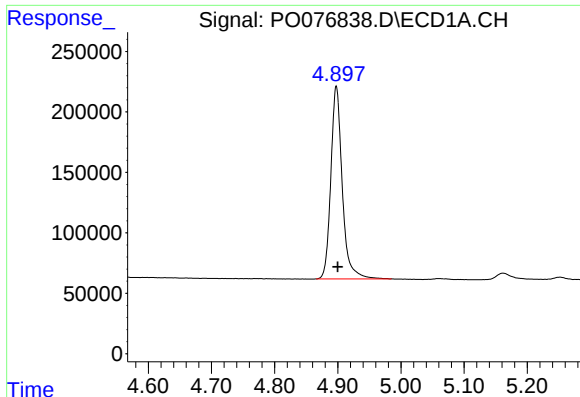

#1 Tetrachloro-m-xylene


R.T.: 4.898 min
Delta R.T.: -0.002 min
Response: 2005144
Conc: 21.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
BENNETT_BH_01_2-2.5

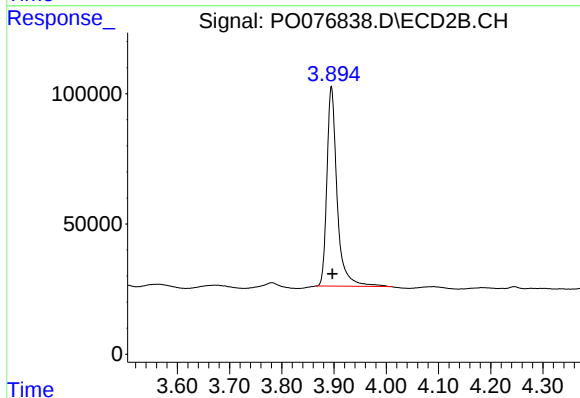


#1 Tetrachloro-m-xylene

R.T.: 3.895 min
Delta R.T.: -0.002 min
Response: 1040597
Conc: 20.74 ng/ml

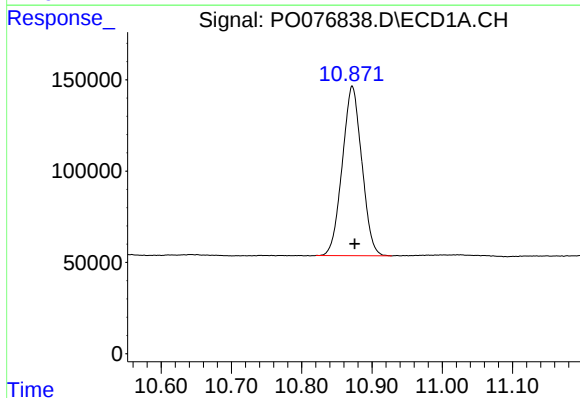

#2 Decachlorobiphenyl

R.T.: 10.872 min
Delta R.T.: -0.004 min
Response: 1792009
Conc: 19.35 ng/ml

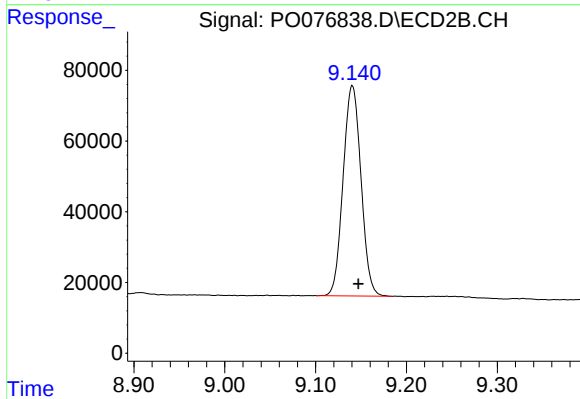

#2 Decachlorobiphenyl

R.T.: 9.140 min
Delta R.T.: -0.007 min
Response: 813758
Conc: 16.77 ng/ml