

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040621\
 Data File : P0076843.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Apr 2021 23:15
 Operator : DD\AJ
 Sample : M1933-16
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BENNET_BH_05_1-1.5

Manual Integrations
 APPROVED

Ankita
 4/7/2021 4:47:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 02:25:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.898	3.895	1818565	947611	19.552	18.883
2) SA Decachlor...	10.870	9.139	1268257	587718	13.693m	12.111

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040621\
Data File : P0076843.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Apr 2021 23:15
Operator : DD\AJ
Sample : M1933-16
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BENNET_BH_05_1-1.5


Manual Integrations
APPROVED

Ankita
4/7/2021 4:47:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 02:25:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

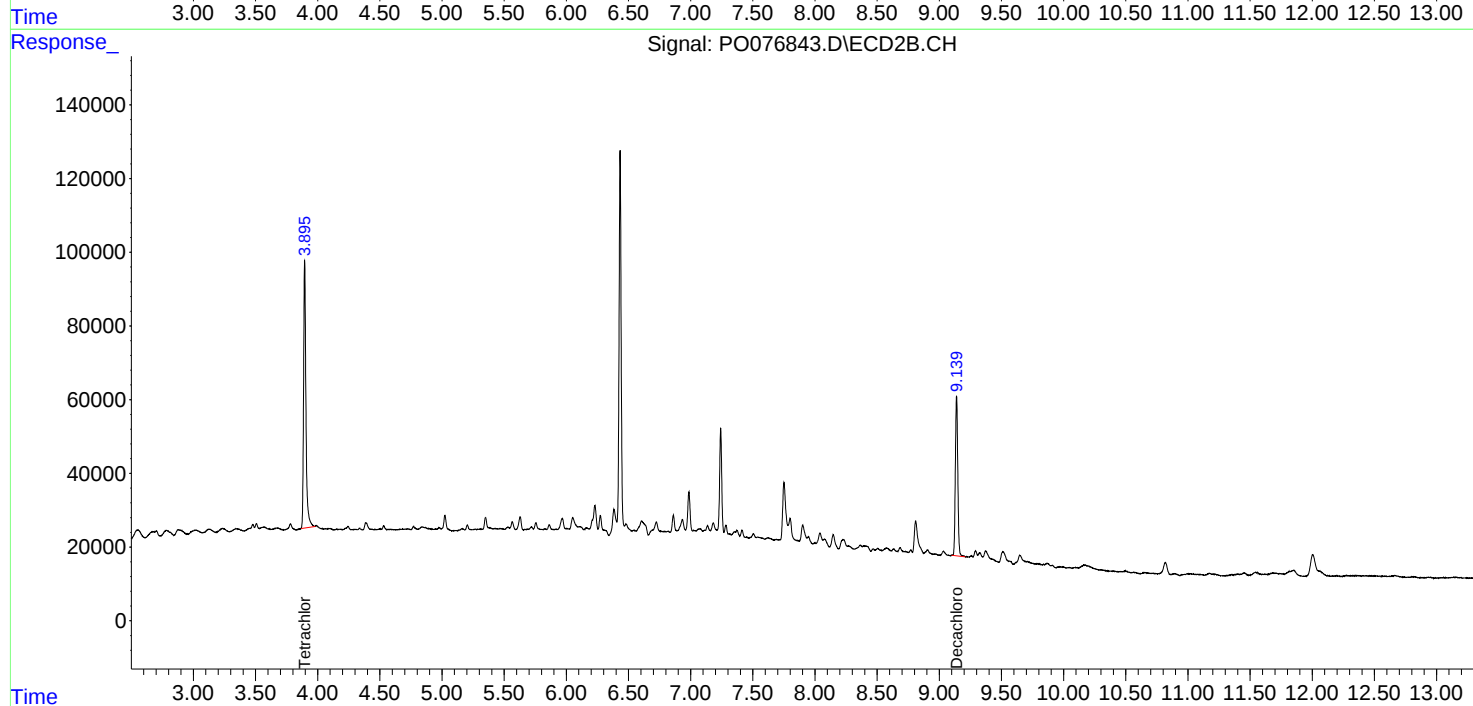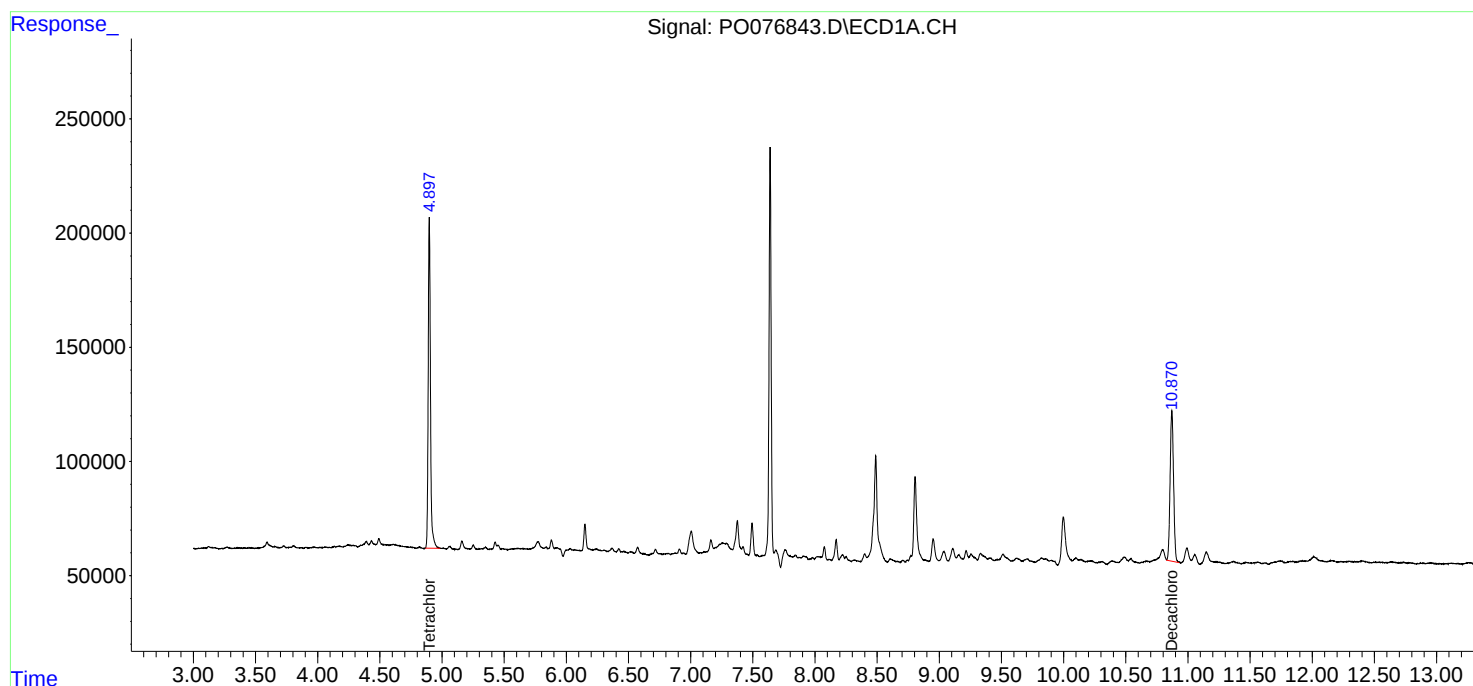

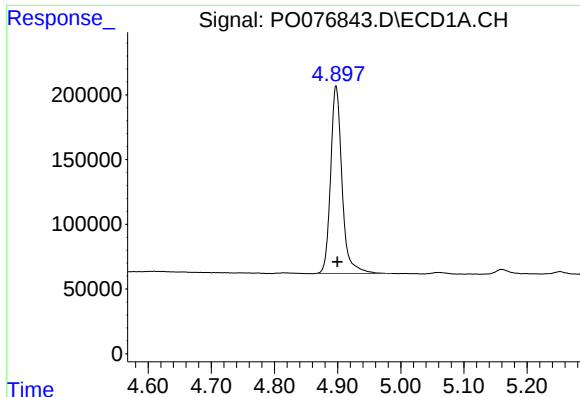


#1 Tetrachloro-m-xylene

R.T.: 4.898 min
Delta R.T.: -0.002 min
Response: 1818565
Conc: 19.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
BENNET_BH_05_1-1.5


Manual Integrations
APPROVED

Ankita
4/7/2021 4:47:56 PM

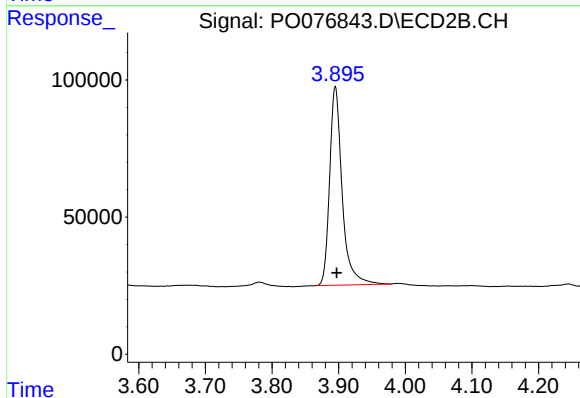


#1 Tetrachloro-m-xylene

R.T.: 3.895 min
Delta R.T.: -0.002 min
Response: 947611
Conc: 18.88 ng/ml

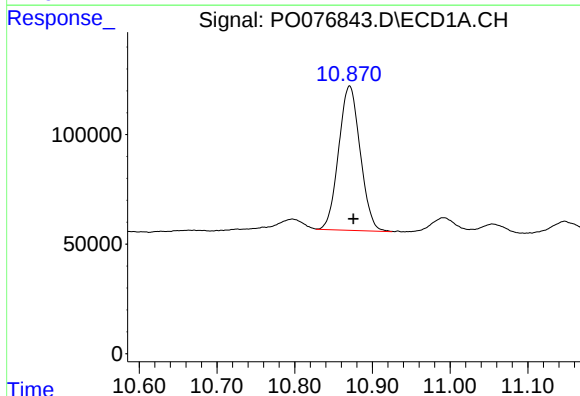

#2 Decachlorobiphenyl

R.T.: 10.870 min
Delta R.T.: -0.005 min
Response: 1268257
Conc: 13.69 ng/ml m

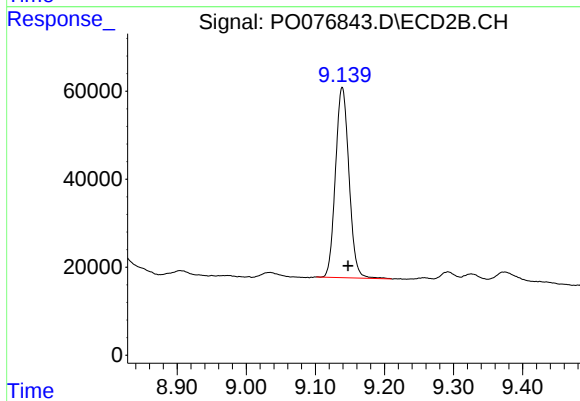

#2 Decachlorobiphenyl

R.T.: 9.139 min
Delta R.T.: -0.008 min
Response: 587718
Conc: 12.11 ng/ml