

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040623\
 Data File : P0093874.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Apr 2023 19:14
 Operator : YP/AJ
 Sample : 02207-02 10X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC226596-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/07/2023
 Supervised By :Ankita Jodhani 04/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 06 21:34:02 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.422	3.626	5407109	1839024	1.446	1.444
2) SA Decachlor...	10.244	8.646	4509811	1903242	2.016	1.904m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040623\
Data File : P0093874.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Apr 2023 19:14
Operator : YP/AJ
Sample : 02207-02 10X
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC226596-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/07/2023
Supervised By :Ankita Jodhani 04/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 06 21:34:02 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

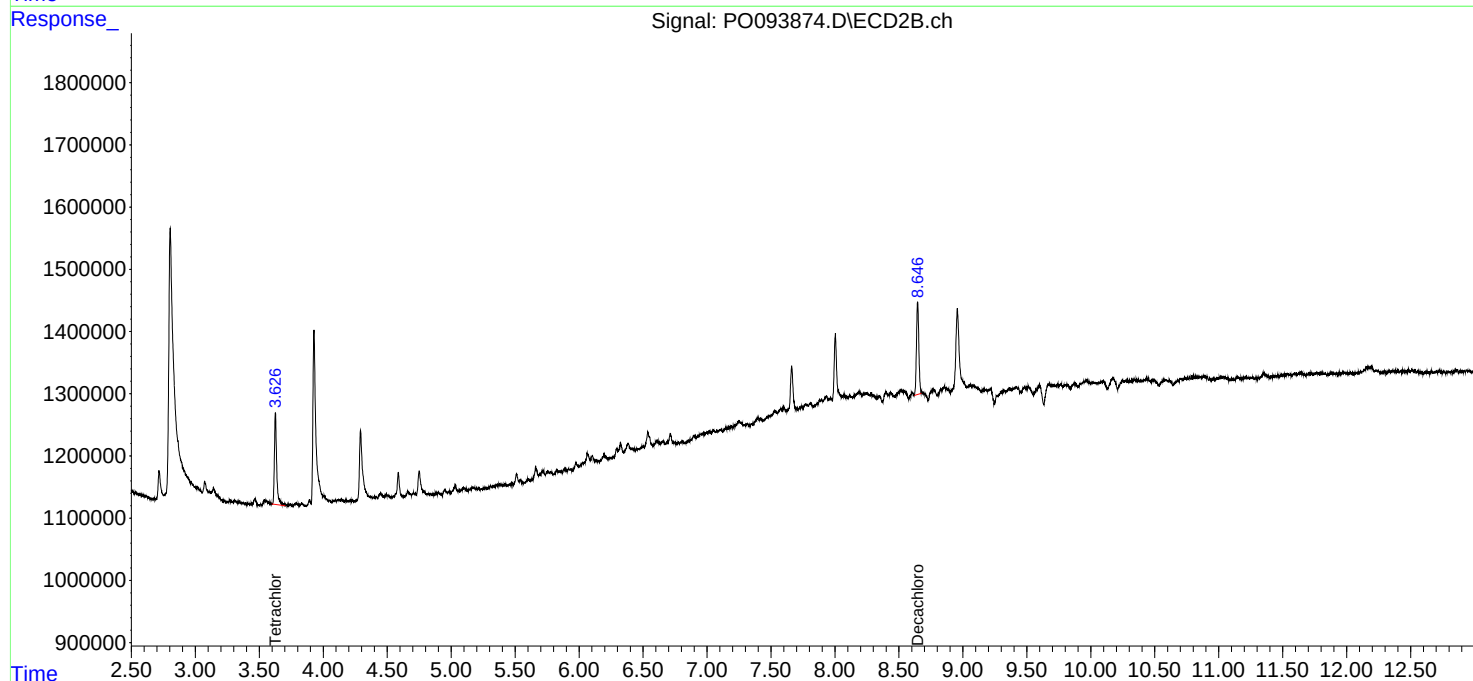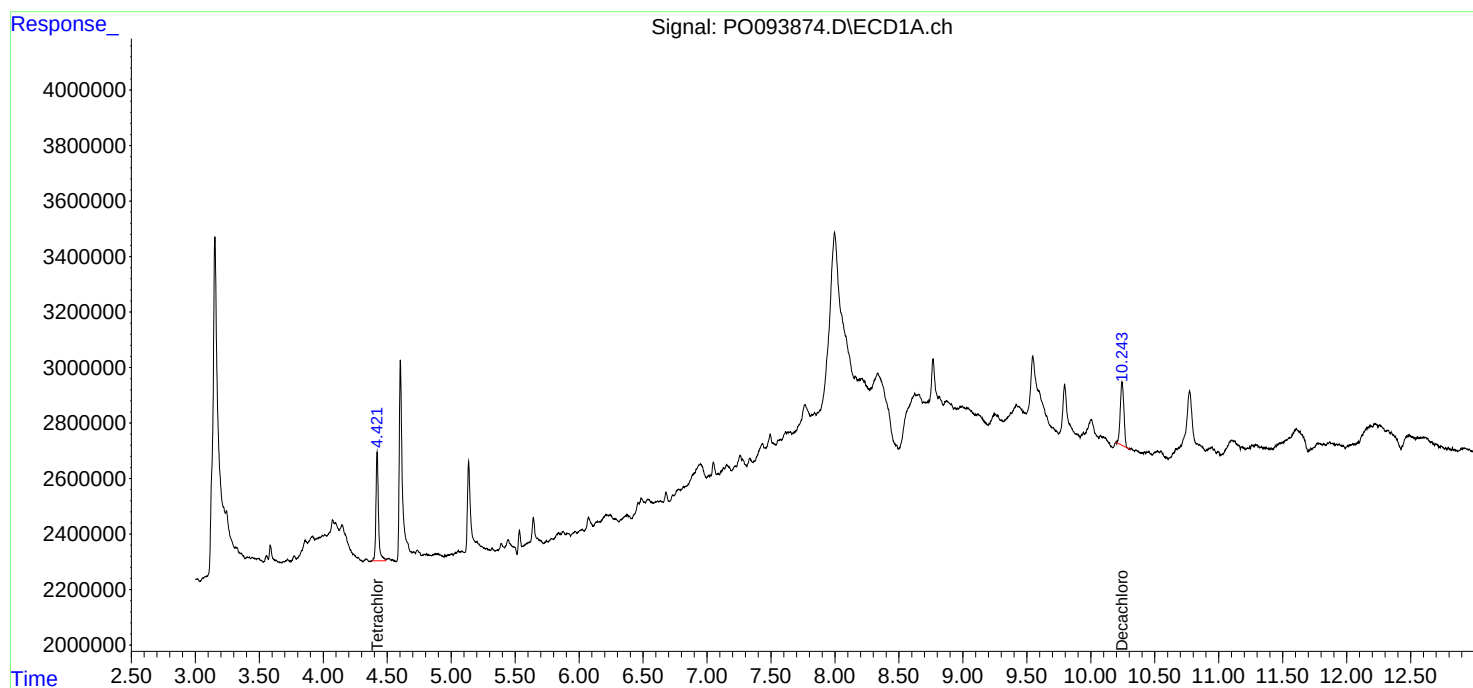

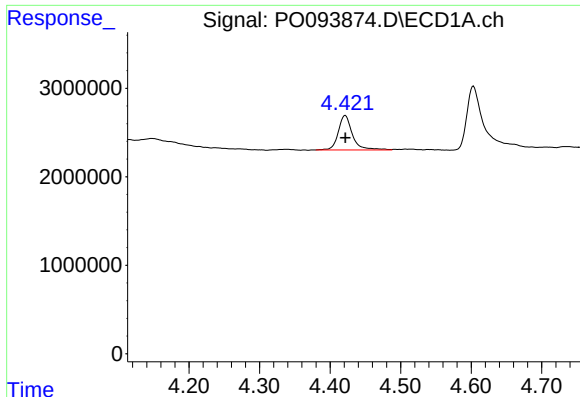


#1 Tetrachloro-m-xylene

R.T.: 4.422 min
Delta R.T.: 0.000 min
Response: 5407109
Conc: 1.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC226596-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/07/2023
Supervised By :Ankita Jodhani 04/07/2023

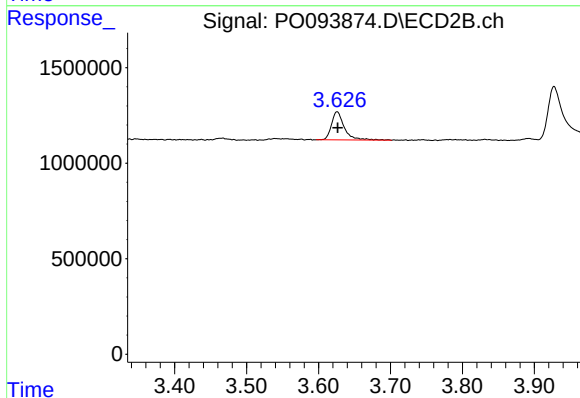


#1 Tetrachloro-m-xylene

R.T.: 3.626 min
Delta R.T.: 0.000 min
Response: 1839024
Conc: 1.44 ng/ml

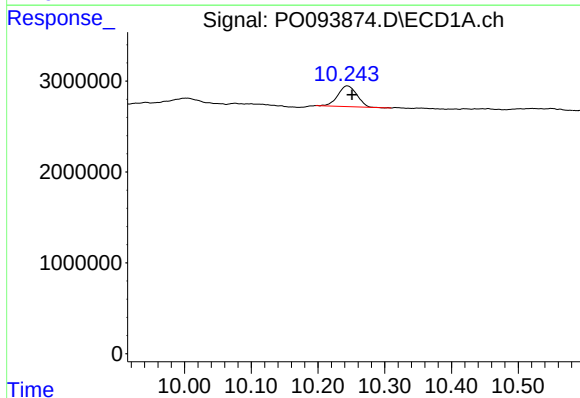

#2 Decachlorobiphenyl

R.T.: 10.244 min
Delta R.T.: -0.006 min
Response: 4509811
Conc: 2.02 ng/ml

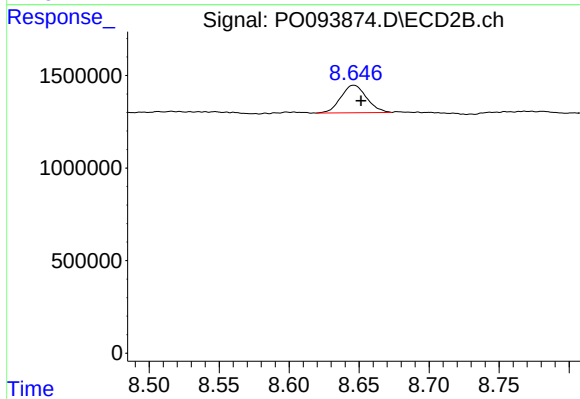

#2 Decachlorobiphenyl

R.T.: 8.646 min
Delta R.T.: -0.006 min
Response: 1903242
Conc: 1.90 ng/ml m