

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0040623\
 Data File : P0093888.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2023 00:11
 Operator : YP/AJ
 Sample : 02218-01 10X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 BC247601-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/07/2023
 Supervised By :Ankita Jodhani 04/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 04:54:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.420	3.624	6982448	2233392	1.868	1.754
2) SA Decachlor...	10.244	8.644	4947213	2036930	2.212	2.037
Target Compounds						
26) L6 AR-1254-1	6.457	5.508	1832060	519644	13.508m	7.602m#
27) L6 AR-1254-2	6.678	5.658	1563721	531190	8.000m	8.722
28) L6 AR-1254-3	7.047	6.059	1824678	302725	9.877m	3.323m#
29) L6 AR-1254-4	7.337	6.291	1076942	444462	10.619	10.435
30) L6 AR-1254-5	7.759	6.710	2069769	725507	15.263	10.055 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040623\
Data File : P0093888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2023 00:11
Operator : YP/AJ
Sample : 02218-01 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC247601-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/07/2023
Supervised By :Ankita Jodhani 04/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 04:54:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

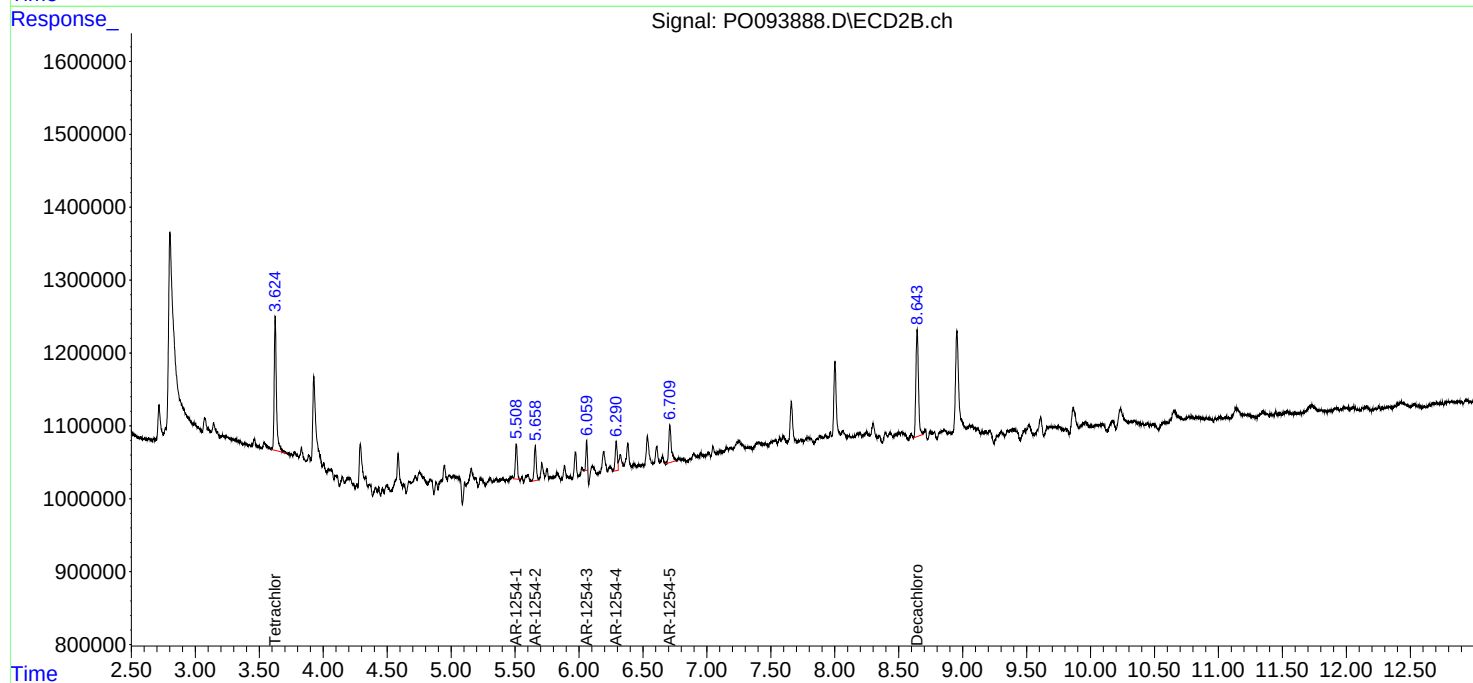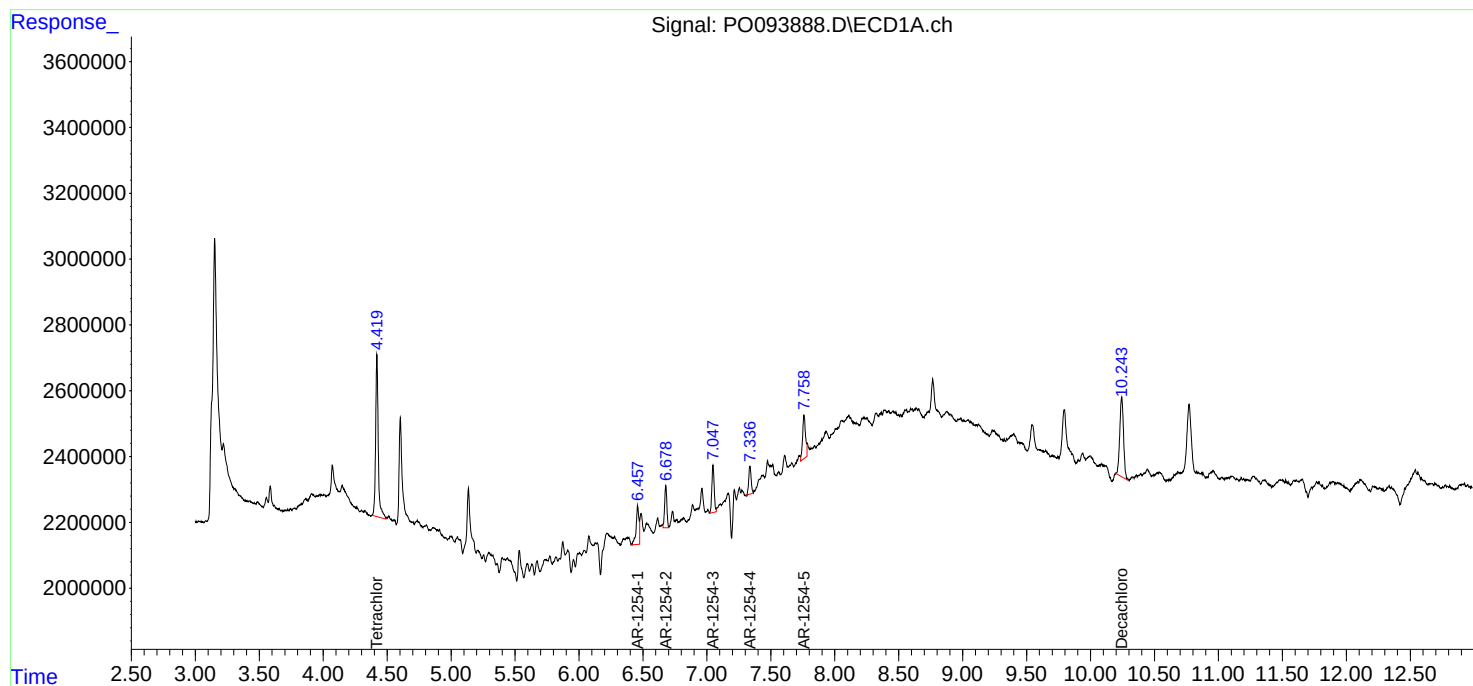

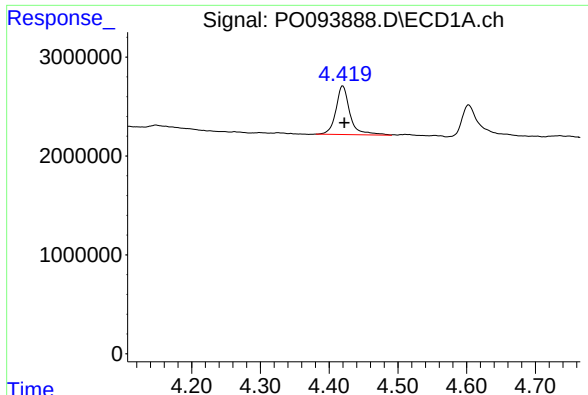


#1 Tetrachloro-m-xylene

R.T.: 4.420 min
Delta R.T.: -0.002 min
Response: 6982448
Conc: 1.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC247601-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/07/2023
Supervised By :Ankita Jodhani 04/07/2023

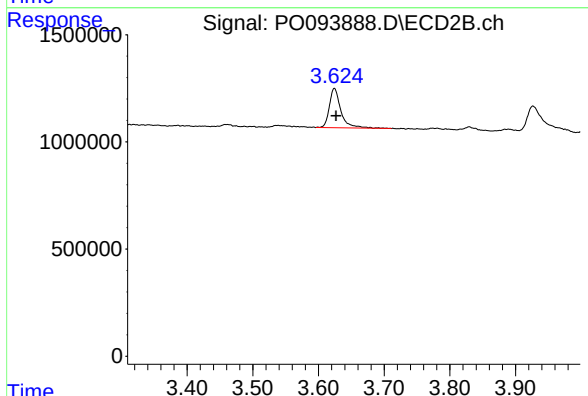


#1 Tetrachloro-m-xylene

R.T.: 3.624 min
Delta R.T.: -0.002 min
Response: 2233392
Conc: 1.75 ng/ml

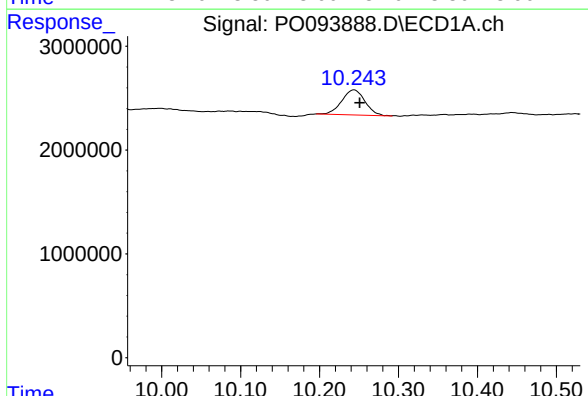


#2 Decachlorobiphenyl

R.T.: 10.244 min
Delta R.T.: -0.007 min
Response: 4947213
Conc: 2.21 ng/ml

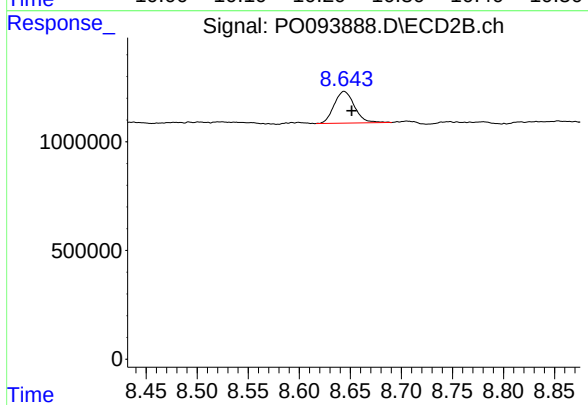

#2 Decachlorobiphenyl

R.T.: 8.644 min
Delta R.T.: -0.007 min
Response: 2036930
Conc: 2.04 ng/ml

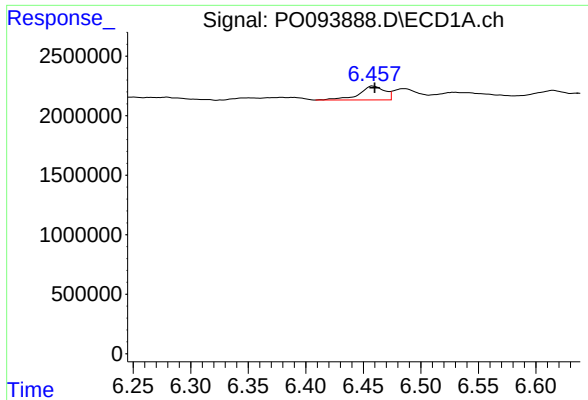


#26 AR-1254-1

R.T.: 6.457 min
Delta R.T.: -0.003 min
Response: 1832060
Conc: 13.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC247601-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/07/2023
Supervised By :Ankita Jodhani 04/07/2023

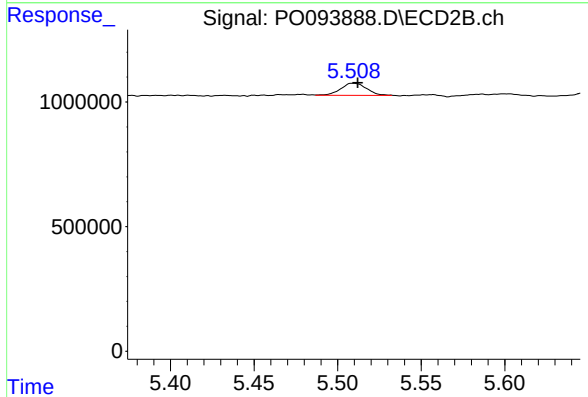


#26 AR-1254-1

R.T.: 5.508 min
Delta R.T.: -0.004 min
Response: 519644
Conc: 7.60 ng/ml m

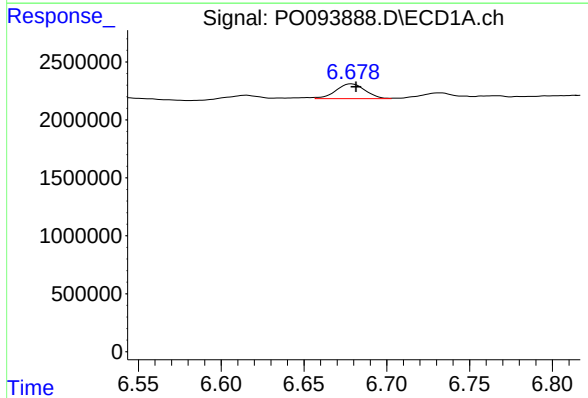


#27 AR-1254-2

R.T.: 6.678 min
Delta R.T.: -0.003 min
Response: 1563721
Conc: 8.00 ng/ml m

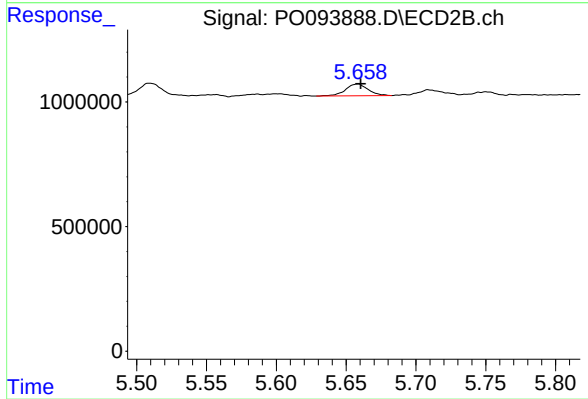

#27 AR-1254-2

R.T.: 5.658 min
Delta R.T.: -0.002 min
Response: 531190
Conc: 8.72 ng/ml

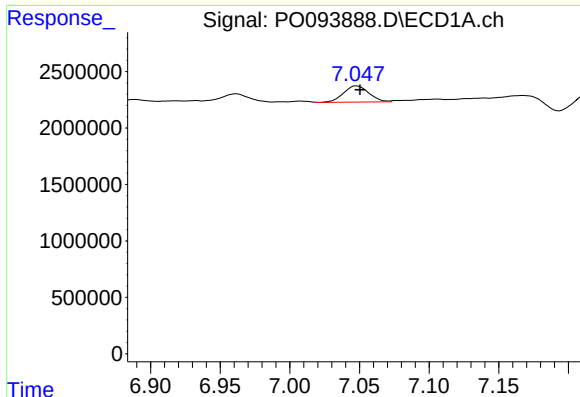


#28 AR-1254-3

R.T.: 7.047 min
Delta R.T.: -0.003 min
Response: 1824678
Conc: 9.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC247601-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/07/2023
Supervised By :Ankita Jodhani 04/07/2023

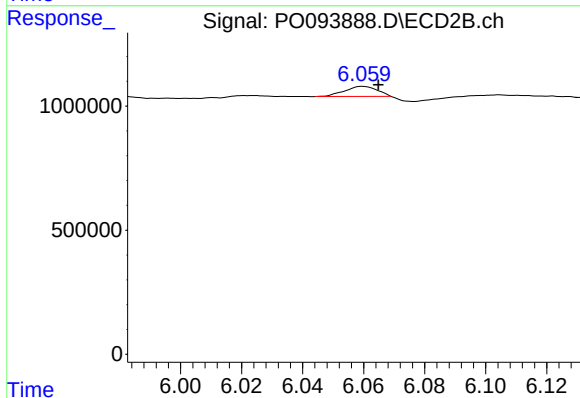


#28 AR-1254-3

R.T.: 6.059 min
Delta R.T.: -0.006 min
Response: 302725
Conc: 3.32 ng/ml m

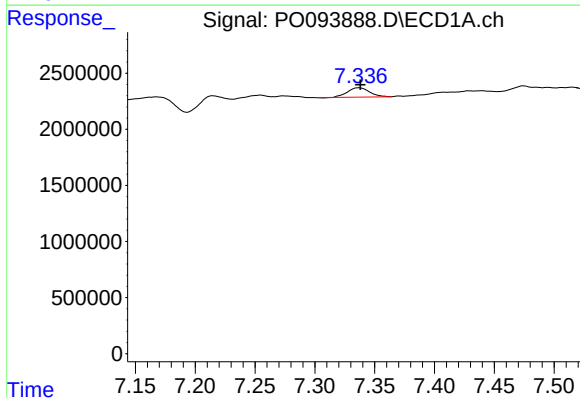


#29 AR-1254-4

R.T.: 7.337 min
Delta R.T.: -0.001 min
Response: 1076942
Conc: 10.62 ng/ml

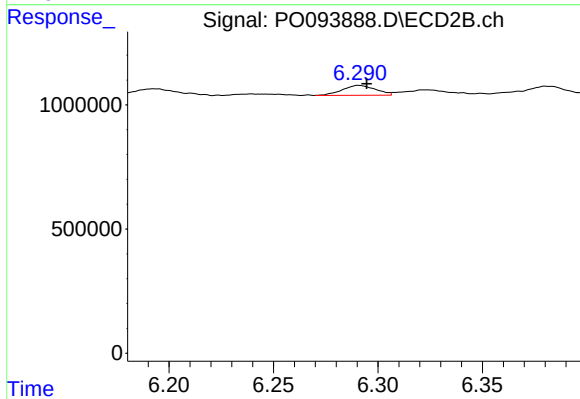

#29 AR-1254-4

R.T.: 6.291 min
Delta R.T.: -0.004 min
Response: 444462
Conc: 10.43 ng/ml

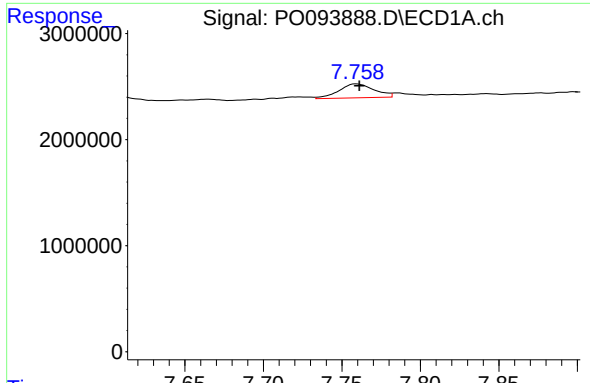


#30 AR-1254-5

R.T.: 7.759 min
Delta R.T.: -0.002 min
Response: 2069769
Conc: 15.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC247601-1-1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/07/2023
Supervised By :Ankita Jodhani 04/07/2023

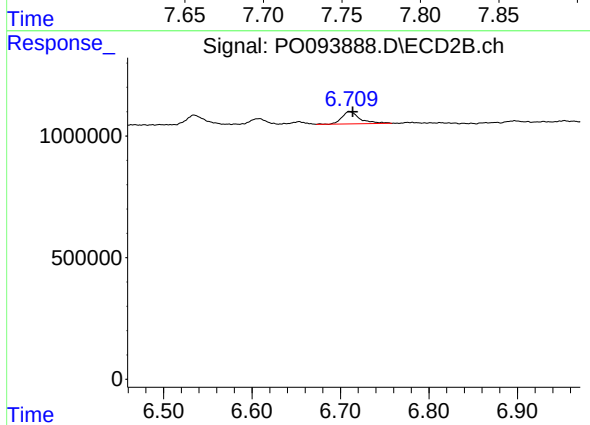

#30 AR-1254-5

R.T.: 6.710 min
Delta R.T.: -0.004 min
Response: 725507
Conc: 10.06 ng/ml