

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040623\
 Data File : P0093895.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2023 03:08
 Operator : YP/AJ
 Sample : 02195-01 10X
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 194

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/07/2023
 Supervised By :Ankita Jodhani 04/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 04:59:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.416	3.624	7212457	1214238	1.929	0.954 #
2) SA Decachlor...	10.243	8.646	6478584	1768069	2.896m	1.768 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040623\
Data File : P0093895.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2023 03:08
Operator : YP/AJ
Sample : 02195-01 10X
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
194


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/07/2023
Supervised By :Ankita Jodhani 04/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 04:59:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

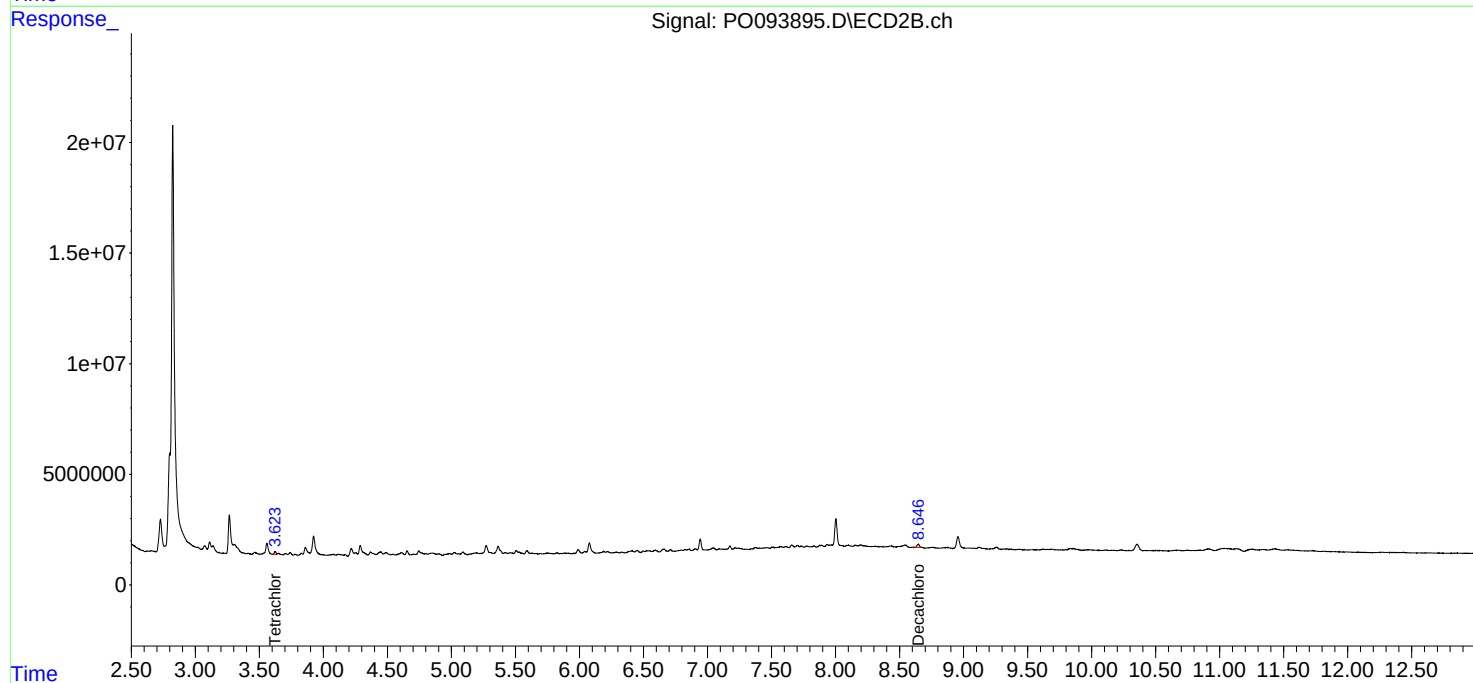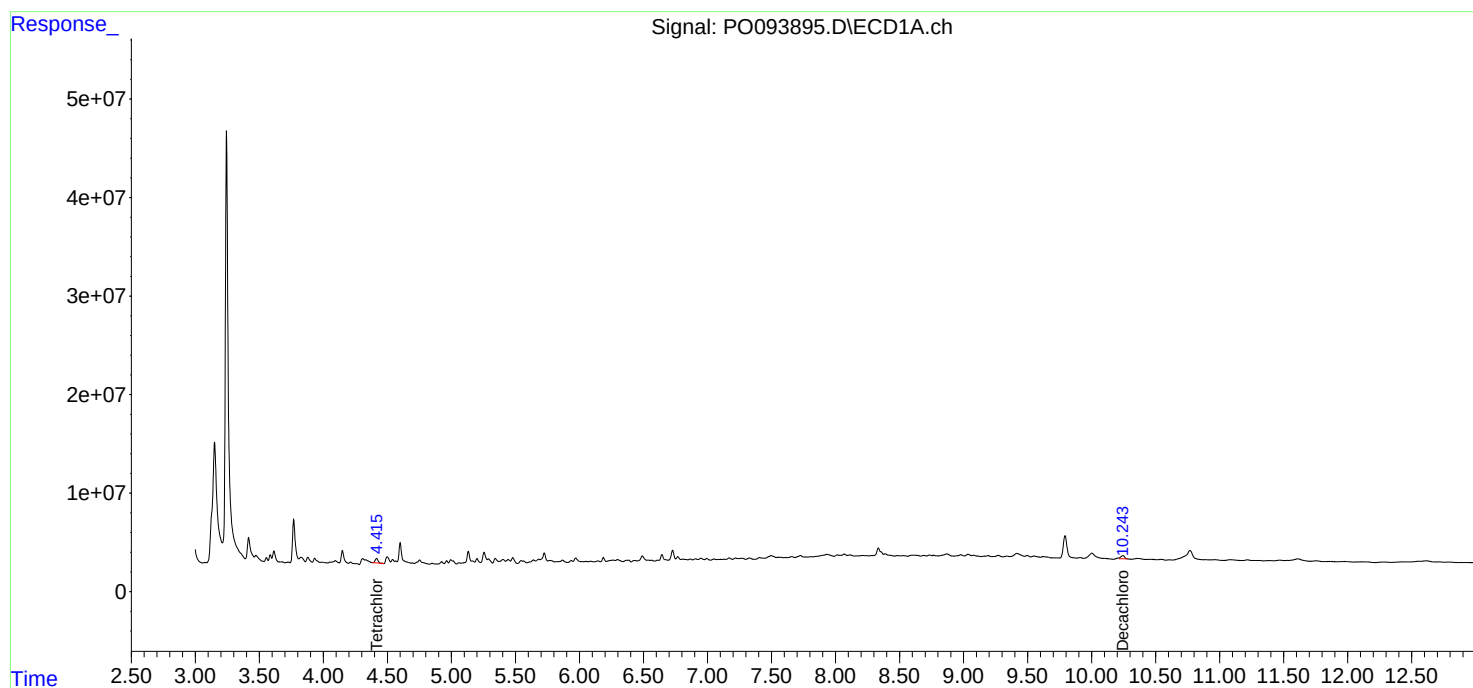

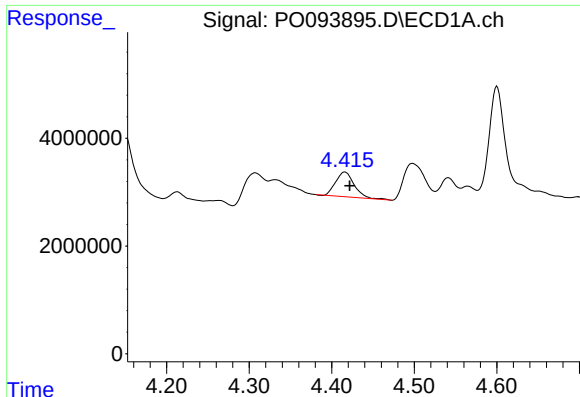


#1 Tetrachloro-m-xylene

R.T.: 4.416 min
Delta R.T.: -0.006 min
Response: 7212457
Conc: 1.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
194


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/07/2023
Supervised By :Ankita Jodhani 04/07/2023

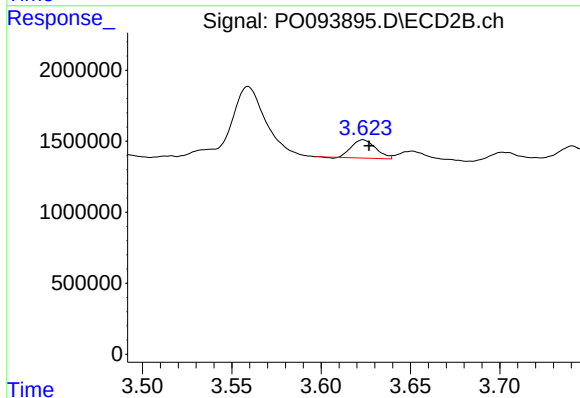


#1 Tetrachloro-m-xylene

R.T.: 3.624 min
Delta R.T.: -0.003 min
Response: 1214238
Conc: 0.95 ng/ml

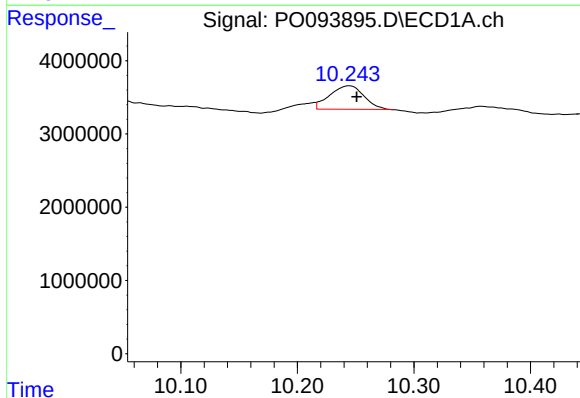

#2 Decachlorobiphenyl

R.T.: 10.243 min
Delta R.T.: -0.007 min
Response: 6478584
Conc: 2.90 ng/ml m

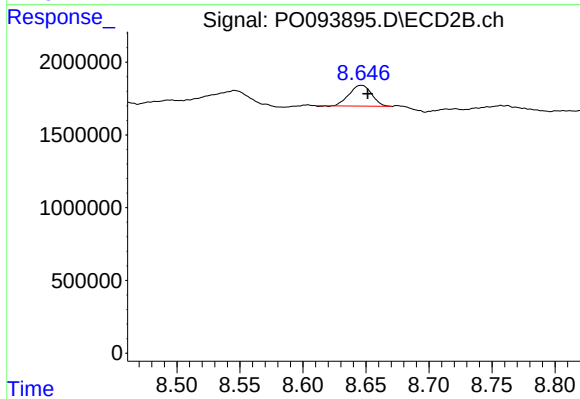

#2 Decachlorobiphenyl

R.T.: 8.646 min
Delta R.T.: -0.005 min
Response: 1768069
Conc: 1.77 ng/ml