

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040721\
 Data File : P0076861.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Apr 2021 14:53
 Operator : DD\AJ
 Sample : M1919-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 15:42:29 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.898	3.895	1289565	664791	13.864	13.247
2) SA Decachlor...	10.871	9.139	532204	255021	5.746	5.255
Target Compounds						
7) L1 AR-1016-5	0.000	5.616f	0	36046	N.D.	26.760 #
15) L3 AR-1232-5	0.000	5.616f	0	36046	N.D.	72.579 #
24) L5 AR-1248-4	0.000	5.616f	0	36046	N.D.	21.113 #
30) L6 AR-1254-5	0.000	7.245	0	17707	N.D.	5.432 #
31) L7 AR-1260-1	0.000	6.724	0	19207	N.D.	7.351 #
32) L7 AR-1260-2	0.000	6.928	0	19691	N.D.	6.236 #
36) L8 AR-1262-1	0.000	7.245	0	17707	N.D.	10.003 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040721\
Data File : P0076861.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Apr 2021 14:53
Operator : DD\AJ
Sample : M1919-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 15:42:29 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

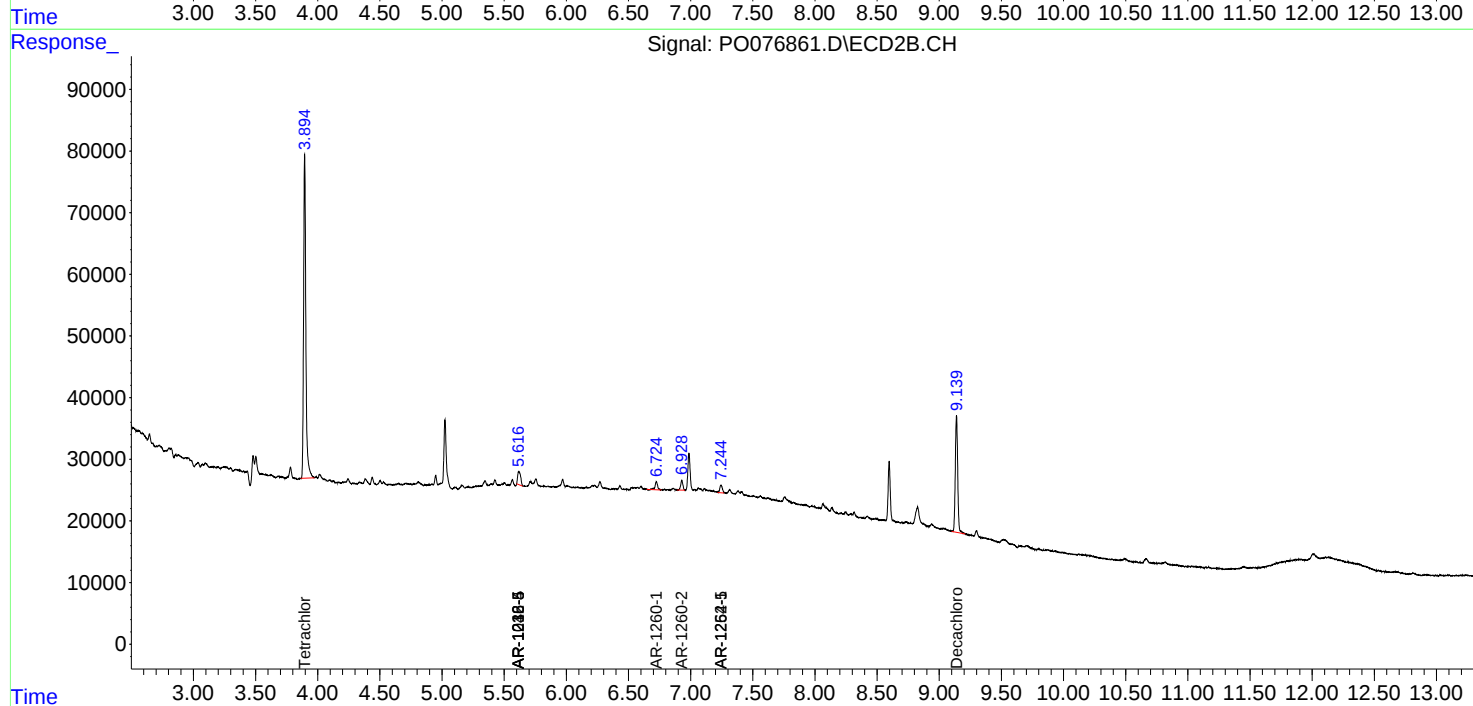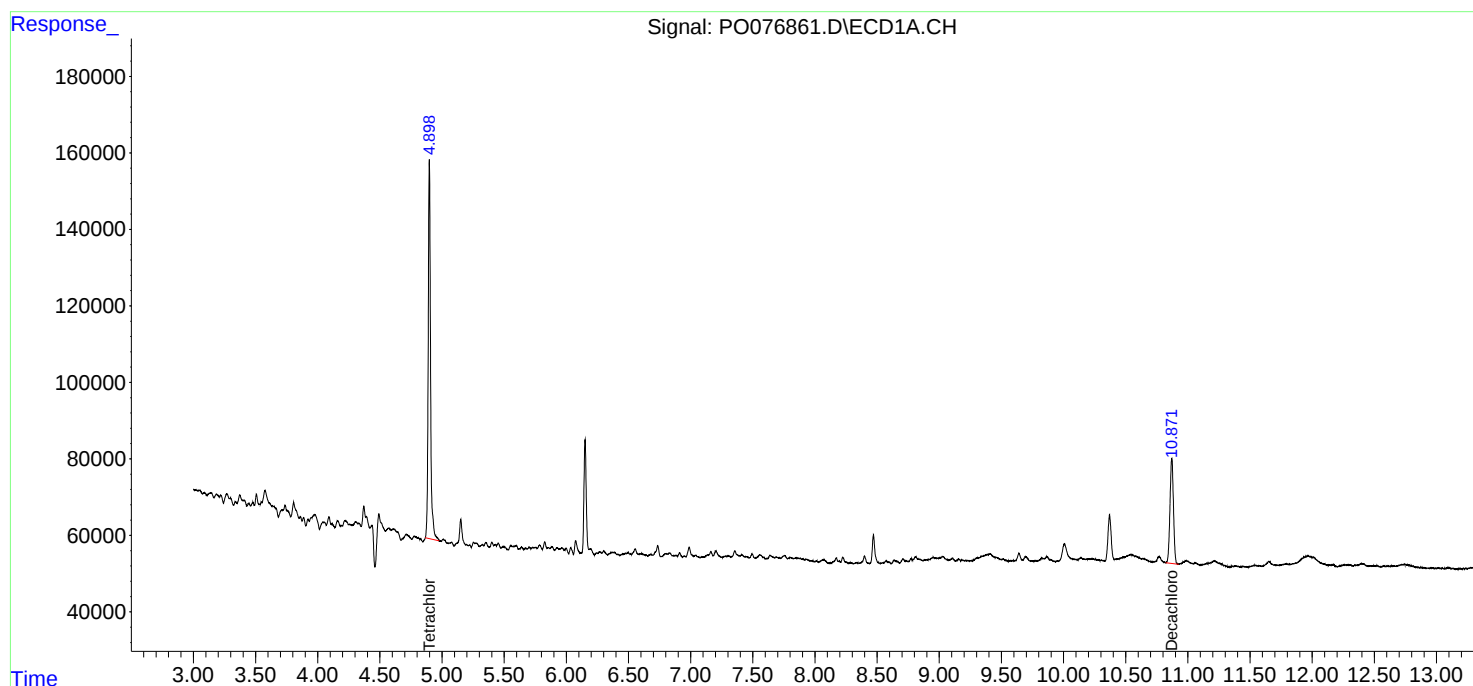


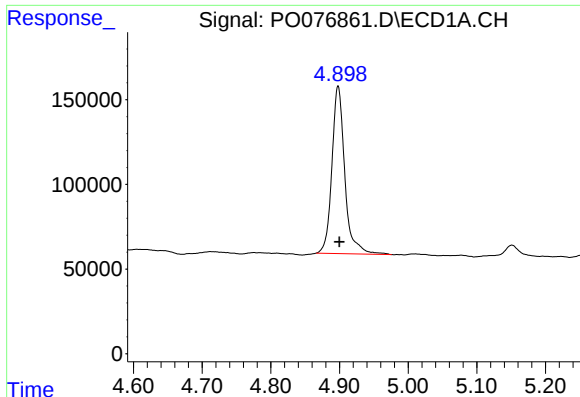

#1 Tetrachloro-m-xylene


R.T.: 4.898 min
Delta R.T.: -0.002 min
Response: 1289565
Conc: 13.86 ng/ml

Instrument :
ECD_O
ClientSampleId :

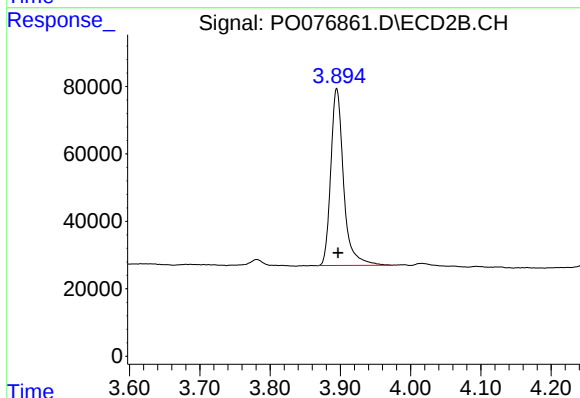


#1 Tetrachloro-m-xylene

R.T.: 3.895 min
Delta R.T.: -0.002 min
Response: 664791
Conc: 13.25 ng/ml

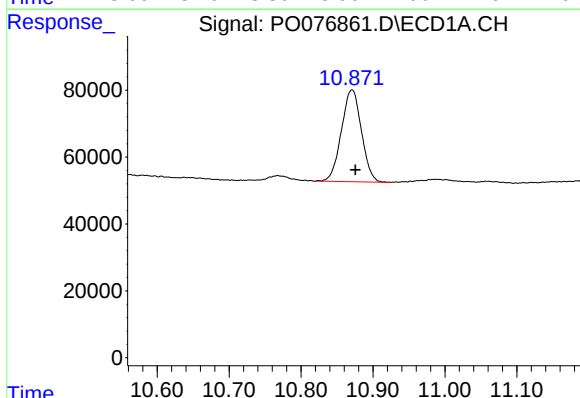


#2 Decachlorobiphenyl

R.T.: 10.871 min
Delta R.T.: -0.005 min
Response: 532204
Conc: 5.75 ng/ml

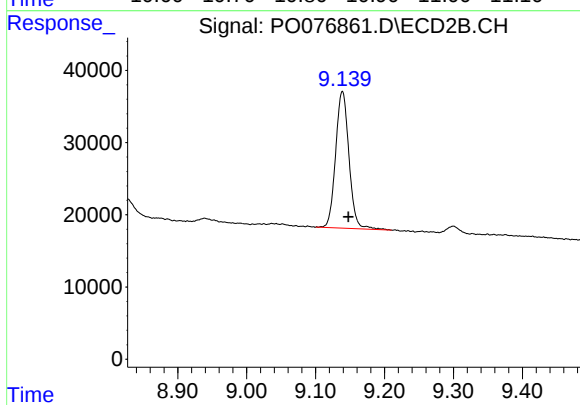

#2 Decachlorobiphenyl


R.T.: 9.139 min
Delta R.T.: -0.008 min
Response: 255021
Conc: 5.26 ng/ml

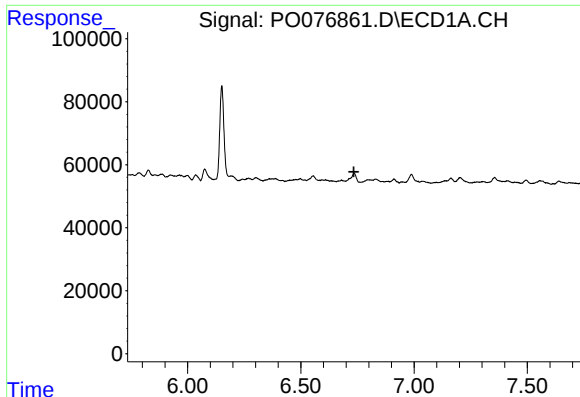

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.734 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

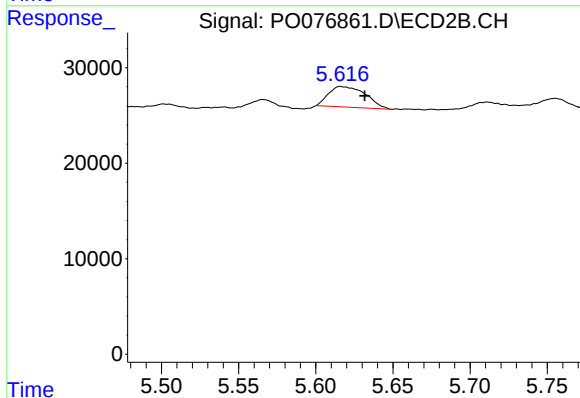


#7 AR-1016-5

R.T.: 5.616 min
Delta R.T.: -0.016 min
Response: 36046
Conc: 26.76 ng/ml

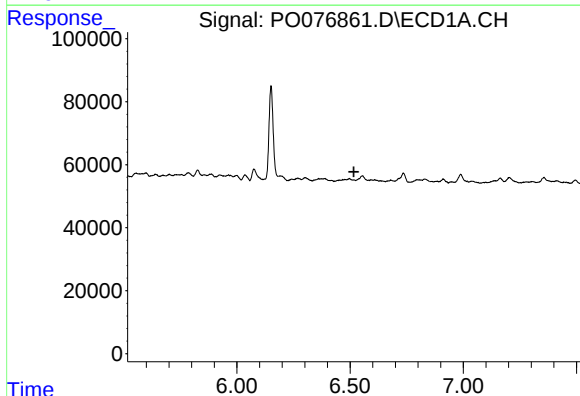


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T.: 6.517 min
Response: 0
Conc: N.D.

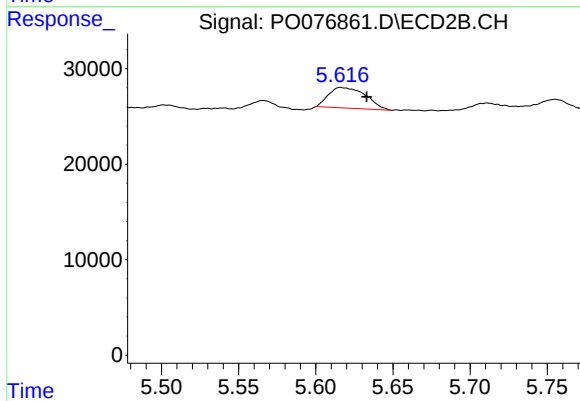

#15 AR-1232-5


R.T.: 5.616 min
Delta R.T.: -0.017 min
Response: 36046
Conc: 72.58 ng/ml

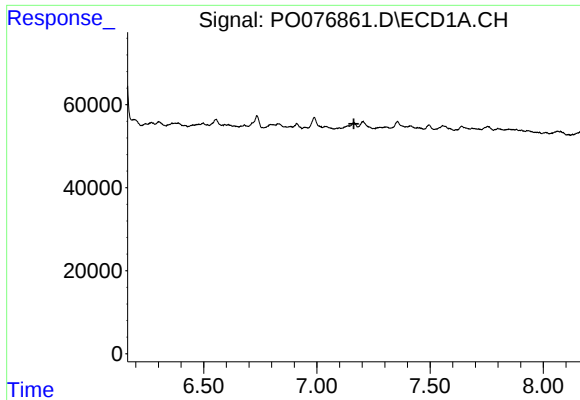

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 7.164 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

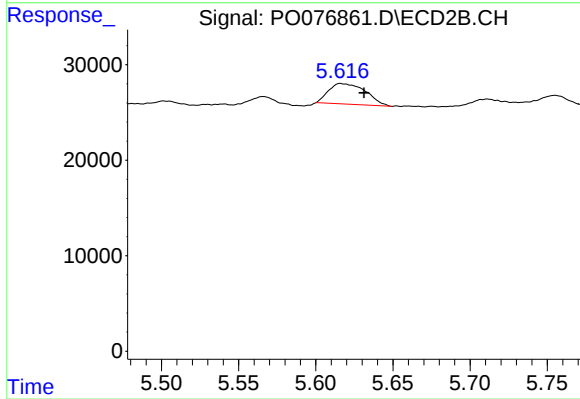


#24 AR-1248-4

R.T.: 5.616 min
Delta R.T.: -0.015 min
Response: 36046
Conc: 21.11 ng/ml

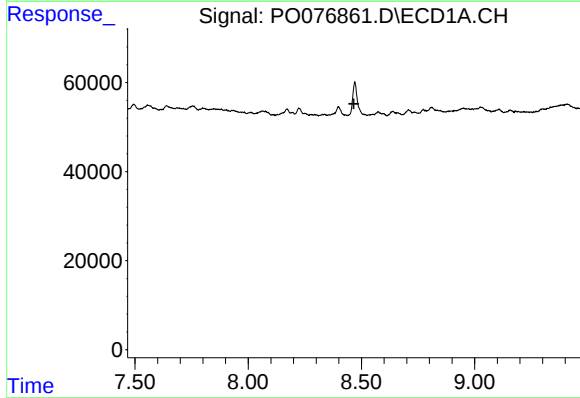


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 8.467 min
Response: 0
Conc: N.D.

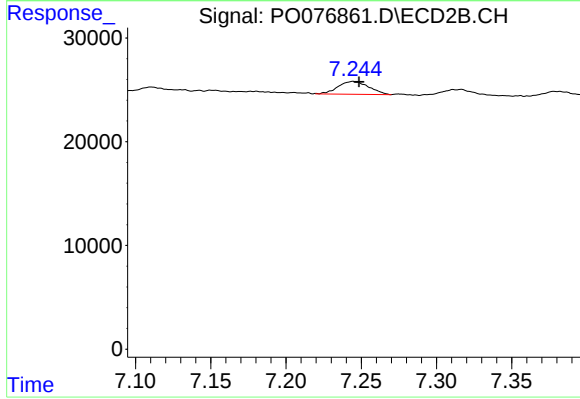

#30 AR-1254-5


R.T.: 7.245 min
Delta R.T.: -0.004 min
Response: 17707
Conc: 5.43 ng/ml

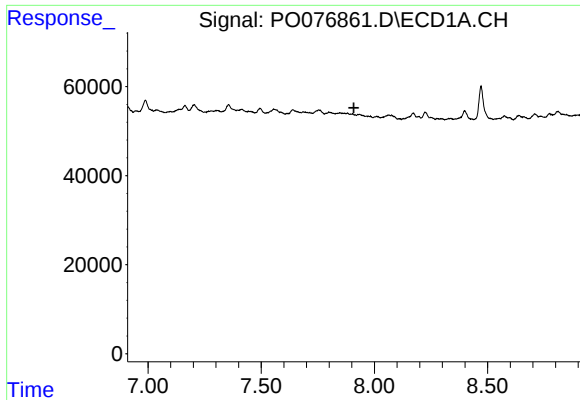

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 7.909 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

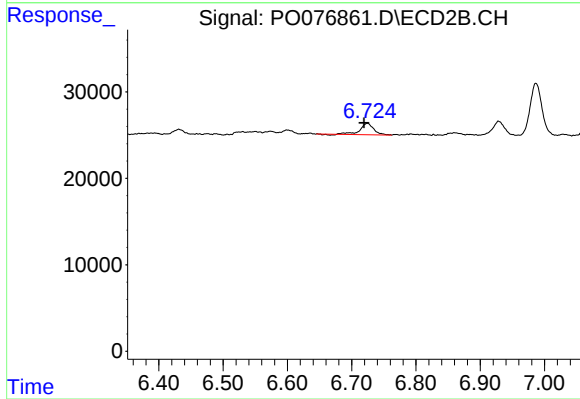


#31 AR-1260-1

R.T.: 6.724 min
Delta R.T.: 0.005 min
Response: 19207
Conc: 7.35 ng/ml

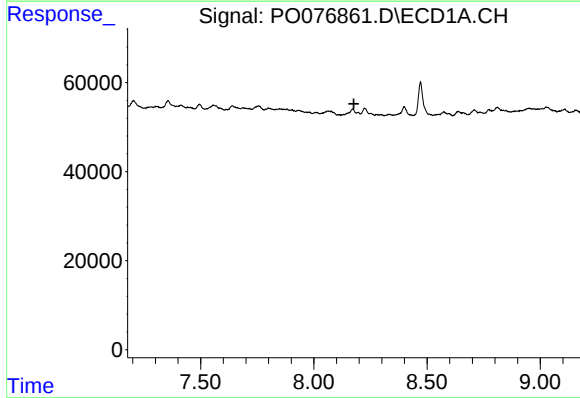


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.176 min
Response: 0
Conc: N.D.

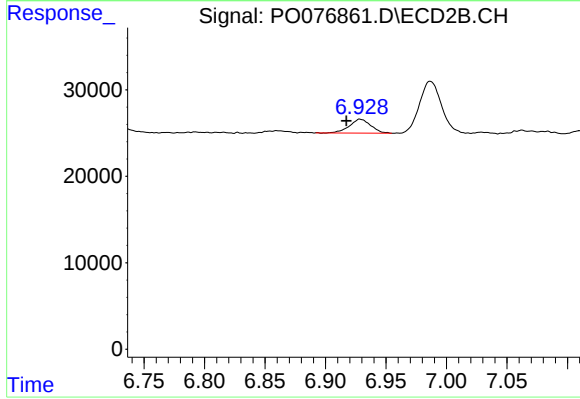

#32 AR-1260-2


R.T.: 6.928 min
Delta R.T.: 0.011 min
Response: 19691
Conc: 6.24 ng/ml

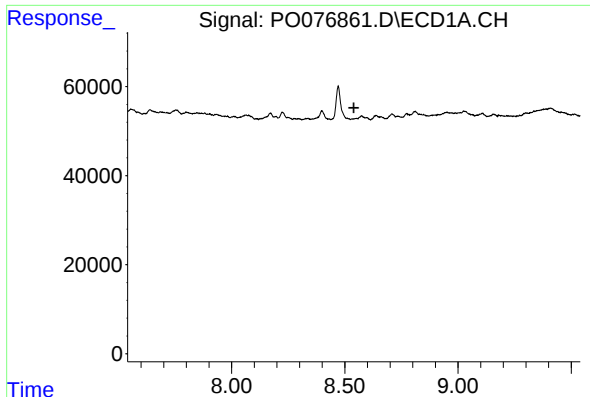

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 8.540 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

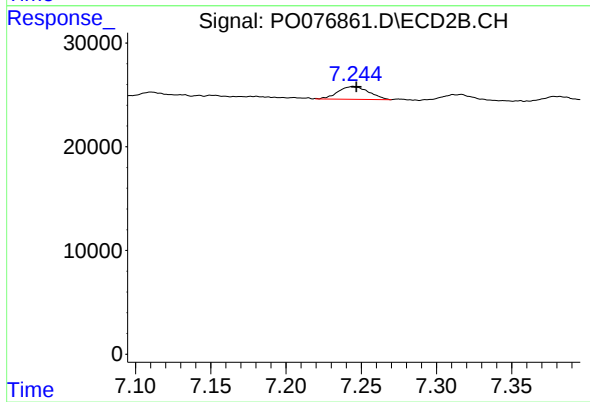

#36 AR-1262-1

R.T.: 7.245 min
Delta R.T.: -0.002 min
Response: 17707
Conc: 10.00 ng/ml