

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040723\
 Data File : P0093996.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2023 10:45
 Operator : YP/AJ
 Sample : 02213-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT2-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 13:35:26 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.419	3.624	71752282	26548108	19.194	20.848
2) SA Decachlor...	10.240	8.641	55262177	25214516	24.705	25.220
Target Compounds						
8) L2 AR-1221-1	4.627	3.836	1175348	420224	25.485	26.836
9) L2 AR-1221-2	4.723	3.922	1601423	626188	46.653	53.056
10) L2 AR-1221-3	4.792	3.998	2807307	1027644	26.804	27.896



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040723\
Data File : PO093996.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2023 10:45
Operator : YP/AJ
Sample : 02213-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 59 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 13:35:26 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

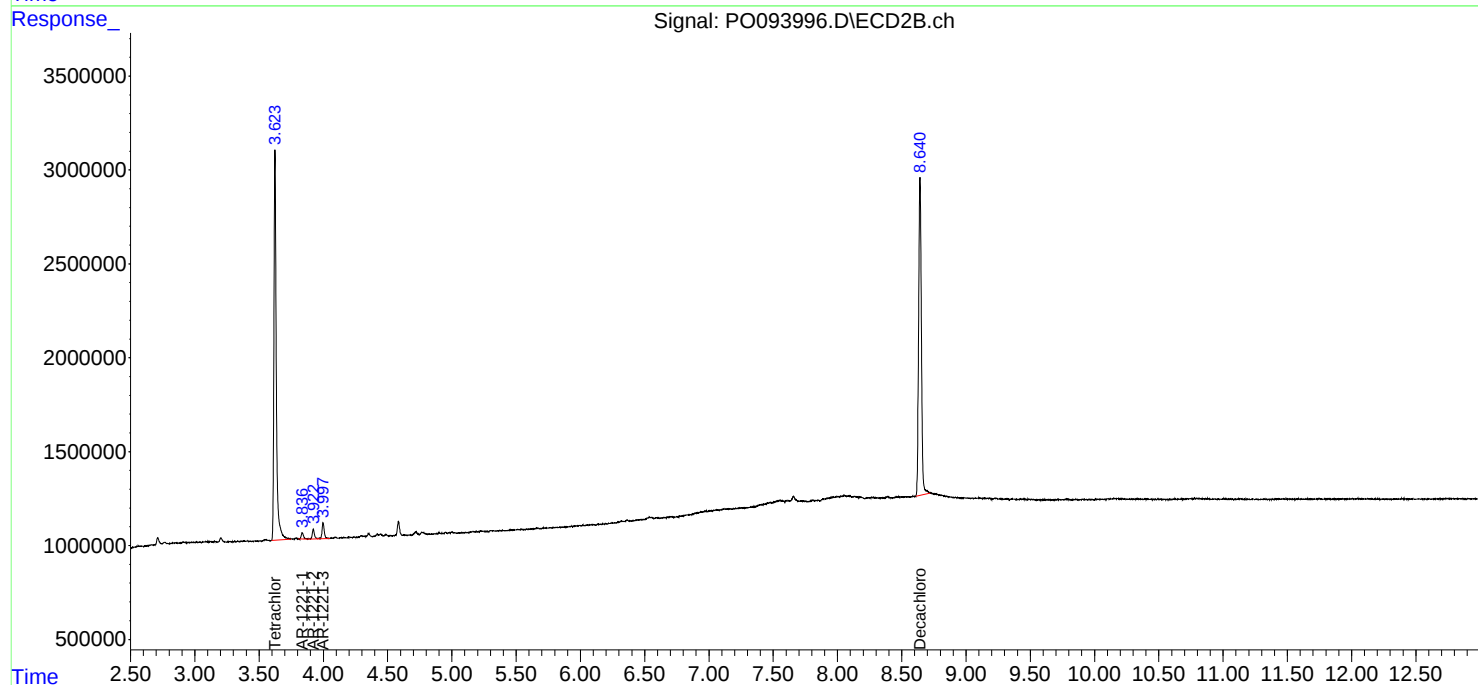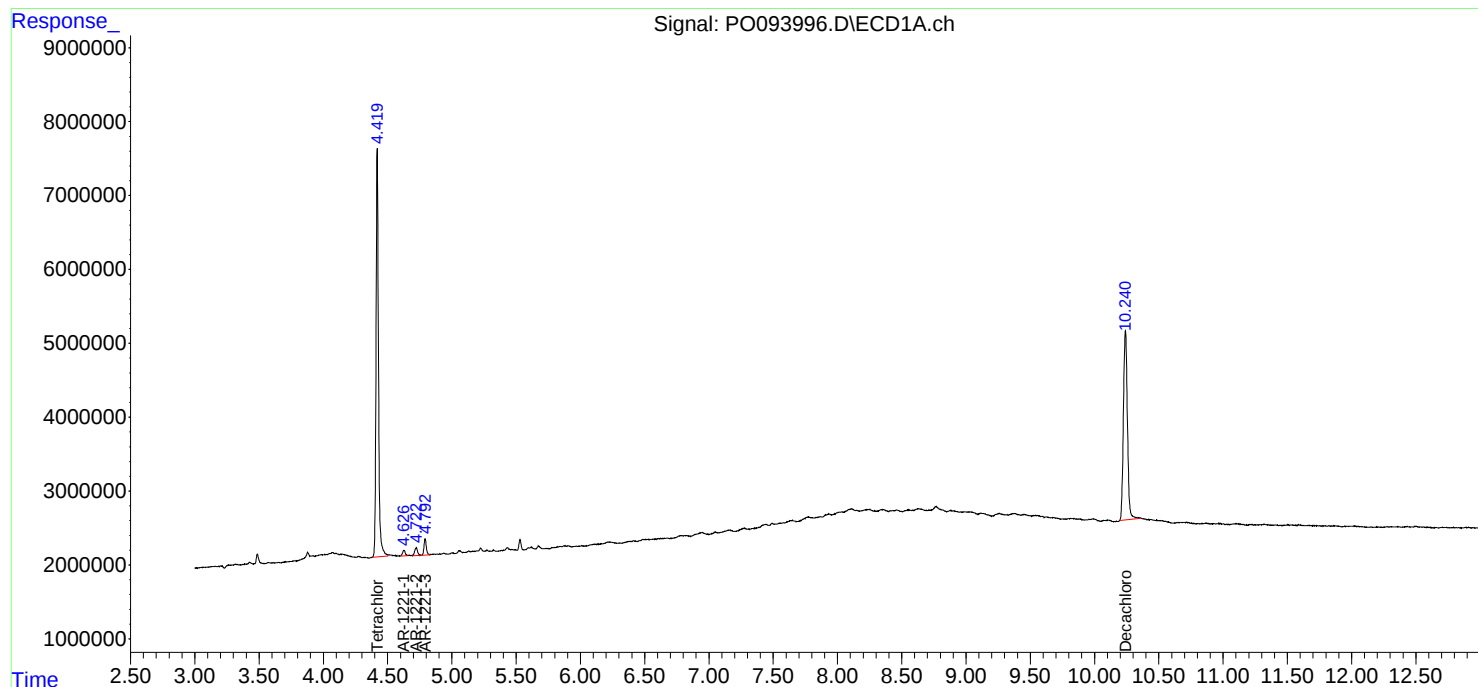


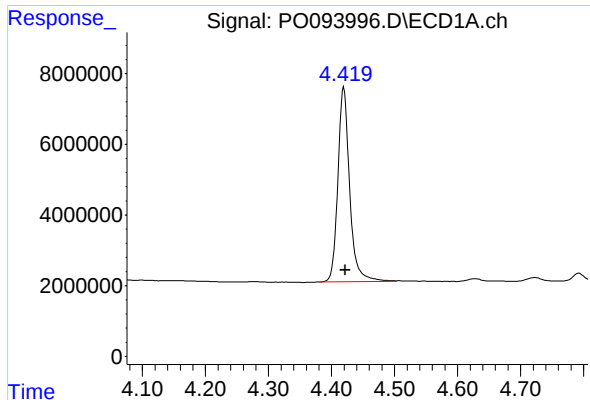

#1 Tetrachloro-m-xylene


R.T.: 4.419 min
Delta R.T.: -0.003 min
Response: 71752282
Conc: 19.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

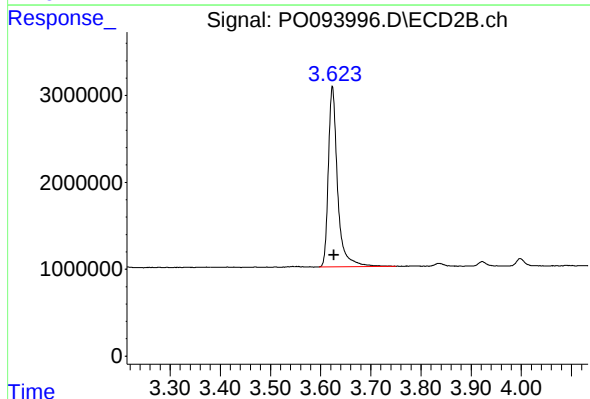


#1 Tetrachloro-m-xylene

R.T.: 3.624 min
Delta R.T.: -0.003 min
Response: 26548108
Conc: 20.85 ng/ml

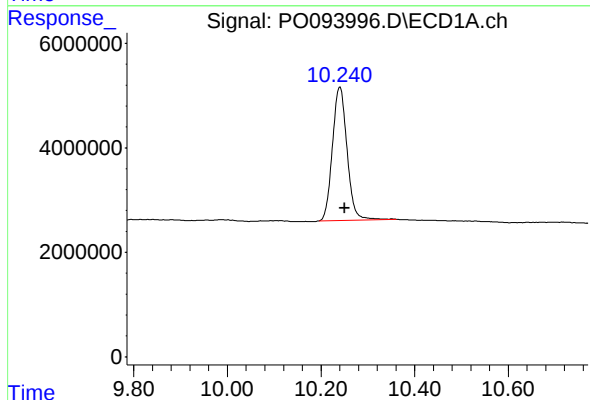


#2 Decachlorobiphenyl

R.T.: 10.240 min
Delta R.T.: -0.011 min
Response: 55262177
Conc: 24.70 ng/ml

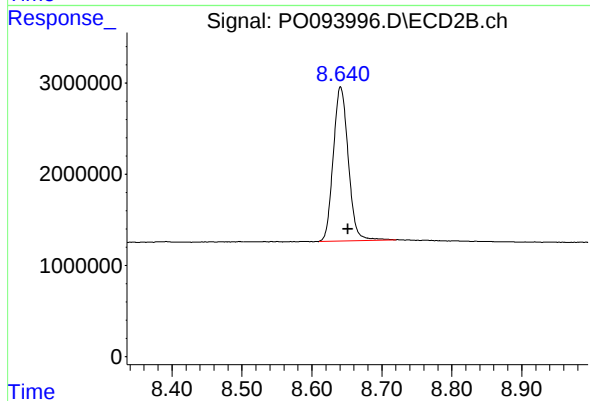

#2 Decachlorobiphenyl


R.T.: 8.641 min
Delta R.T.: -0.010 min
Response: 25214516
Conc: 25.22 ng/ml

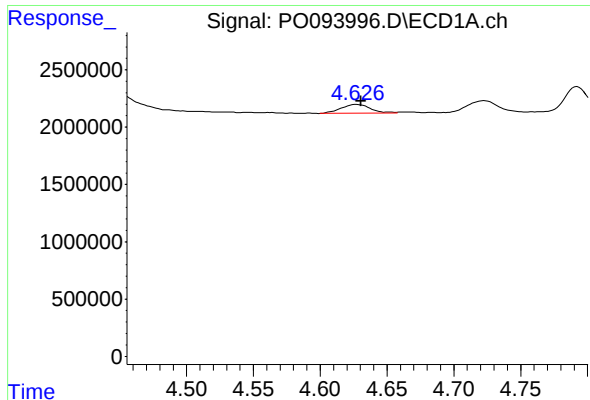

#8 AR-1221-1


R.T.: 4.627 min
Delta R.T.: -0.004 min
Response: 1175348
Conc: 25.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

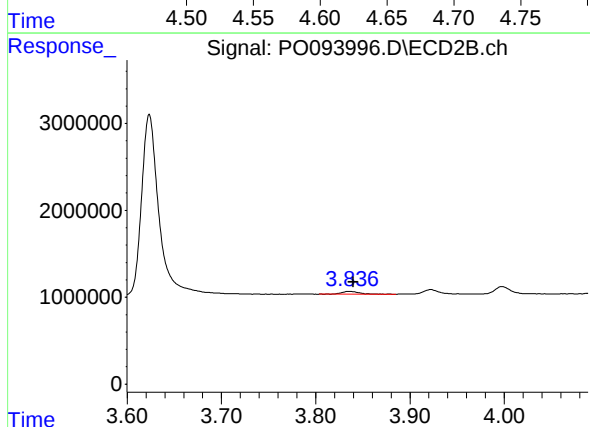


#8 AR-1221-1

R.T.: 3.836 min
Delta R.T.: -0.004 min
Response: 420224
Conc: 26.84 ng/ml

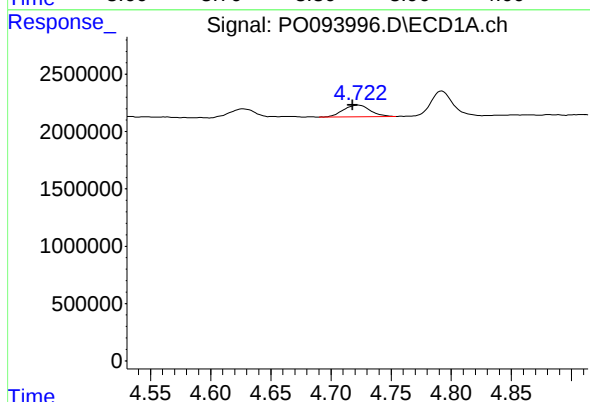


#9 AR-1221-2

R.T.: 4.723 min
Delta R.T.: 0.005 min
Response: 1601423
Conc: 46.65 ng/ml

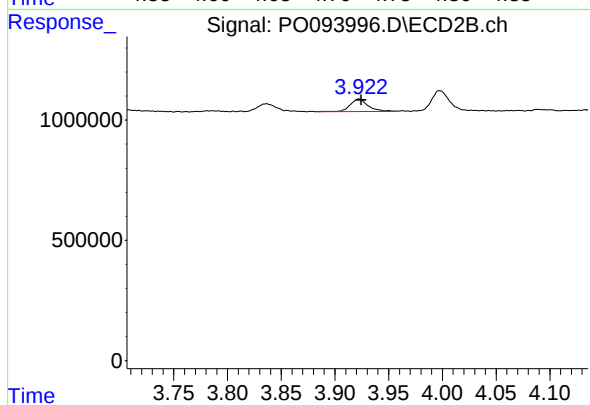

#9 AR-1221-2


R.T.: 3.922 min
Delta R.T.: -0.002 min
Response: 626188
Conc: 53.06 ng/ml

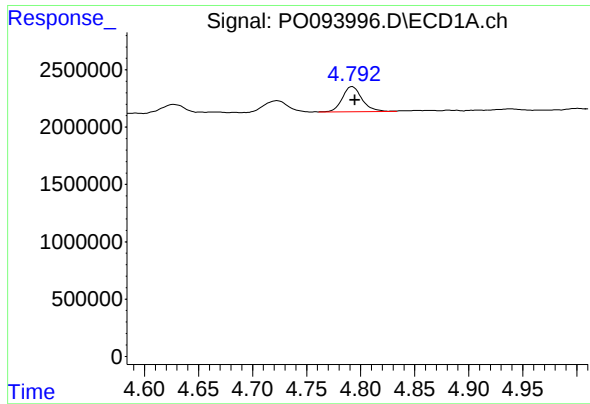

#10 AR-1221-3

R.T.: 4.792 min
Delta R.T.: -0.002 min
Response: 2807307
Conc: 26.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

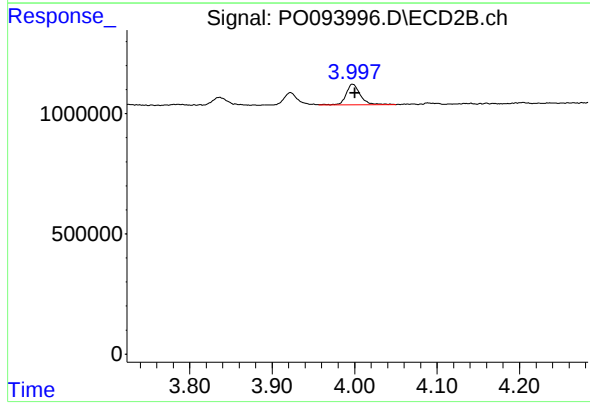

#10 AR-1221-3

R.T.: 3.998 min
Delta R.T.: -0.003 min
Response: 1027644
Conc: 27.90 ng/ml