

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040723\
 Data File : P0093997.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2023 11:02
 Operator : YP/AJ
 Sample : 02213-09
 Misc : AR1232 MDL 25 PPB
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT2-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 13:36:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.419	3.624	72169058	26560752	19.306	20.858
2) SA Decachlor...	10.239	8.640	54578520	25281742	24.399	25.287
Target Compounds						
11) L3 AR-1232-1	4.792	3.998	2353405	874660	26.965	27.997
12) L3 AR-1232-2	5.324	4.724	1087659	749890	25.433	28.326
13) L3 AR-1232-3	5.617	4.900	2052123	305844	27.937	23.189
14) L3 AR-1232-4	5.779	4.985	764439	301838	22.208	21.240
15) L3 AR-1232-5	5.872	5.157	870377	542238	27.403	35.100 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040723\
Data File : PO093997.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2023 11:02
Operator : YP/AJ
Sample : 02213-09
Misc : AR1232 MDL 25 PPB
ALS Vial : 60 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 13:36:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

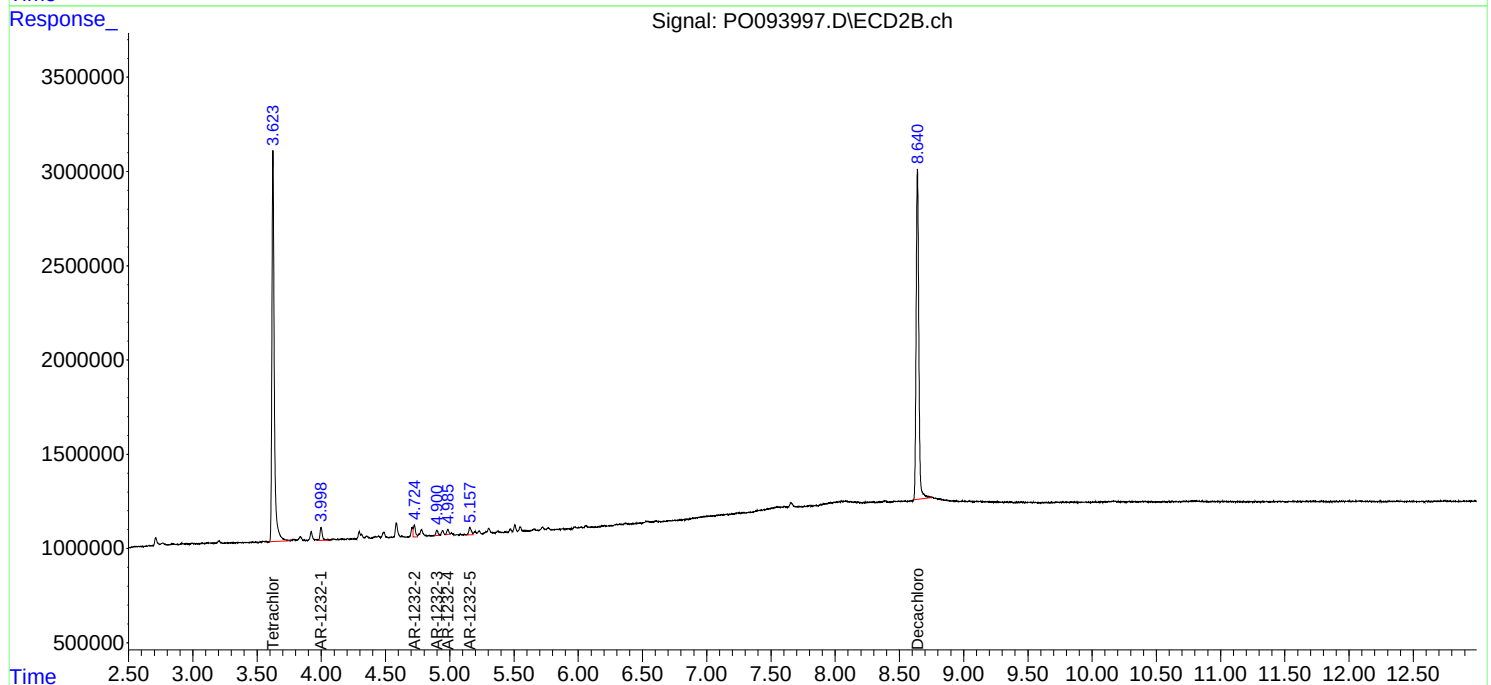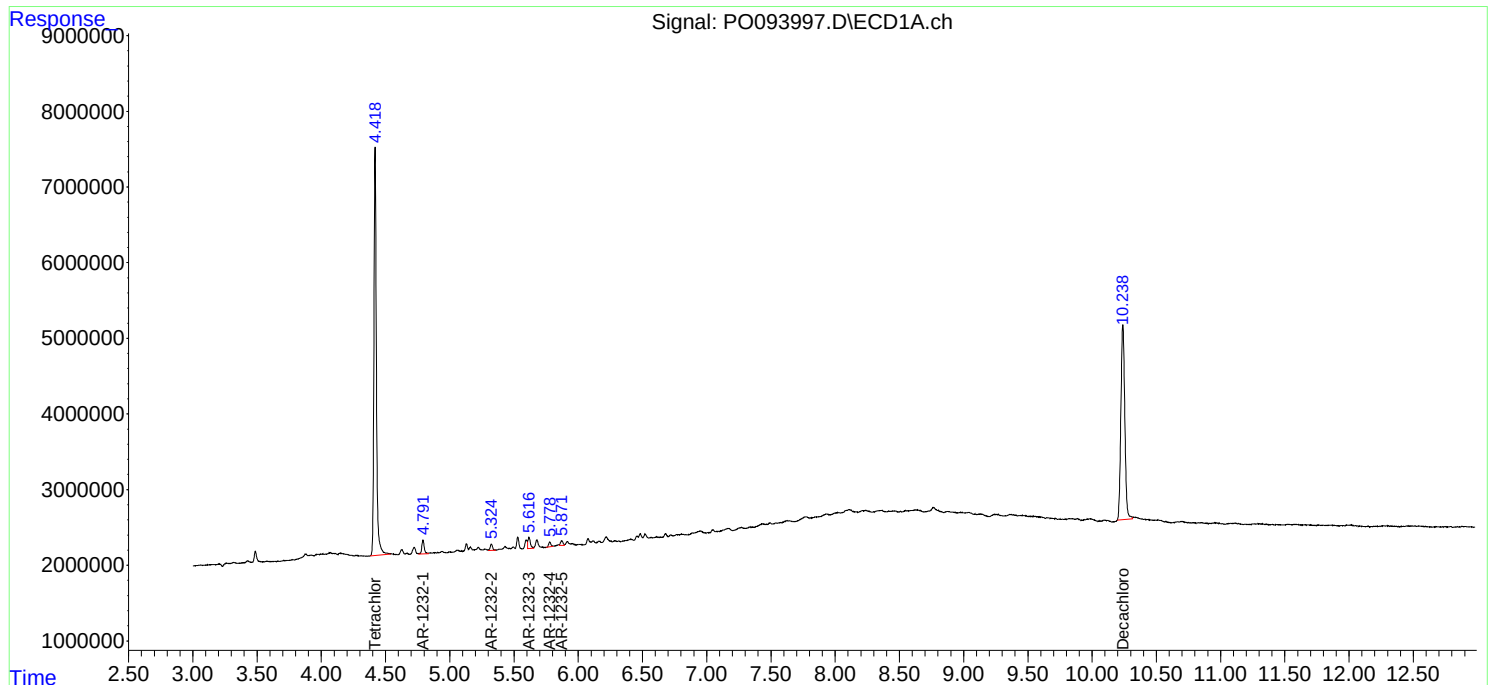


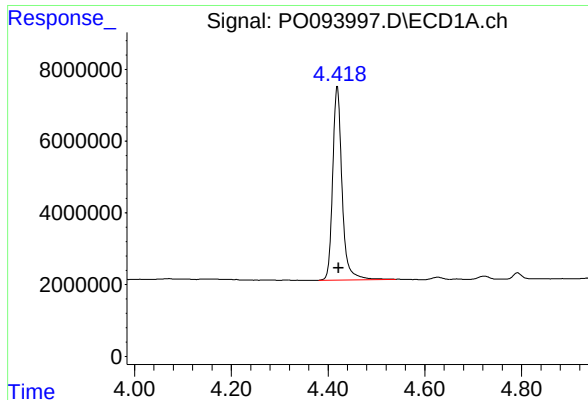

#1 Tetrachloro-m-xylene


R.T.: 4.419 min
Delta R.T.: -0.003 min
Response: 72169058
Conc: 19.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

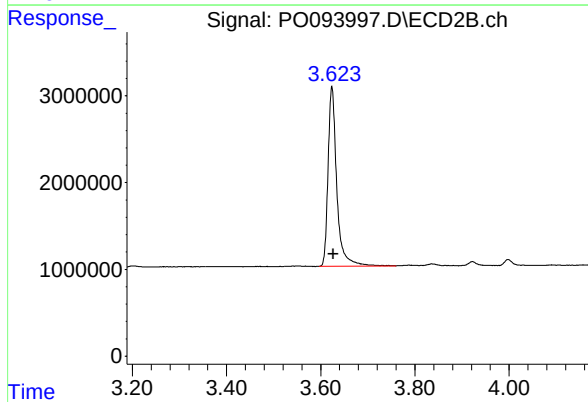


#1 Tetrachloro-m-xylene

R.T.: 3.624 min
Delta R.T.: -0.003 min
Response: 26560752
Conc: 20.86 ng/ml

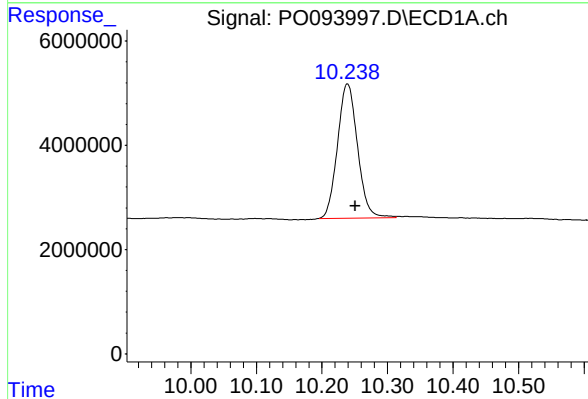


#2 Decachlorobiphenyl

R.T.: 10.239 min
Delta R.T.: -0.012 min
Response: 54578520
Conc: 24.40 ng/ml

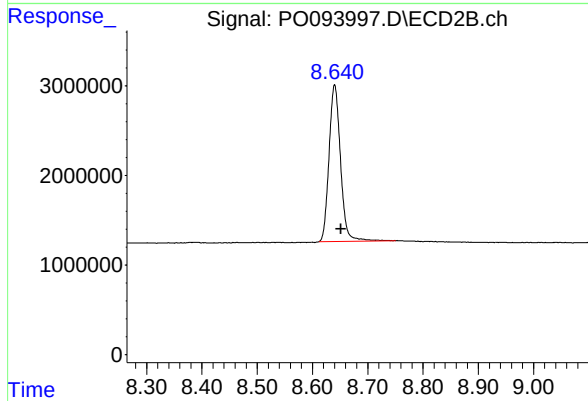

#2 Decachlorobiphenyl


R.T.: 8.640 min
Delta R.T.: -0.011 min
Response: 25281742
Conc: 25.29 ng/ml

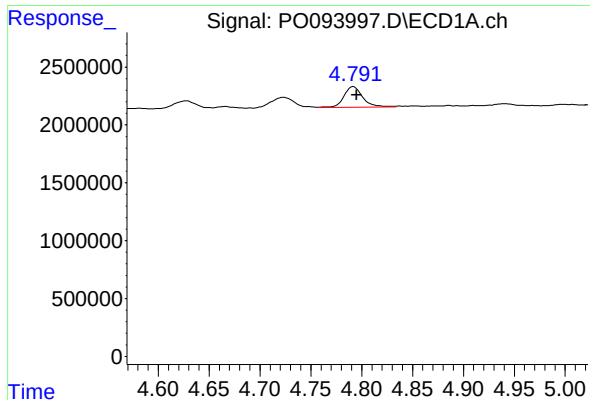

#11 AR-1232-1


R.T.: 4.792 min
Delta R.T.: -0.003 min
Response: 2353405
Conc: 26.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

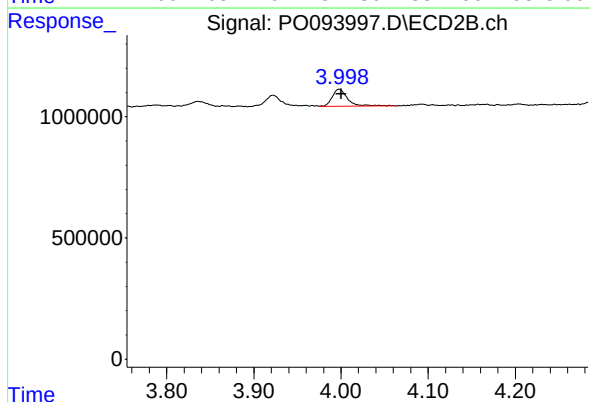


#11 AR-1232-1

R.T.: 3.998 min
Delta R.T.: -0.002 min
Response: 874660
Conc: 28.00 ng/ml

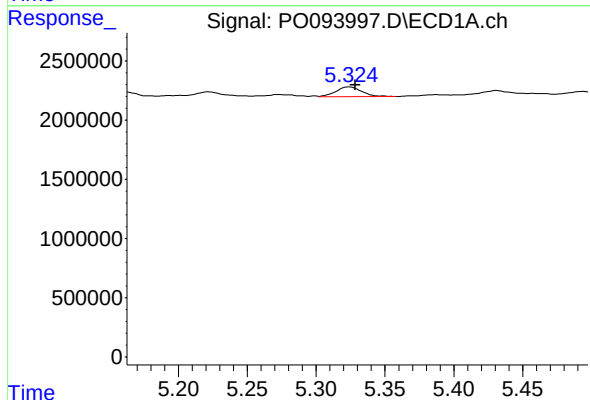


#12 AR-1232-2

R.T.: 5.324 min
Delta R.T.: -0.005 min
Response: 1087659
Conc: 25.43 ng/ml

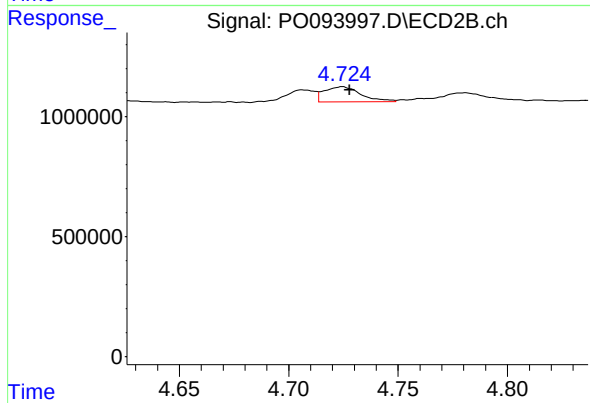

#12 AR-1232-2


R.T.: 4.724 min
Delta R.T.: -0.004 min
Response: 749890
Conc: 28.33 ng/ml

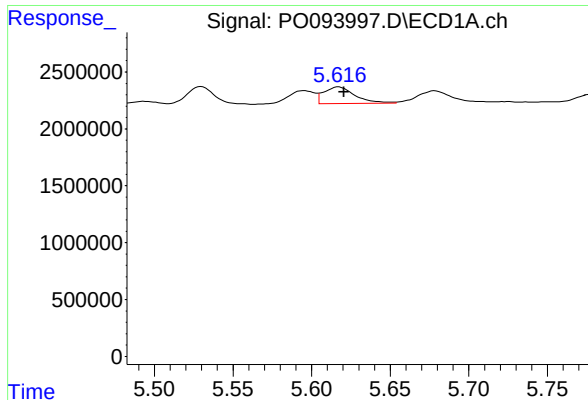

#13 AR-1232-3


R.T.: 5.617 min
Delta R.T.: -0.004 min
Response: 2052123
Conc: 27.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

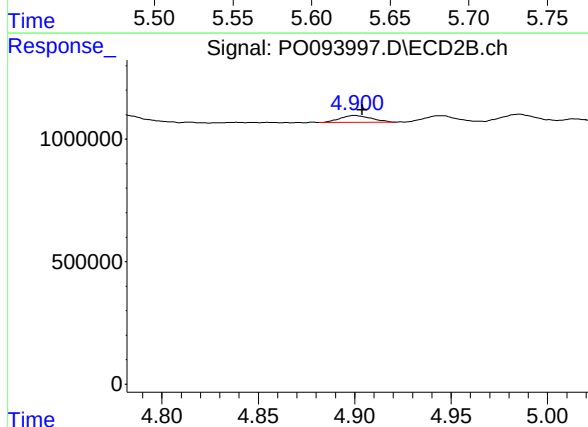


#13 AR-1232-3

R.T.: 4.900 min
Delta R.T.: -0.004 min
Response: 305844
Conc: 23.19 ng/ml

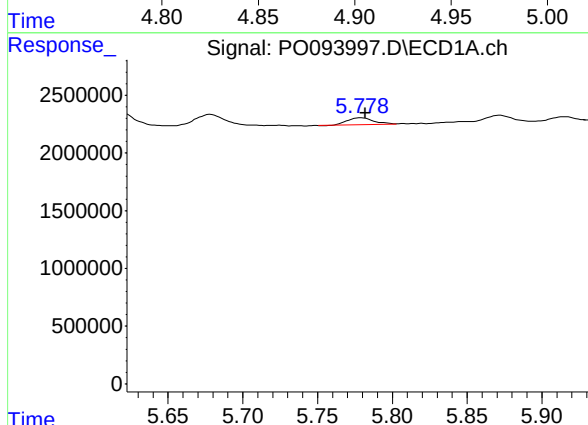


#14 AR-1232-4

R.T.: 5.779 min
Delta R.T.: -0.003 min
Response: 764439
Conc: 22.21 ng/ml

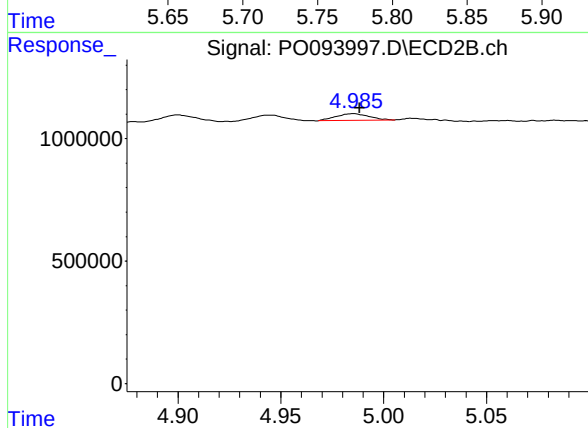

#14 AR-1232-4


R.T.: 4.985 min
Delta R.T.: -0.003 min
Response: 301838
Conc: 21.24 ng/ml

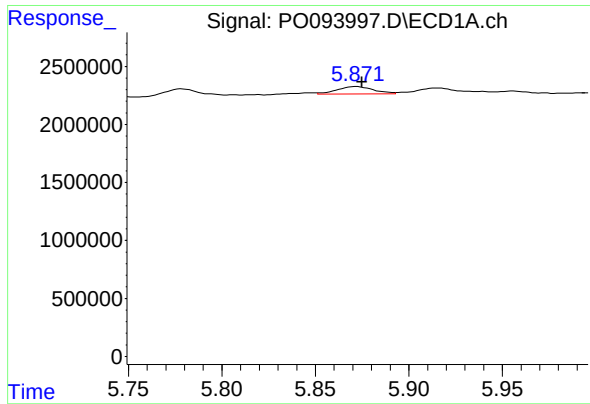

#15 AR-1232-5

R.T.: 5.872 min
Delta R.T.: -0.003 min
Response: 870377
Conc: 27.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

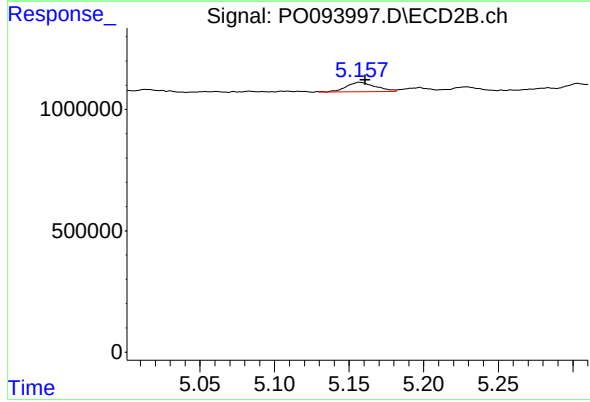

#15 AR-1232-5

R.T.: 5.157 min
Delta R.T.: -0.004 min
Response: 542238
Conc: 35.10 ng/ml