

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040723\
 Data File : P0093999.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2023 11:37
 Operator : YP/AJ
 Sample : 02213-09
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT2-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 13:38:03 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.418	3.622	74242471	27124512	19.860	21.301
2) SA Decachlor...	10.235	8.638	56005959	25392766	25.037	25.398
Target Compounds						
21) L5 AR-1248-1	5.593	4.705	1970659	682972	29.289	28.634
22) L5 AR-1248-2	5.869	4.941	3167545	1187728	28.957	29.818
23) L5 AR-1248-3	6.074	4.983	3612955	1251552	29.928	29.985
24) L5 AR-1248-4	6.481	5.154	3280042	1473695	30.541	31.339
25) L5 AR-1248-5	6.520	5.547	3304894	895666	28.485	23.991



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040723\
Data File : PO093999.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2023 11:37
Operator : YP/AJ
Sample : 02213-09
Misc : AR1248 MDL 25 PPB
ALS Vial : 62 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 13:38:03 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

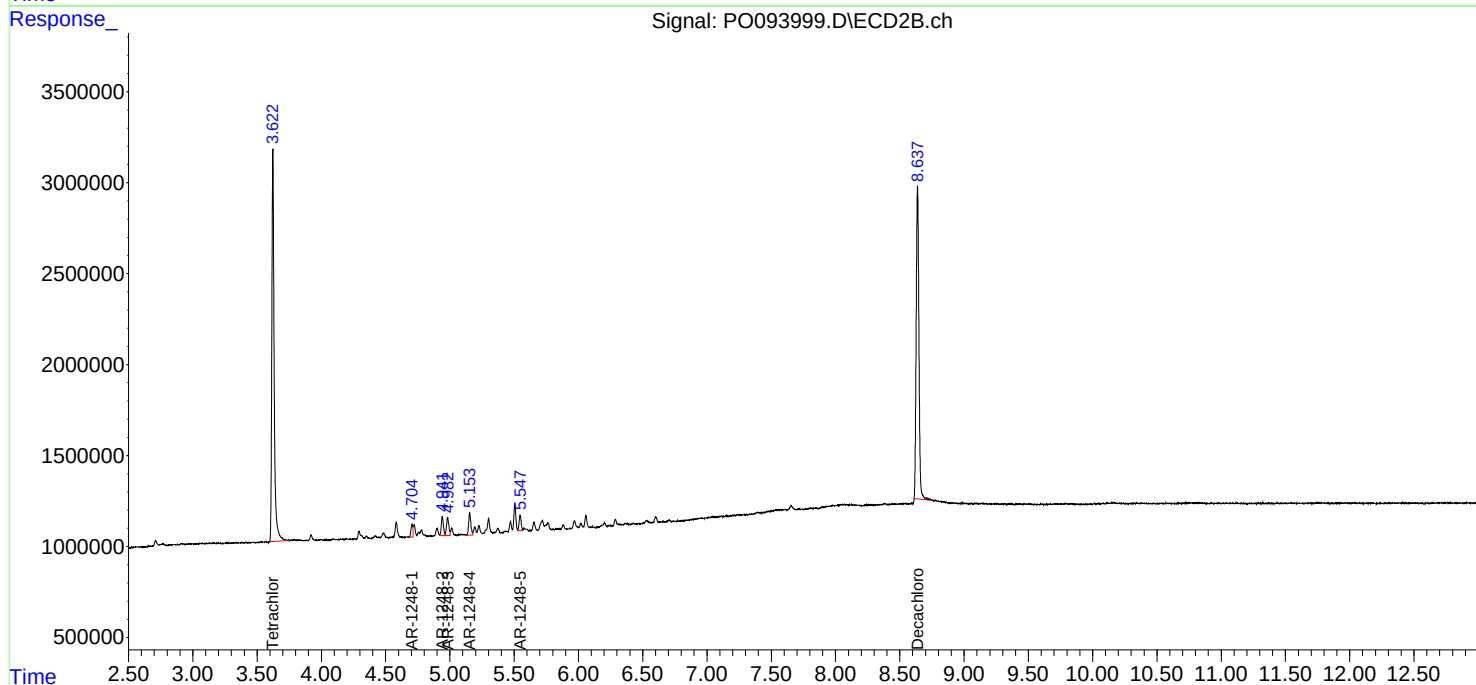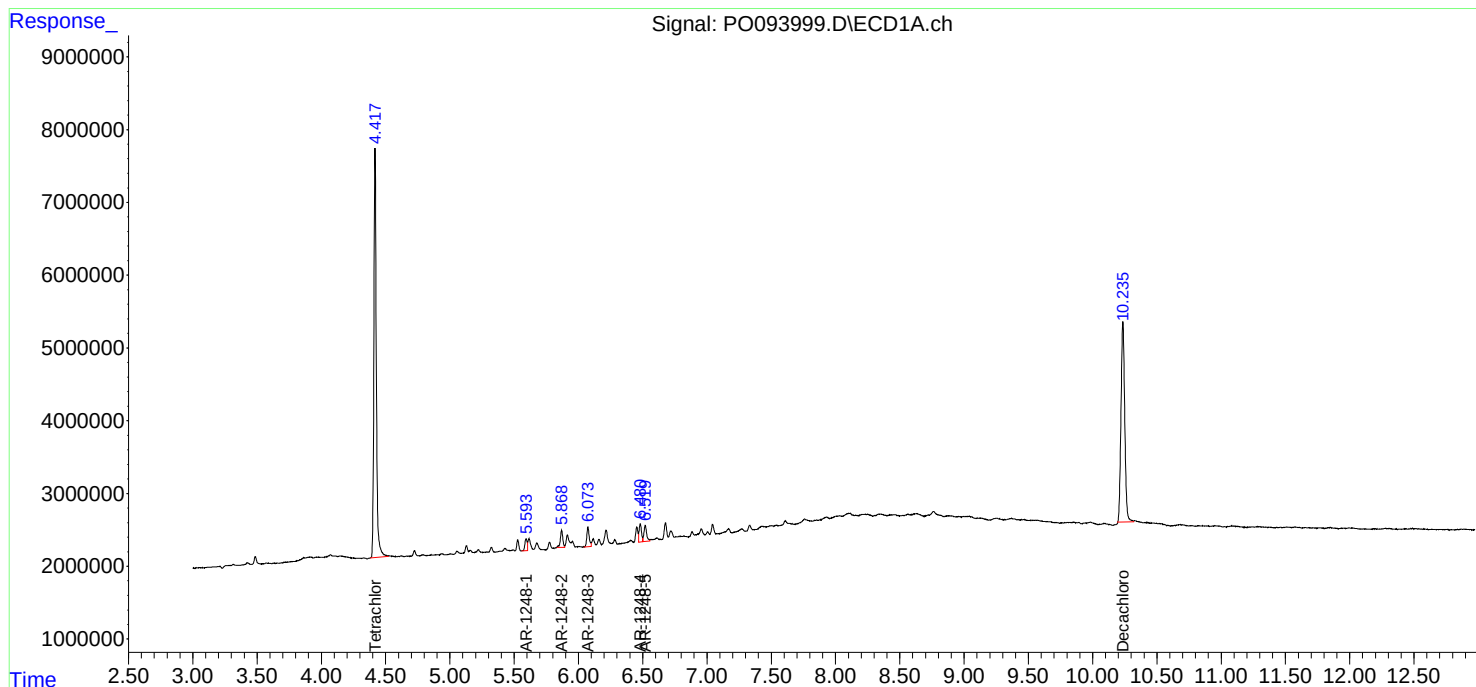


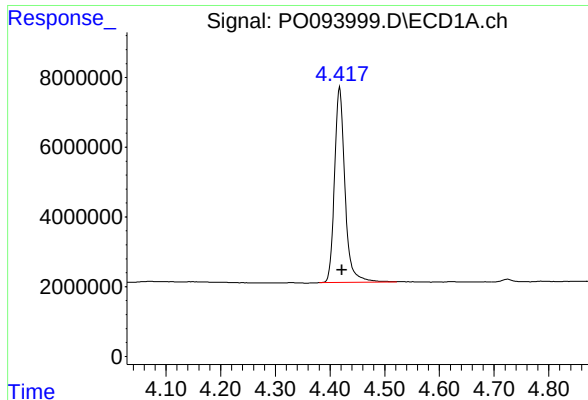

#1 Tetrachloro-m-xylene


R.T.: 4.418 min
Delta R.T.: -0.004 min
Response: 74242471
Conc: 19.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

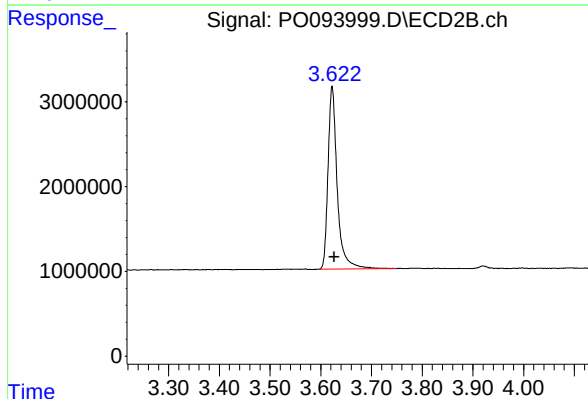


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.004 min
Response: 27124512
Conc: 21.30 ng/ml

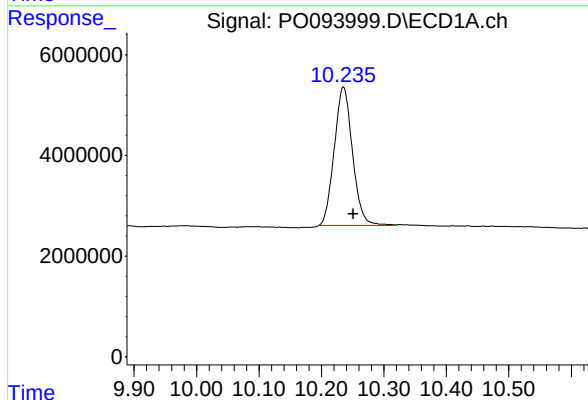


#2 Decachlorobiphenyl

R.T.: 10.235 min
Delta R.T.: -0.015 min
Response: 56005959
Conc: 25.04 ng/ml

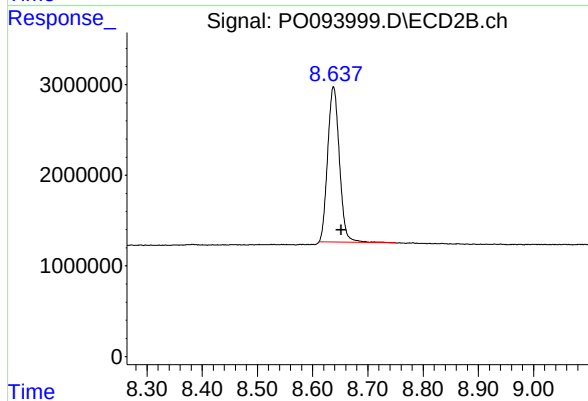

#2 Decachlorobiphenyl


R.T.: 8.638 min
Delta R.T.: -0.014 min
Response: 25392766
Conc: 25.40 ng/ml

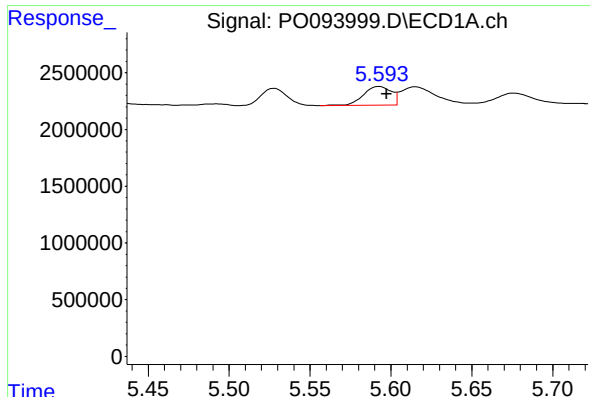

#21 AR-1248-1


R.T.: 5.593 min
Delta R.T.: -0.004 min
Response: 1970659
Conc: 29.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

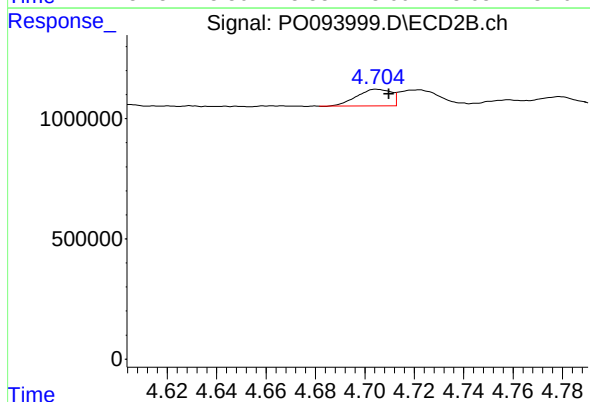


#21 AR-1248-1

R.T.: 4.705 min
Delta R.T.: -0.005 min
Response: 682972
Conc: 28.63 ng/ml

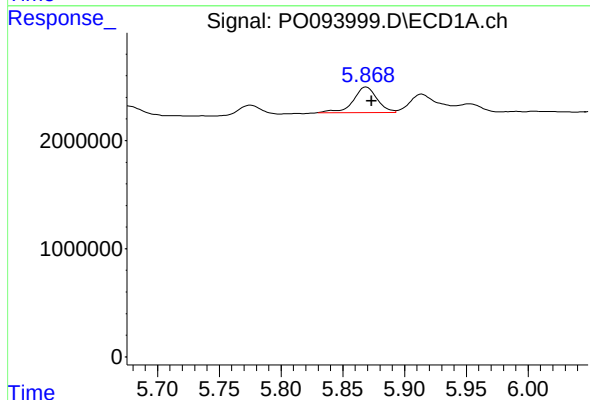


#22 AR-1248-2

R.T.: 5.869 min
Delta R.T.: -0.004 min
Response: 3167545
Conc: 28.96 ng/ml

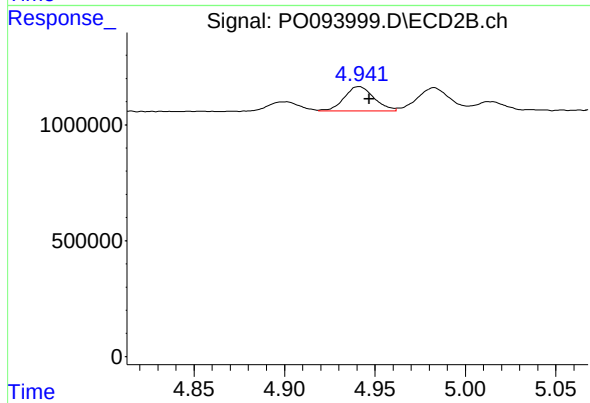

#22 AR-1248-2


R.T.: 4.941 min
Delta R.T.: -0.006 min
Response: 1187728
Conc: 29.82 ng/ml

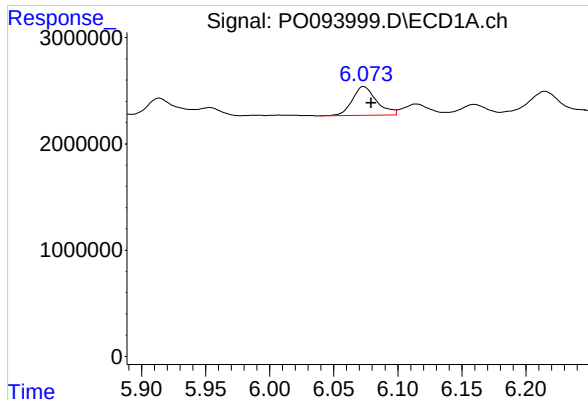

#23 AR-1248-3


R.T.: 6.074 min
Delta R.T.: -0.006 min
Response: 3612955
Conc: 29.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

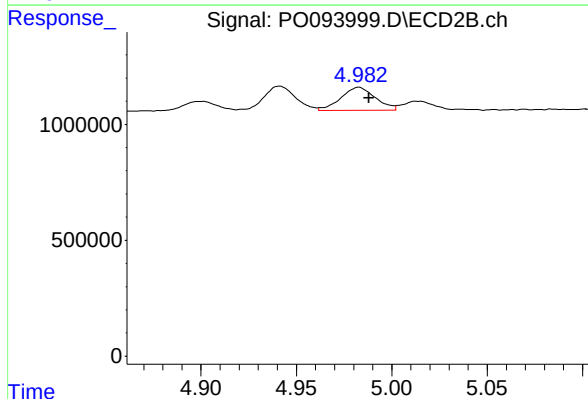


#23 AR-1248-3

R.T.: 4.983 min
Delta R.T.: -0.005 min
Response: 1251552
Conc: 29.99 ng/ml

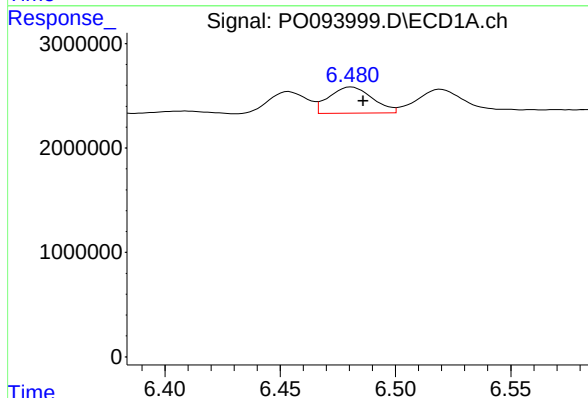


#24 AR-1248-4

R.T.: 6.481 min
Delta R.T.: -0.005 min
Response: 3280042
Conc: 30.54 ng/ml

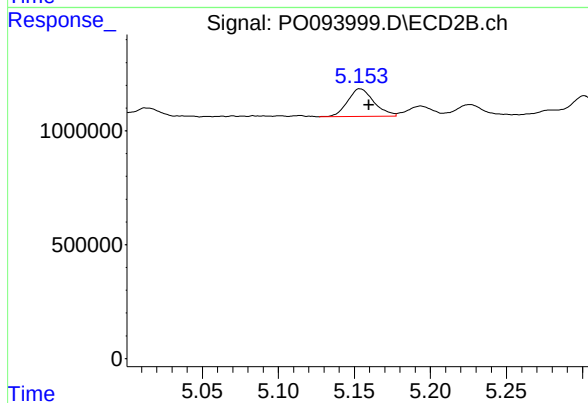

#24 AR-1248-4


R.T.: 5.154 min
Delta R.T.: -0.006 min
Response: 1473695
Conc: 31.34 ng/ml

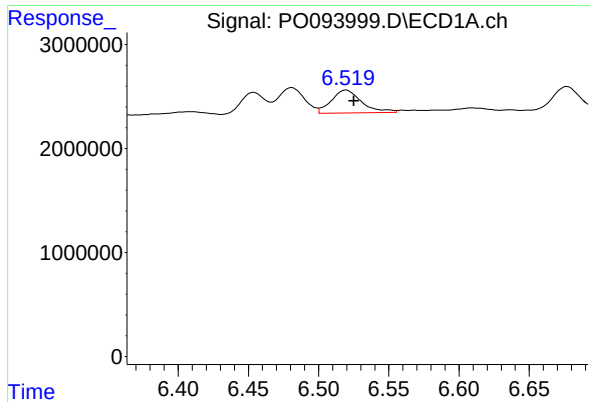

#25 AR-1248-5

R.T.: 6.520 min
Delta R.T.: -0.005 min
Response: 3304894
Conc: 28.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

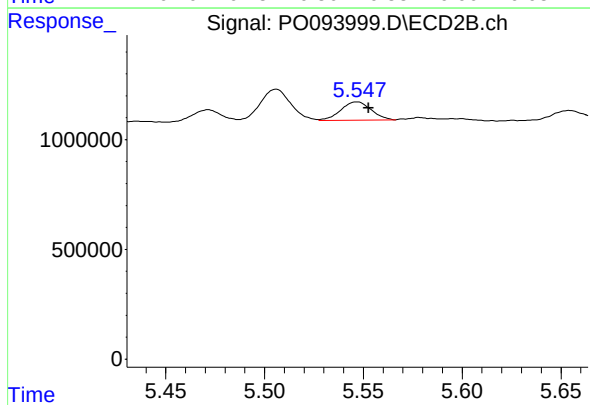

#25 AR-1248-5

R.T.: 5.547 min
Delta R.T.: -0.006 min
Response: 895666
Conc: 23.99 ng/ml