

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040723\
 Data File : P0094000.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2023 11:54
 Operator : YP/AJ
 Sample : 02213-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT2-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 13:39:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.417	3.622	73562829	26806528	19.679	21.051
2) SA Decachlor...	10.236	8.638	55007744	25210267	24.591	25.216
Target Compounds						
26) L6 AR-1254-1	6.454	5.506	4114807	2152018	30.339	31.484
27) L6 AR-1254-2	6.675	5.655	5970058	1983350	30.542	32.565
28) L6 AR-1254-3	7.044	6.058	5448028	2897803	29.490	31.813
29) L6 AR-1254-4	7.333	6.288	2993306	1393213	29.516	32.708
30) L6 AR-1254-5	7.755	6.706	4465737	2246593	32.932	31.136



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040723\
Data File : PO094000.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2023 11:54
Operator : YP/AJ
Sample : 02213-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 63 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 13:39:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

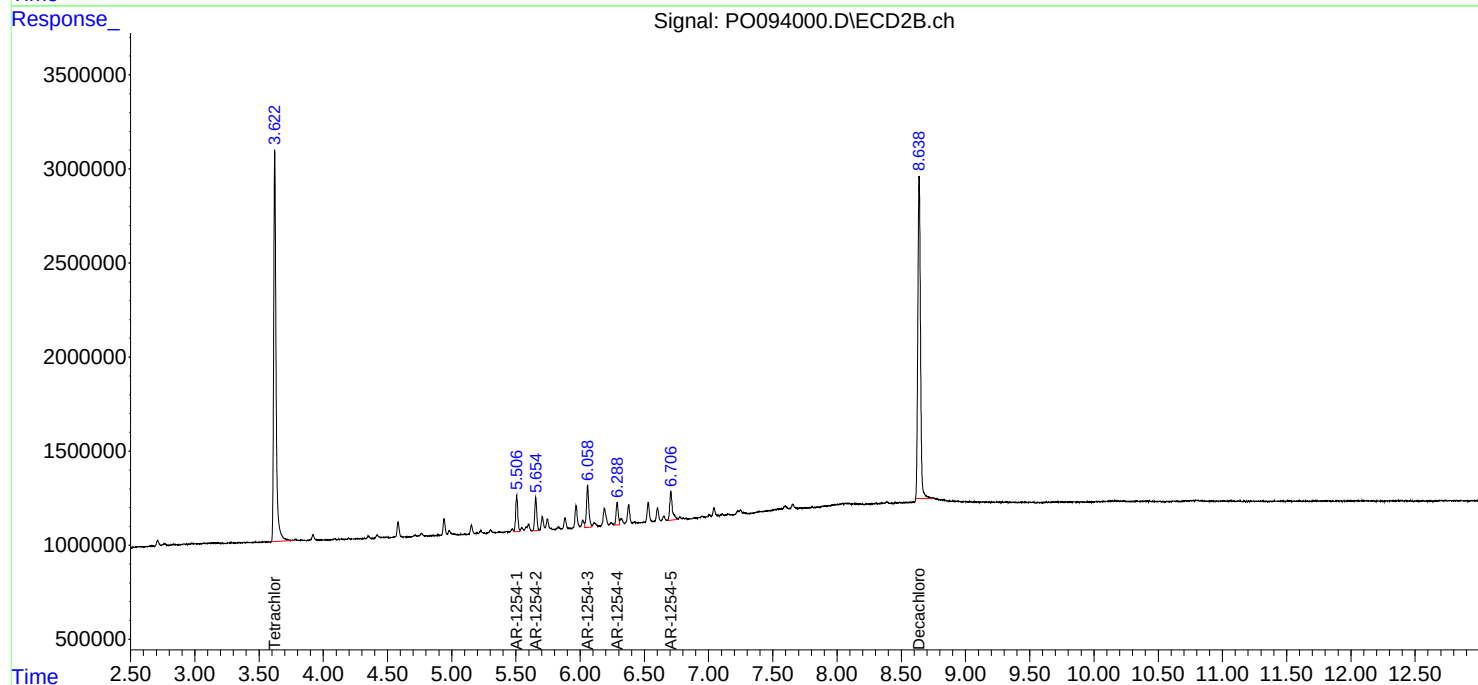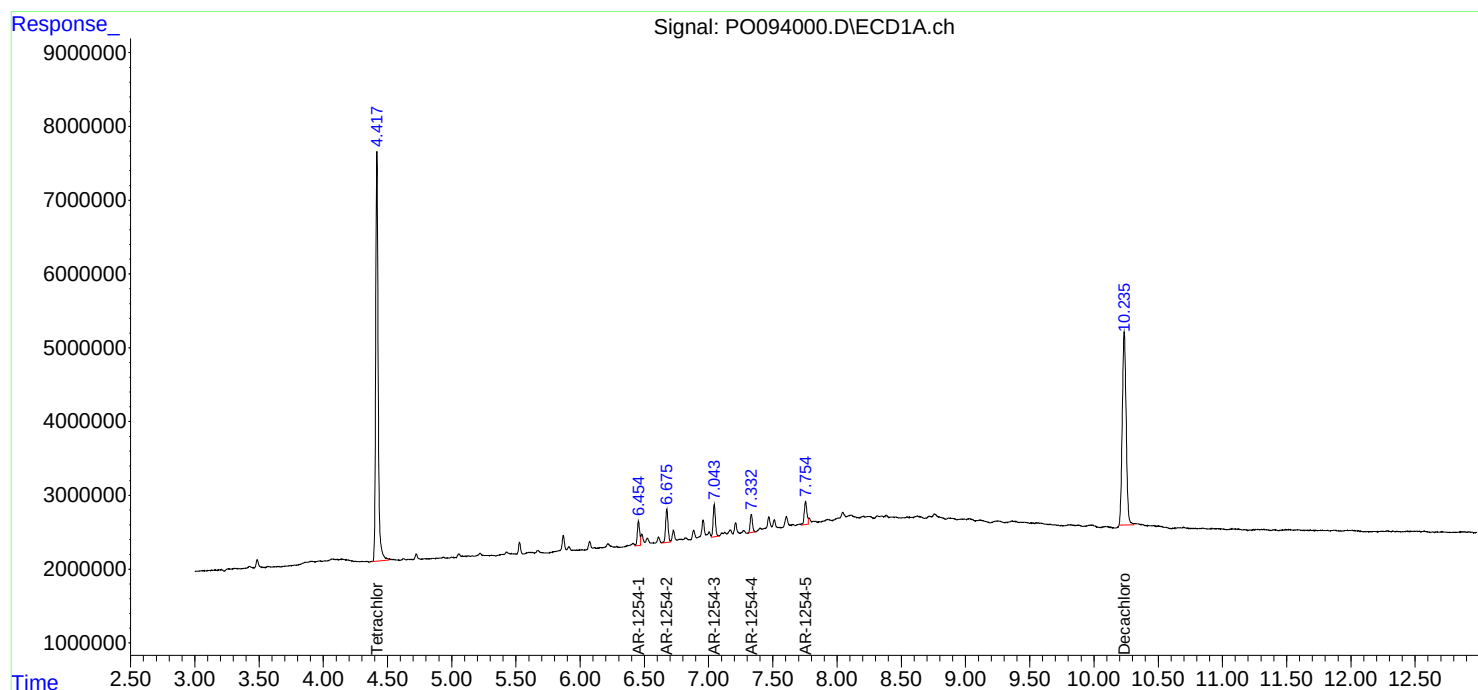


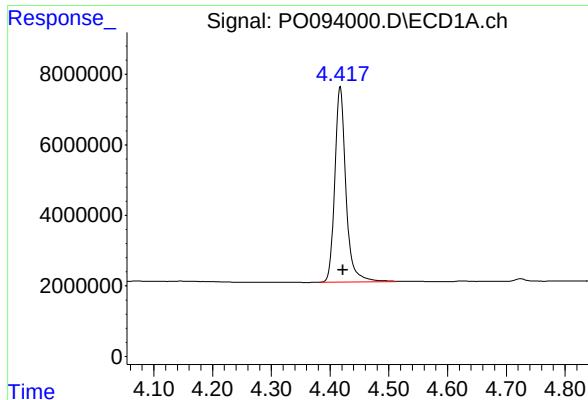

#1 Tetrachloro-m-xylene


R.T.: 4.417 min
Delta R.T.: -0.005 min
Response: 73562829
Conc: 19.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

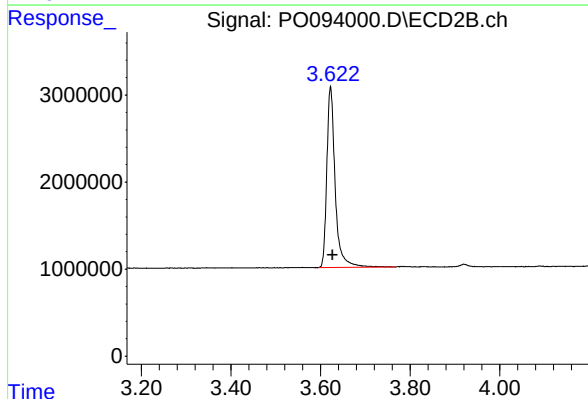


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.005 min
Response: 26806528
Conc: 21.05 ng/ml

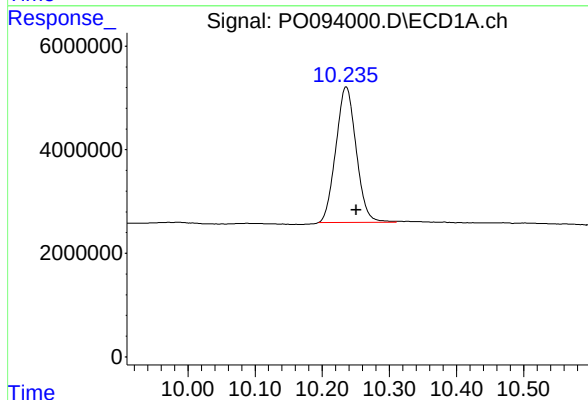


#2 Decachlorobiphenyl

R.T.: 10.236 min
Delta R.T.: -0.015 min
Response: 55007744
Conc: 24.59 ng/ml

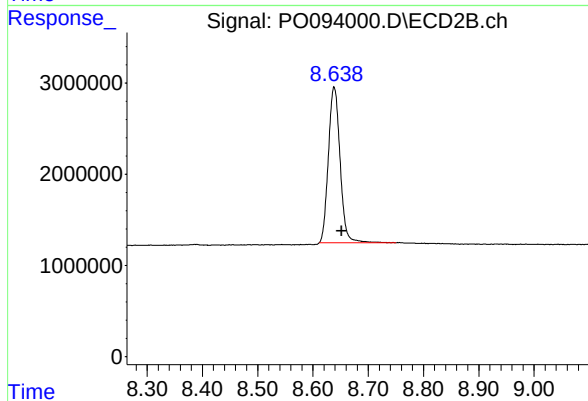

#2 Decachlorobiphenyl


R.T.: 8.638 min
Delta R.T.: -0.013 min
Response: 25210267
Conc: 25.22 ng/ml

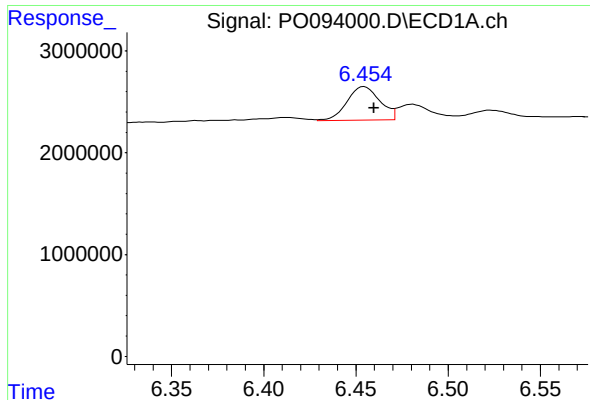

#26 AR-1254-1


R.T.: 6.454 min
Delta R.T.: -0.006 min
Response: 4114807
Conc: 30.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

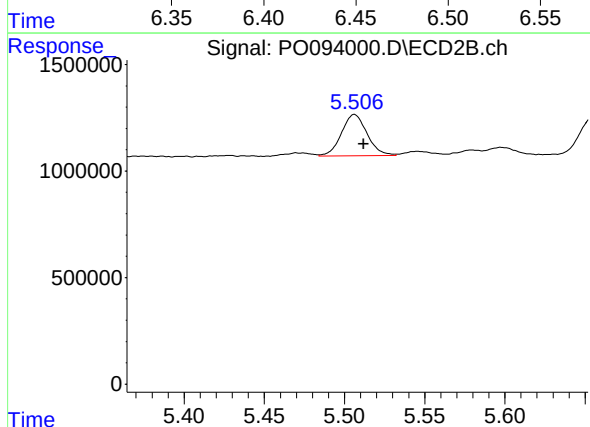


#26 AR-1254-1

R.T.: 5.506 min
Delta R.T.: -0.006 min
Response: 2152018
Conc: 31.48 ng/ml

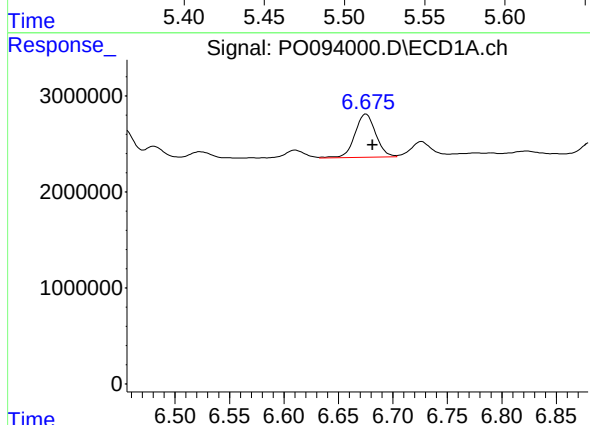


#27 AR-1254-2

R.T.: 6.675 min
Delta R.T.: -0.006 min
Response: 5970058
Conc: 30.54 ng/ml

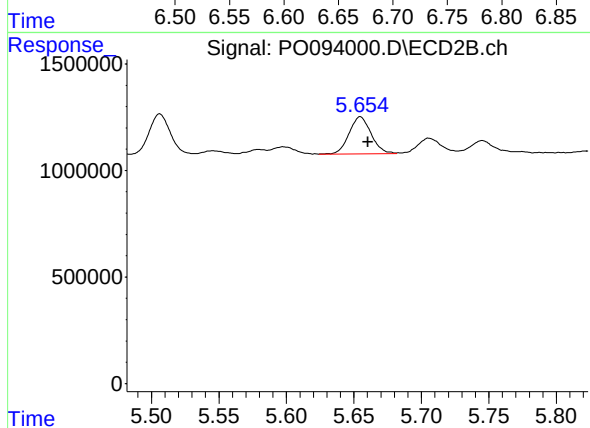

#27 AR-1254-2


R.T.: 5.655 min
Delta R.T.: -0.006 min
Response: 1983350
Conc: 32.56 ng/ml

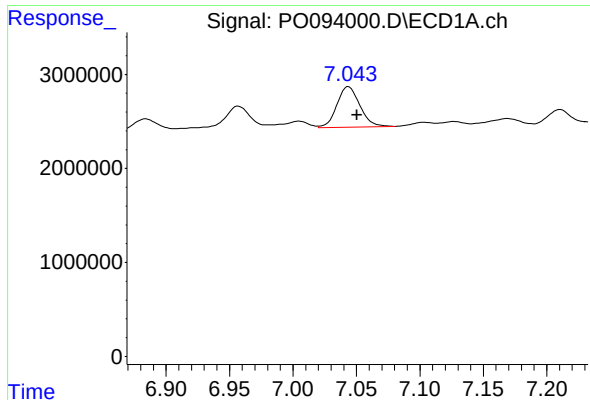

#28 AR-1254-3


R.T.: 7.044 min
Delta R.T.: -0.007 min
Response: 5448028
Conc: 29.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

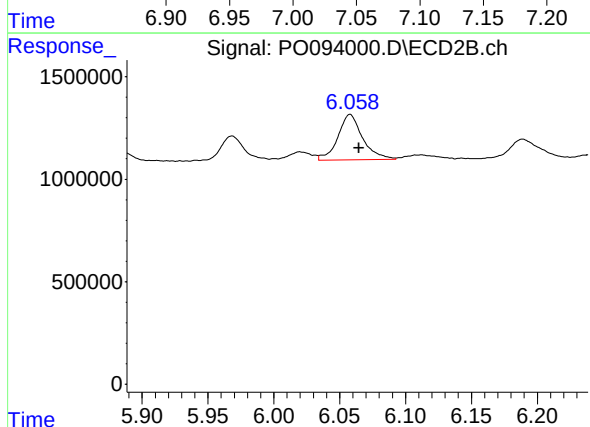


#28 AR-1254-3

R.T.: 6.058 min
Delta R.T.: -0.007 min
Response: 2897803
Conc: 31.81 ng/ml

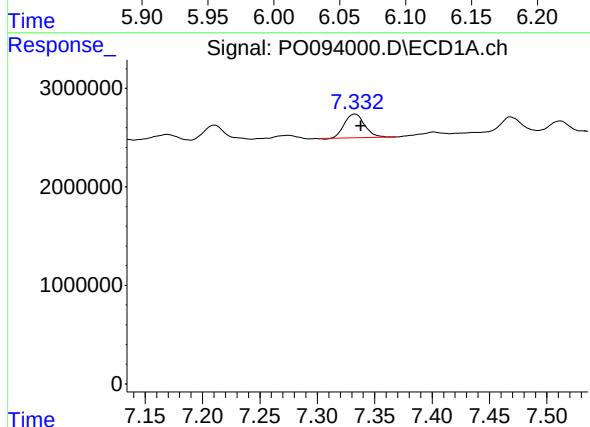


#29 AR-1254-4

R.T.: 7.333 min
Delta R.T.: -0.005 min
Response: 2993306
Conc: 29.52 ng/ml

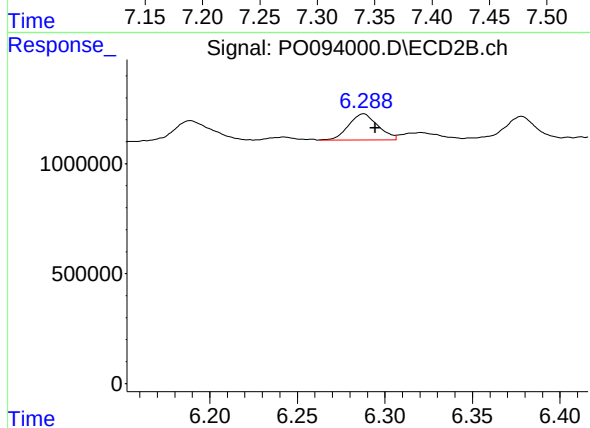

#29 AR-1254-4


R.T.: 6.288 min
Delta R.T.: -0.007 min
Response: 1393213
Conc: 32.71 ng/ml

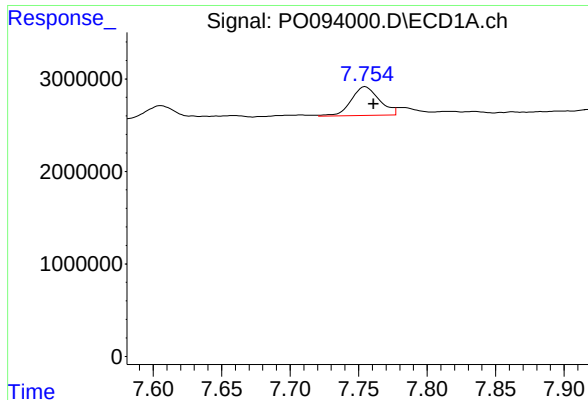

#30 AR-1254-5

R.T.: 7.755 min
Delta R.T.: -0.006 min
Response: 4465737
Conc: 32.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

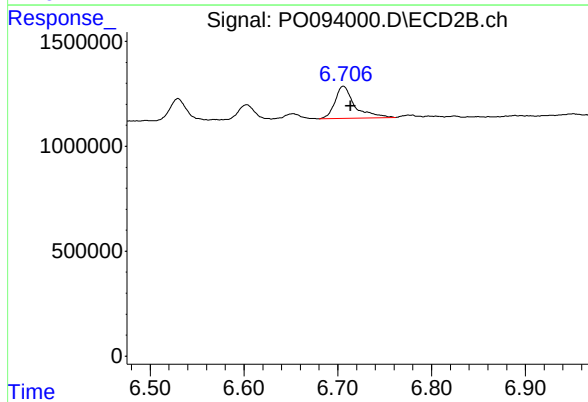

#30 AR-1254-5

R.T.: 6.706 min
Delta R.T.: -0.008 min
Response: 2246593
Conc: 31.14 ng/ml