

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040723\
 Data File : P0094001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2023 12:11
 Operator : YP/AJ
 Sample : 02213-09
 Misc : AR1262 MDL 25 PPB
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT2-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 13:40:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.417	3.622	74794204	27184588	20.008	21.348
2) SA Decachlor...	10.235	8.639	55144011	25523088	24.652	25.529
Target Compounds						
36) L8 AR-1262-1	7.832	6.797	5698830	1100190	33.361	31.445
37) L8 AR-1262-2	8.383	7.003	7709013	2462819	33.164m	34.858
38) L8 AR-1262-3	8.705	7.531	5790401	1770904	35.349	35.395m
39) L8 AR-1262-4	8.794	7.596	2784623	3085032	27.792	37.200 #
40) L8 AR-1262-5	9.464	8.094	3519811	1107753	43.732	34.053



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040723\
Data File : PO094001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2023 12:11
Operator : YP/AJ
Sample : 02213-09
Misc : AR1262 MDL 25 PPB
ALS Vial : 64 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 13:40:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

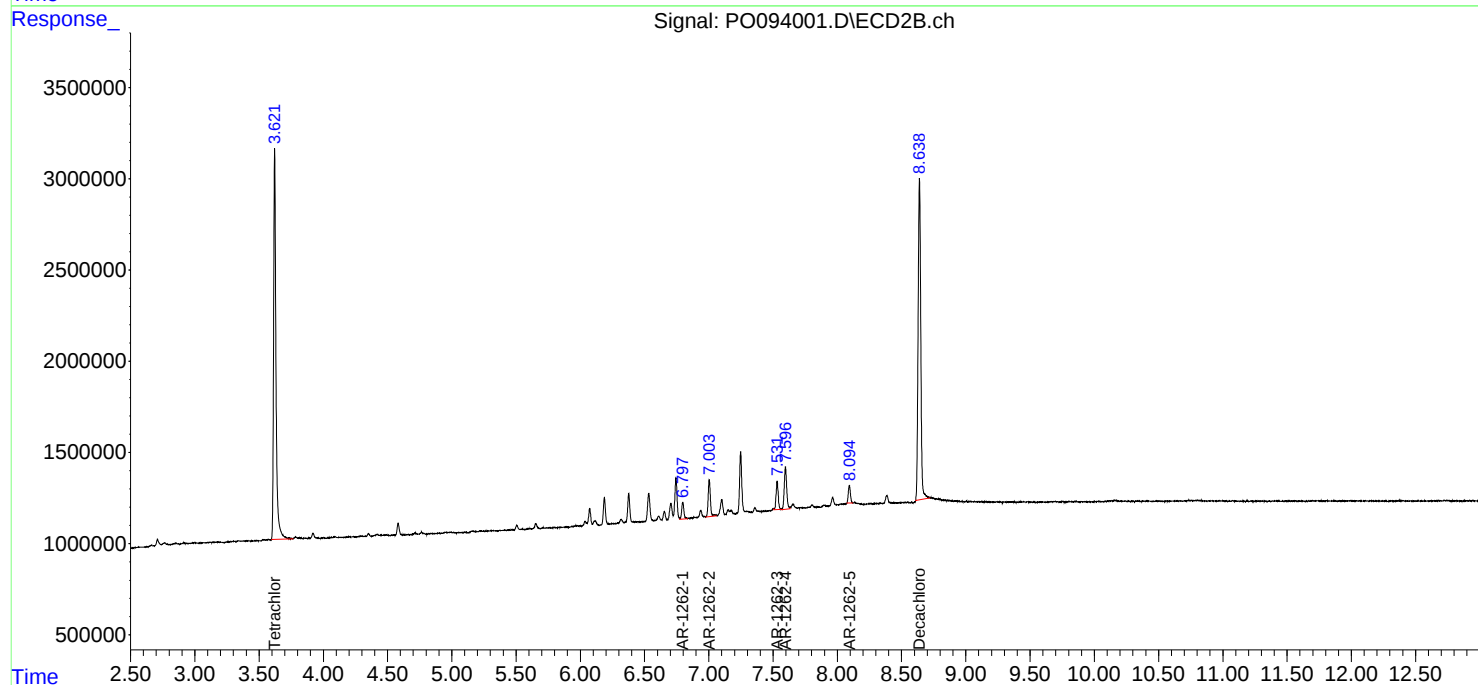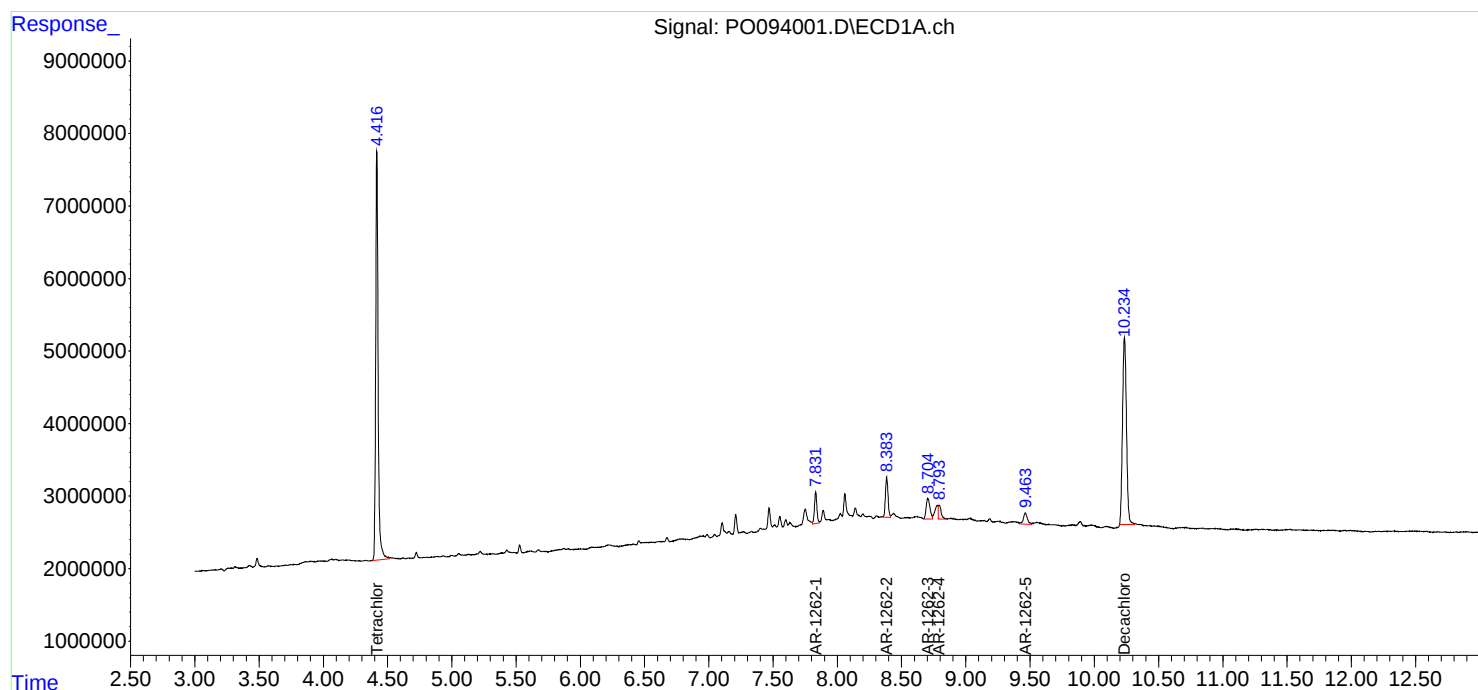


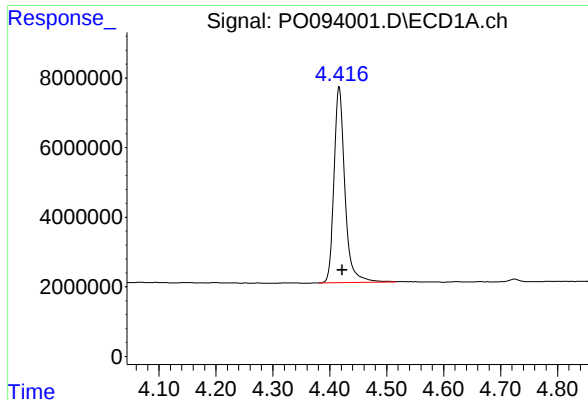

#1 Tetrachloro-m-xylene


R.T.: 4.417 min
Delta R.T.: -0.005 min
Response: 74794204
Conc: 20.01 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

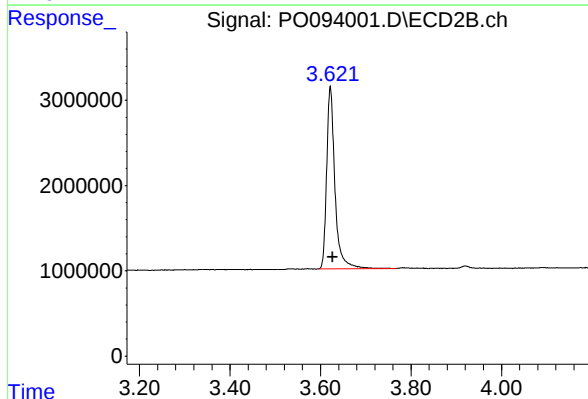


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.005 min
Response: 27184588
Conc: 21.35 ng/ml

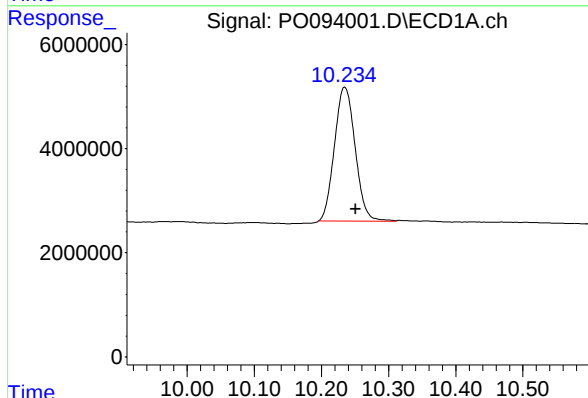


#2 Decachlorobiphenyl

R.T.: 10.235 min
Delta R.T.: -0.016 min
Response: 55144011
Conc: 24.65 ng/ml

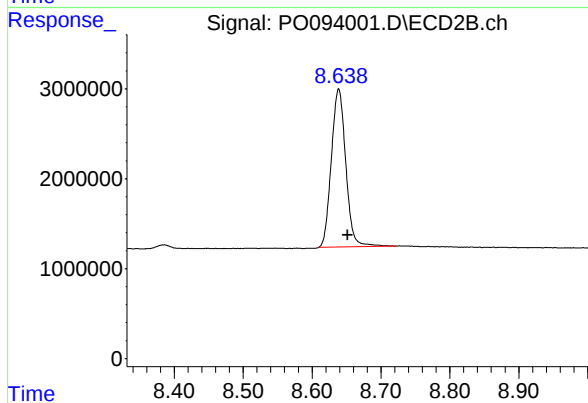

#2 Decachlorobiphenyl


R.T.: 8.639 min
Delta R.T.: -0.013 min
Response: 25523088
Conc: 25.53 ng/ml

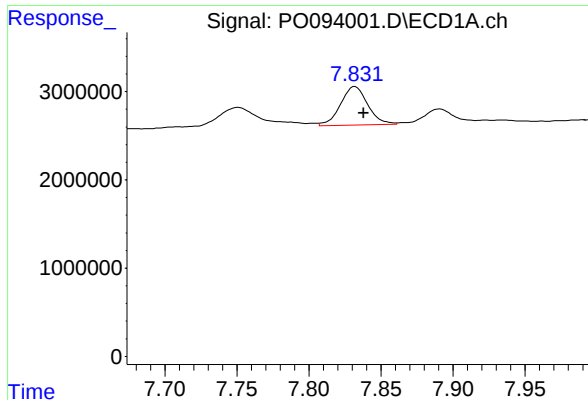

#36 AR-1262-1


R.T.: 7.832 min
Delta R.T.: -0.006 min
Response: 5698830
Conc: 33.36 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

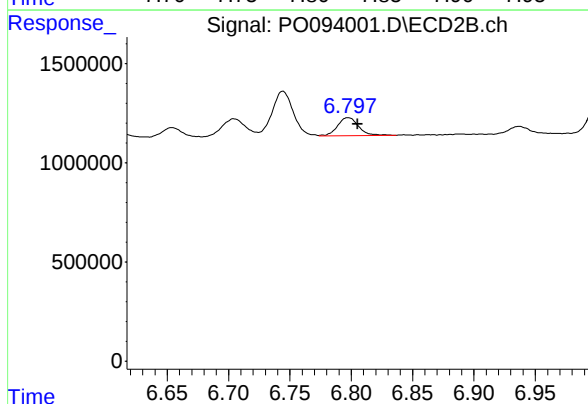


#36 AR-1262-1

R.T.: 6.797 min
Delta R.T.: -0.008 min
Response: 1100190
Conc: 31.44 ng/ml

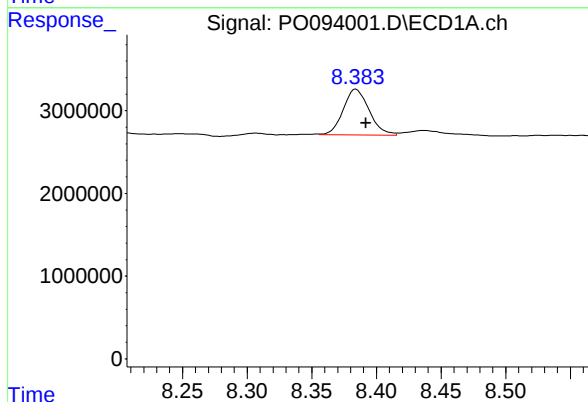


#37 AR-1262-2

R.T.: 8.383 min
Delta R.T.: -0.009 min
Response: 7709013
Conc: 33.16 ng/ml m

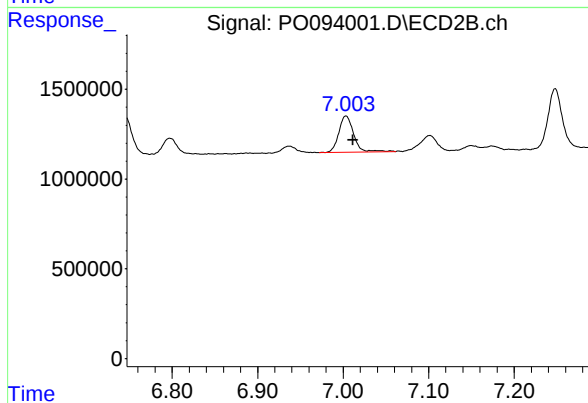

#37 AR-1262-2


R.T.: 7.003 min
Delta R.T.: -0.008 min
Response: 2462819
Conc: 34.86 ng/ml

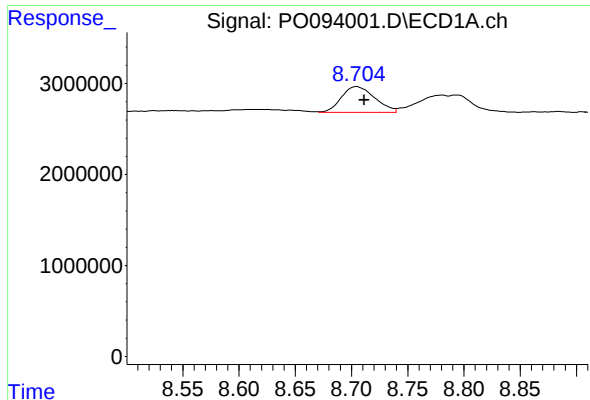

#38 AR-1262-3


R.T.: 8.705 min
Delta R.T.: -0.007 min
Response: 5790401
Conc: 35.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

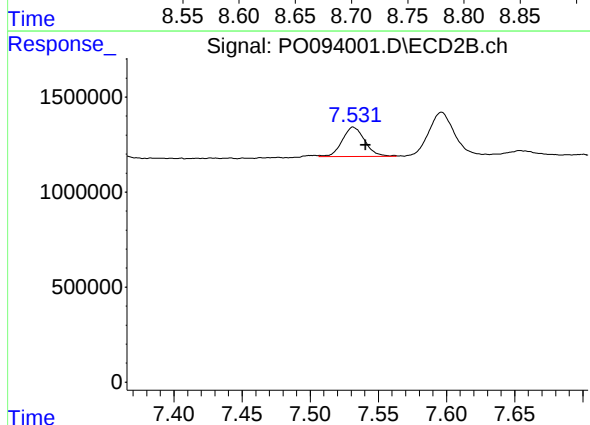


#38 AR-1262-3

R.T.: 7.531 min
Delta R.T.: -0.010 min
Response: 1770904
Conc: 35.39 ng/ml

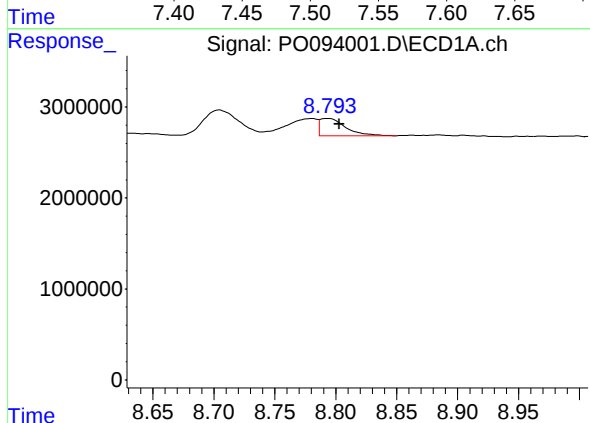


#39 AR-1262-4

R.T.: 8.794 min
Delta R.T.: -0.009 min
Response: 2784623
Conc: 27.79 ng/ml

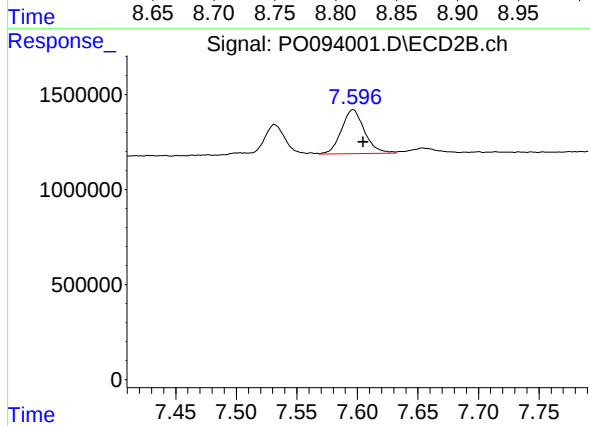

#39 AR-1262-4


R.T.: 7.596 min
Delta R.T.: -0.008 min
Response: 3085032
Conc: 37.20 ng/ml

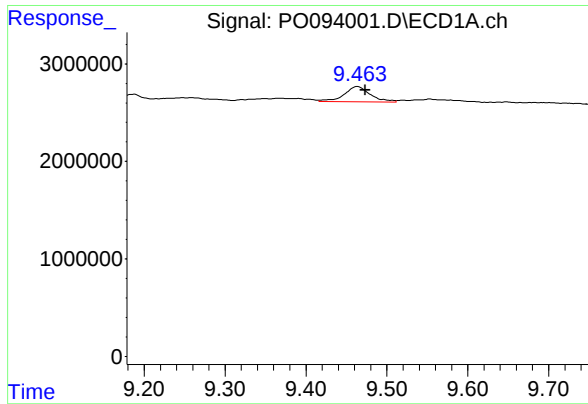

#40 AR-1262-5

R.T.: 9.464 min
Delta R.T.: -0.009 min
Response: 3519811
Conc: 43.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

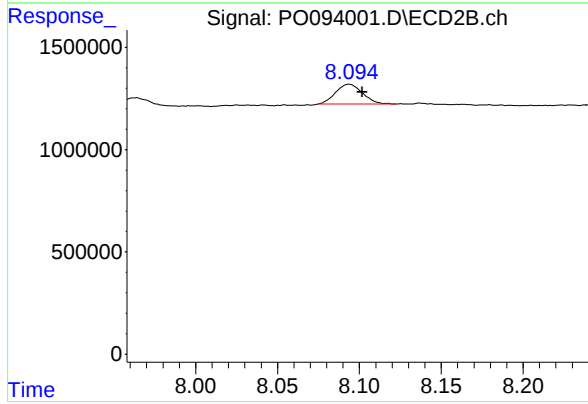

#40 AR-1262-5

R.T.: 8.094 min
Delta R.T.: -0.008 min
Response: 1107753
Conc: 34.05 ng/ml