

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040723\
 Data File : P0094002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2023 12:28
 Operator : YP/AJ
 Sample : 02213-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT2-2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 13:41:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.417	3.621	75825661	27567112	20.284	21.648
2) SA Decachlor...	10.236	8.639	62089635	27838144	27.757	27.844
Target Compounds						
41) L9 AR-1268-1	8.702	7.532	10961334	5661756	32.569	37.063
42) L9 AR-1268-2	8.796	7.597	11281042	4814637	35.052	35.438
43) L9 AR-1268-3	9.030	7.804	8809839	4183312	31.066	31.963
44) L9 AR-1268-4	9.466	8.093	3798442	1234118	39.286	31.177
45) L9 AR-1268-5	9.890	8.385	26008053	11752148	30.967	33.531



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040723\
Data File : PO094002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2023 12:28
Operator : YP/AJ
Sample : 02213-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 65 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 13:41:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

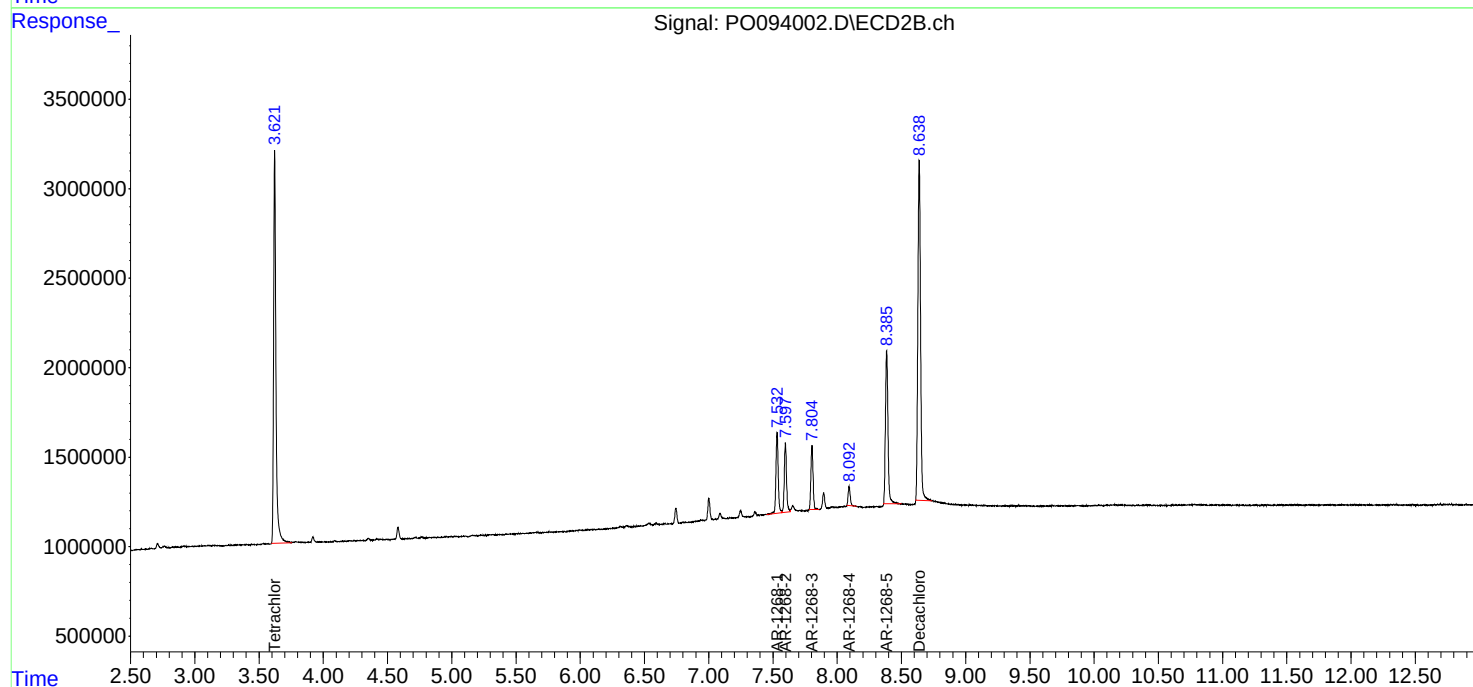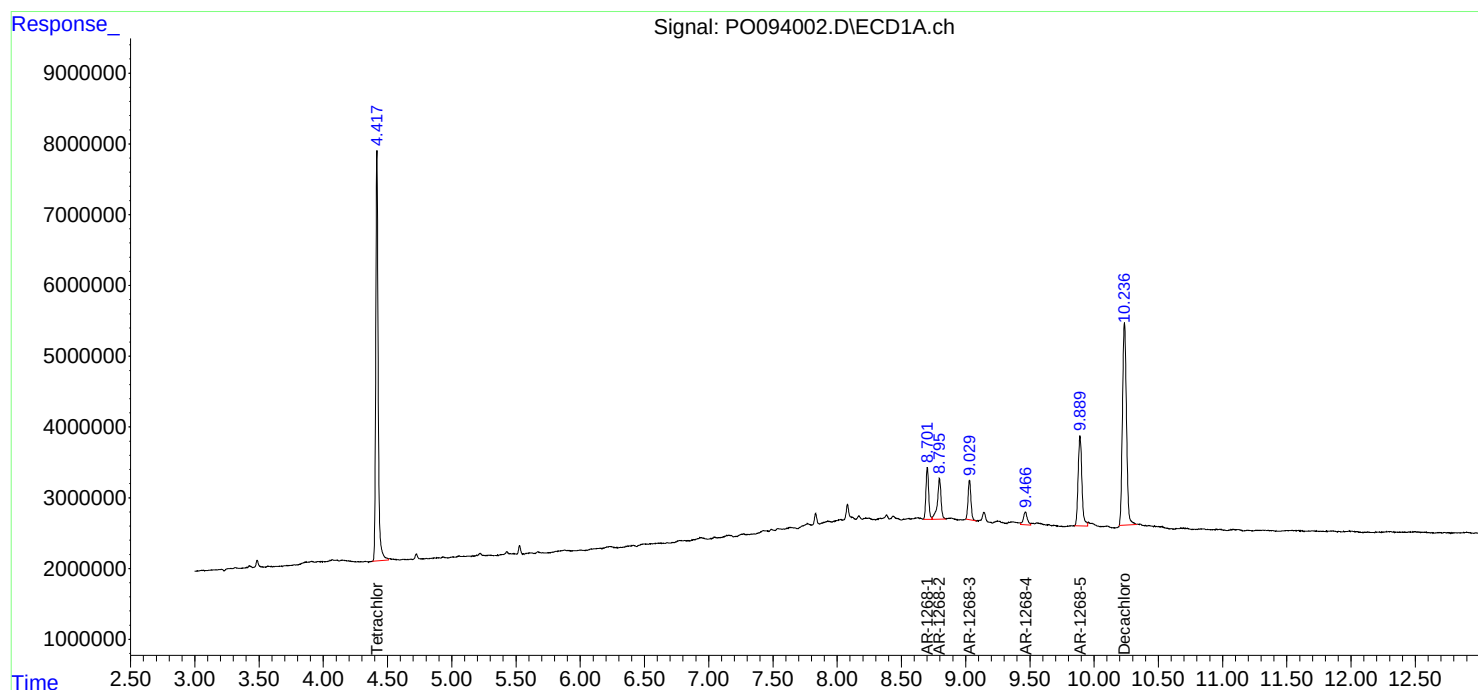


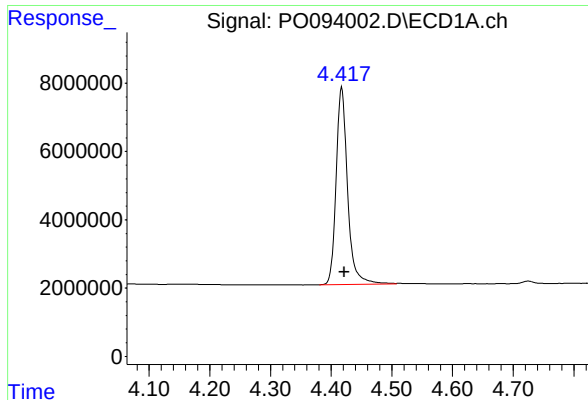

#1 Tetrachloro-m-xylene


R.T.: 4.417 min
Delta R.T.: -0.005 min
Response: 75825661
Conc: 20.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

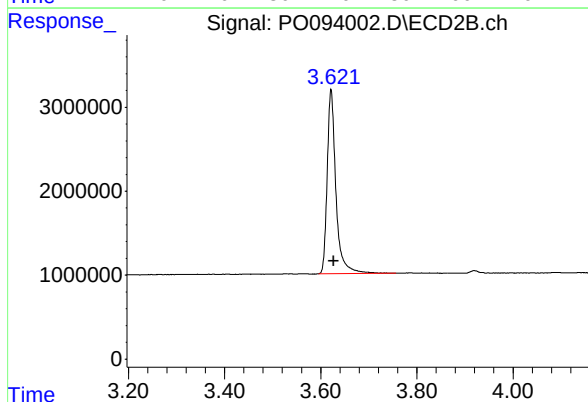


#1 Tetrachloro-m-xylene

R.T.: 3.621 min
Delta R.T.: -0.005 min
Response: 27567112
Conc: 21.65 ng/ml

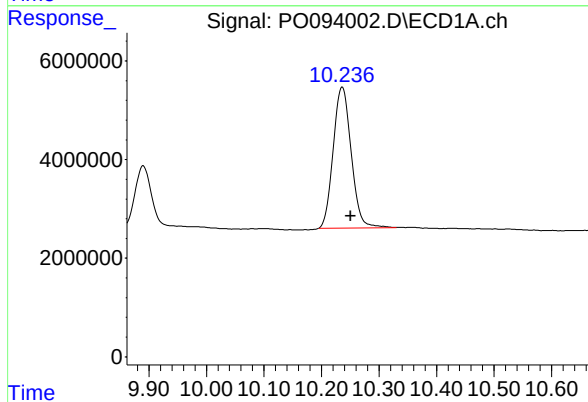


#2 Decachlorobiphenyl

R.T.: 10.236 min
Delta R.T.: -0.015 min
Response: 62089635
Conc: 27.76 ng/ml

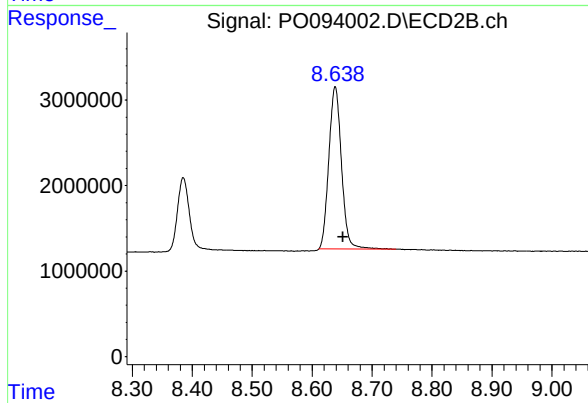

#2 Decachlorobiphenyl


R.T.: 8.639 min
Delta R.T.: -0.013 min
Response: 27838144
Conc: 27.84 ng/ml

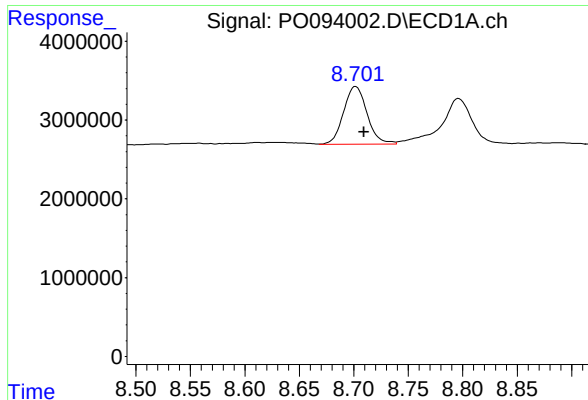

#41 AR-1268-1


R.T.: 8.702 min
Delta R.T.: -0.008 min
Response: 10961334
Conc: 32.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

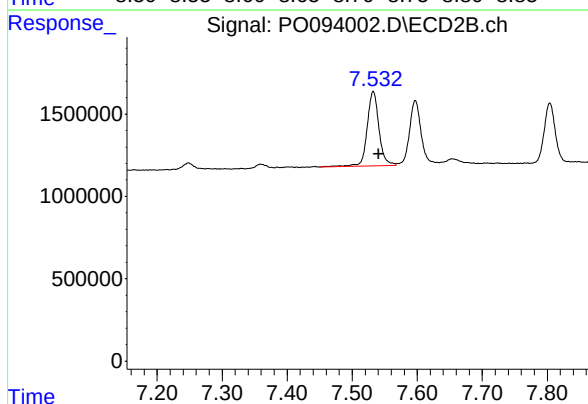


#41 AR-1268-1

R.T.: 7.532 min
Delta R.T.: -0.008 min
Response: 5661756
Conc: 37.06 ng/ml

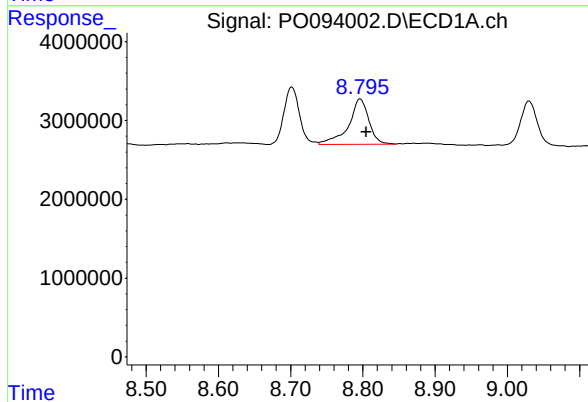


#42 AR-1268-2

R.T.: 8.796 min
Delta R.T.: -0.009 min
Response: 11281042
Conc: 35.05 ng/ml

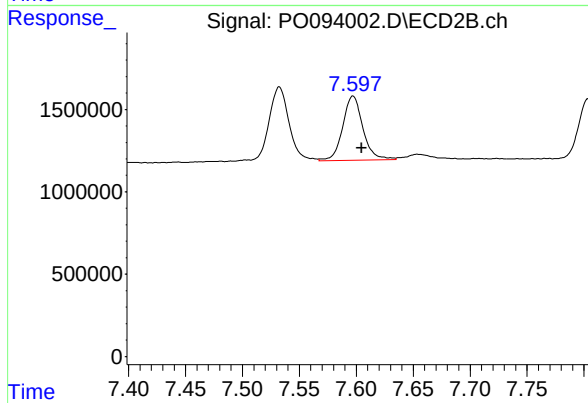

#42 AR-1268-2


R.T.: 7.597 min
Delta R.T.: -0.008 min
Response: 4814637
Conc: 35.44 ng/ml

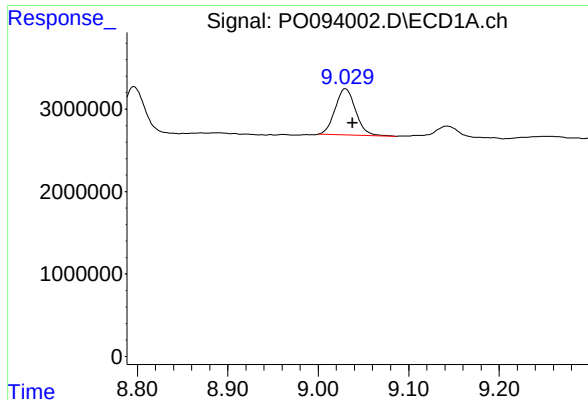

#43 AR-1268-3


R.T.: 9.030 min
Delta R.T.: -0.008 min
Response: 8809839
Conc: 31.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

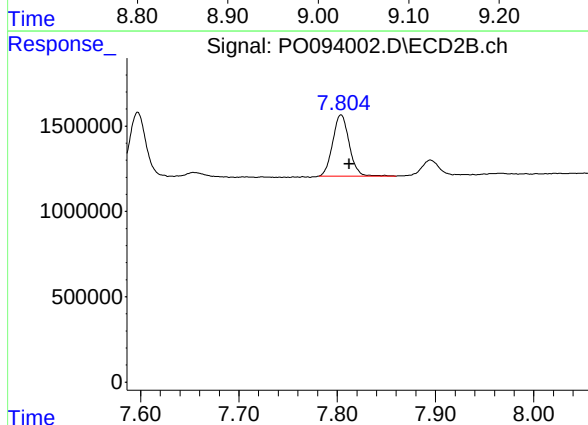


#43 AR-1268-3

R.T.: 7.804 min
Delta R.T.: -0.008 min
Response: 4183312
Conc: 31.96 ng/ml

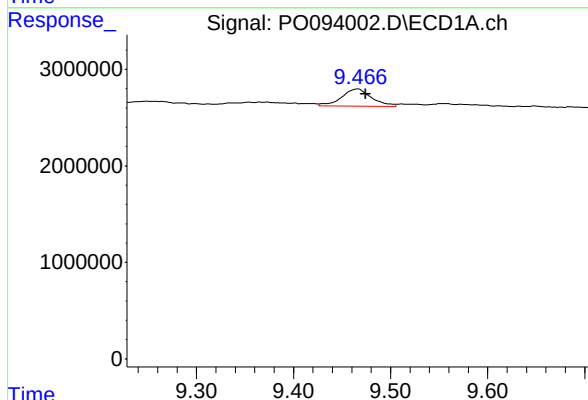


#44 AR-1268-4

R.T.: 9.466 min
Delta R.T.: -0.008 min
Response: 3798442
Conc: 39.29 ng/ml

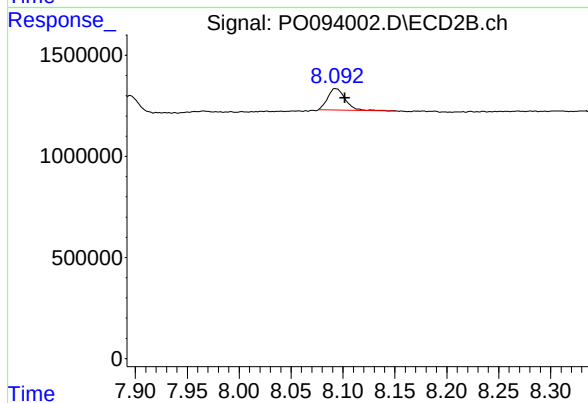

#44 AR-1268-4


R.T.: 8.093 min
Delta R.T.: -0.009 min
Response: 1234118
Conc: 31.18 ng/ml

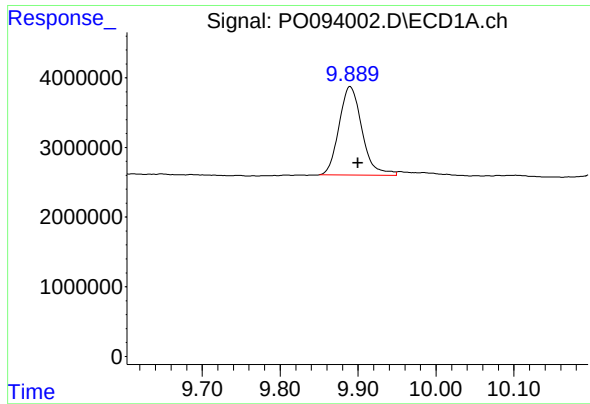

#45 AR-1268-5

R.T.: 9.890 min
Delta R.T.: -0.010 min
Response: 26008053
Conc: 30.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2023

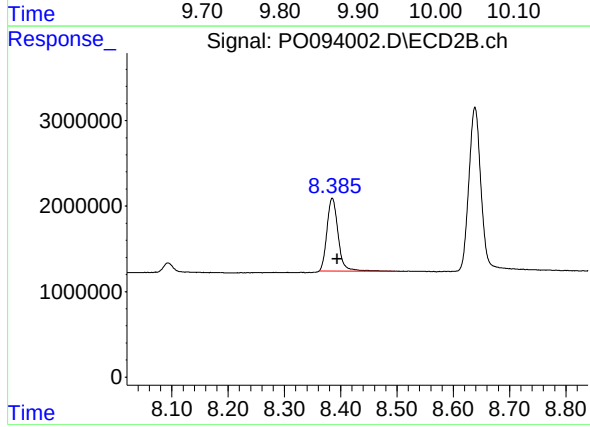

#45 AR-1268-5

R.T.: 8.385 min
Delta R.T.: -0.009 min
Response: 11752148
Conc: 33.53 ng/ml