

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040725\
 Data File : P0110276.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Apr 2025 15:47
 Operator : YP/AJ
 Sample : Q1733-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ETGI-328

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/08/2025
 Supervised By :mohammad ahmed 04/09/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 07 16:26:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 19 02:52:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.695	3.692	89056628	51834184	9.785	9.884
2) SA Decachlor...	8.753	8.703	77266432	19597106	10.049m	8.078m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040725\
Data File : PO110276.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Apr 2025 15:47
Operator : YP/AJ
Sample : Q1733-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ETGI-328


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/08/2025
Supervised By :mohammad ahmed 04/09/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 07 16:26:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

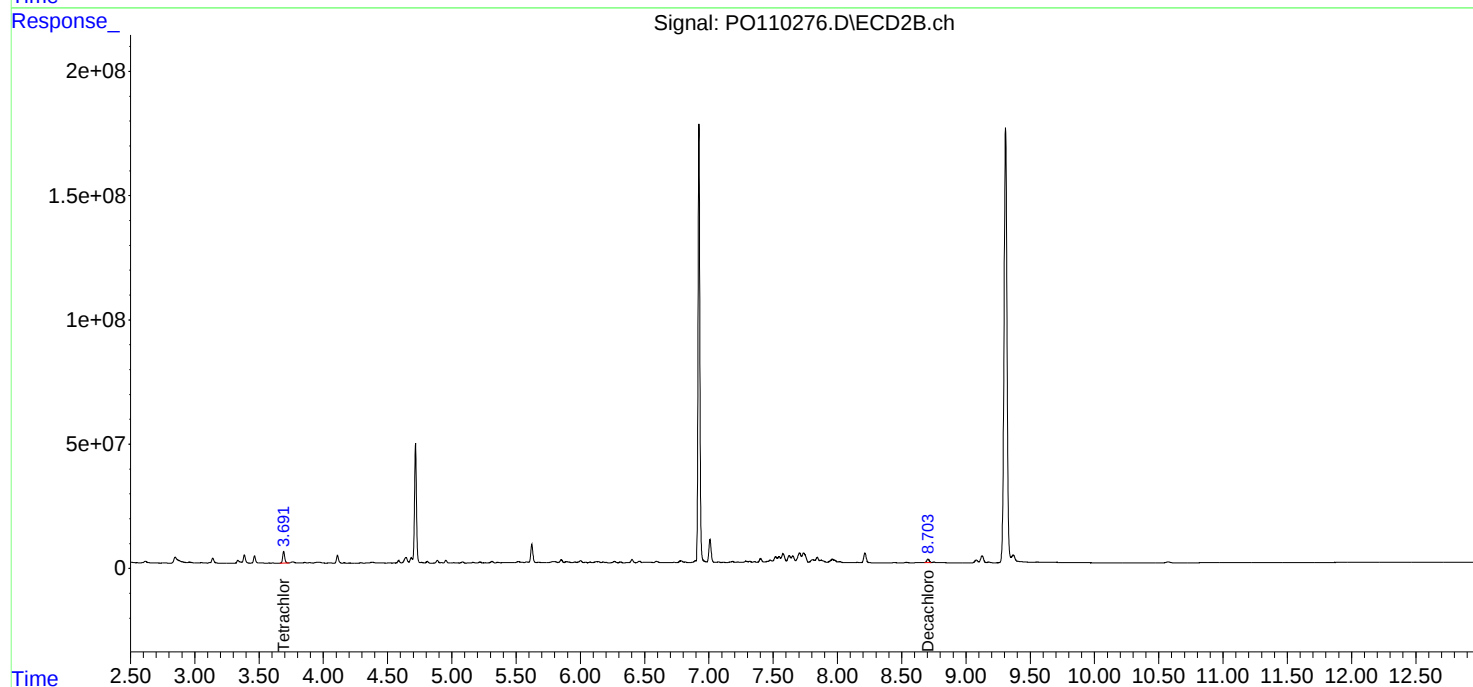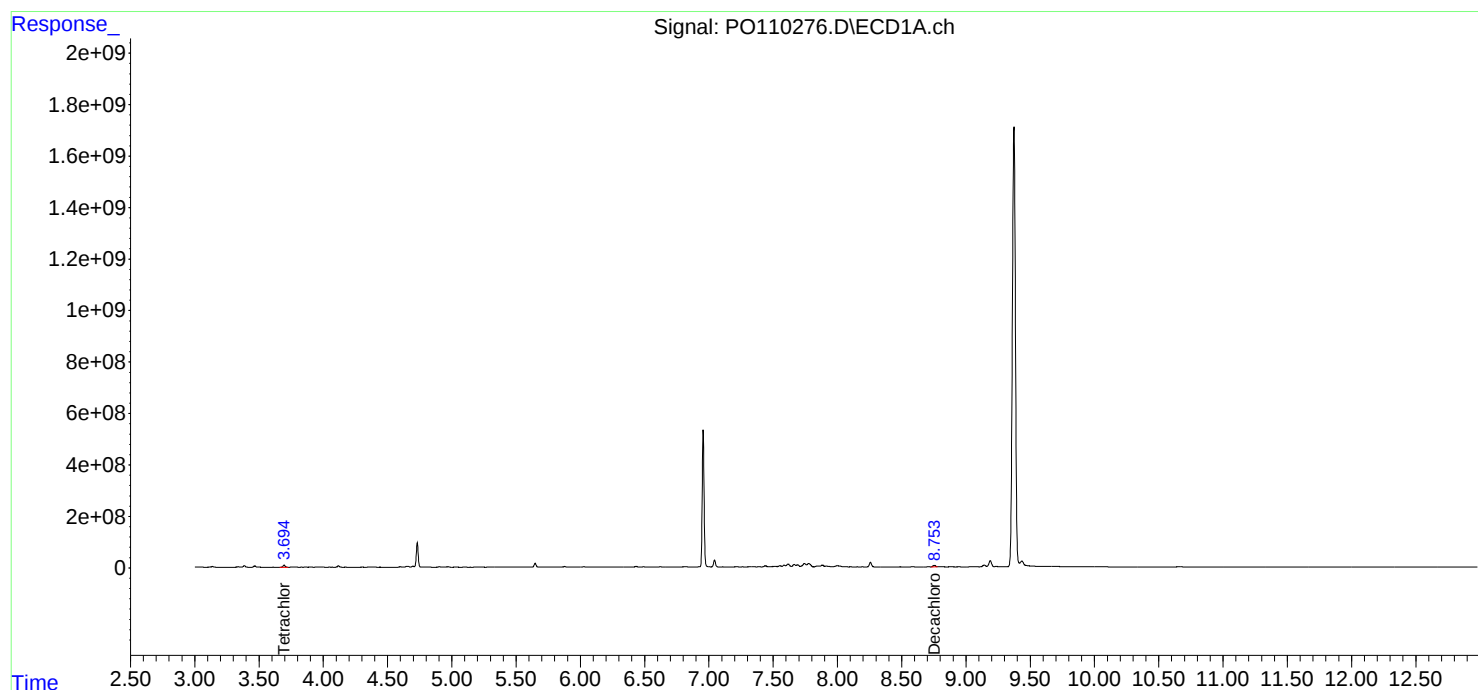

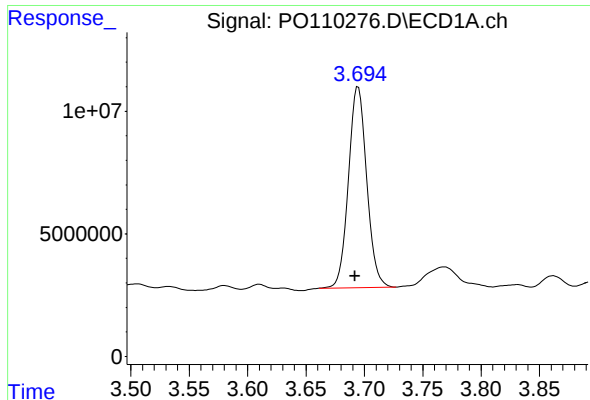


#1 Tetrachloro-m-xylene

R.T.: 3.695 min
Delta R.T.: 0.003 min
Response: 89056628
Conc: 9.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-328


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/08/2025
Supervised By :mohammad ahmed 04/09/2025

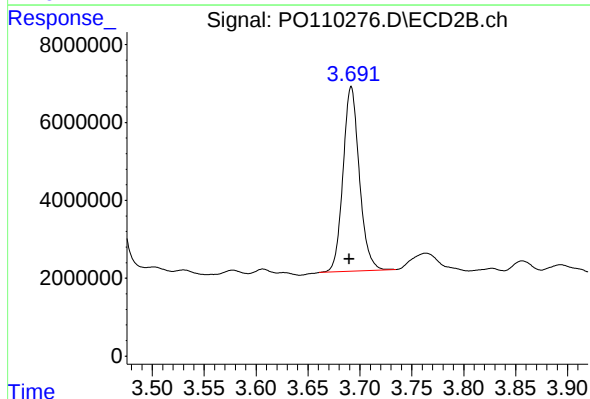


#1 Tetrachloro-m-xylene

R.T.: 3.692 min
Delta R.T.: 0.002 min
Response: 51834184
Conc: 9.88 ng/ml

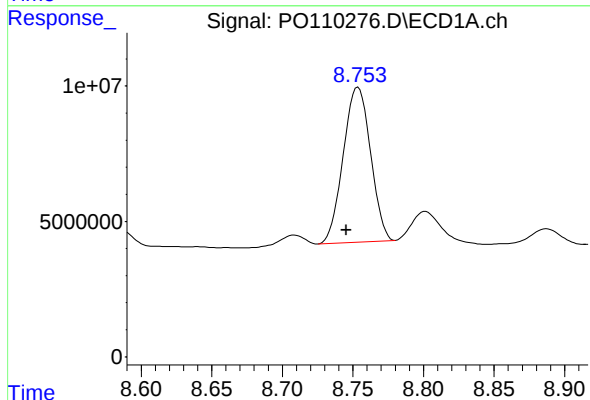

#2 Decachlorobiphenyl

R.T.: 8.753 min
Delta R.T.: 0.008 min
Response: 77266432
Conc: 10.05 ng/ml m

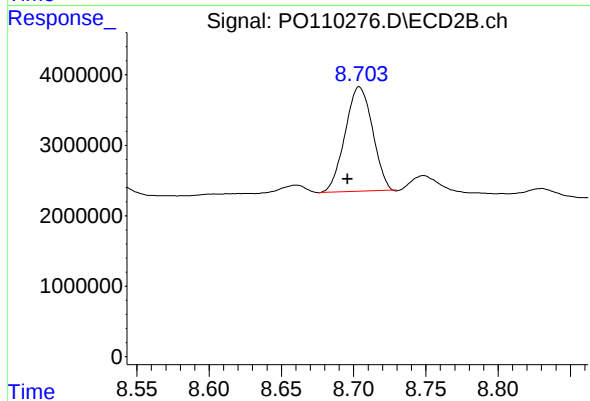

#2 Decachlorobiphenyl

R.T.: 8.703 min
Delta R.T.: 0.008 min
Response: 19597106
Conc: 8.08 ng/ml m