

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040821\
 Data File : P0076870.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Apr 2021 11:02
 Operator : DD\AJ
 Sample : PB135396BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 14:57:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.897	3.894	1971915	1064210	21.200	21.207
2) SA Decachlor...	10.870	9.137	1942857	885862	20.977	18.255
Target Compounds						
9) L2 AR-1221-2	0.000	4.242	0	11808	N.D.	33.483 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040821\
Data File : P0076870.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Apr 2021 11:02
Operator : DD\AJ
Sample : PB135396BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 14:57:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

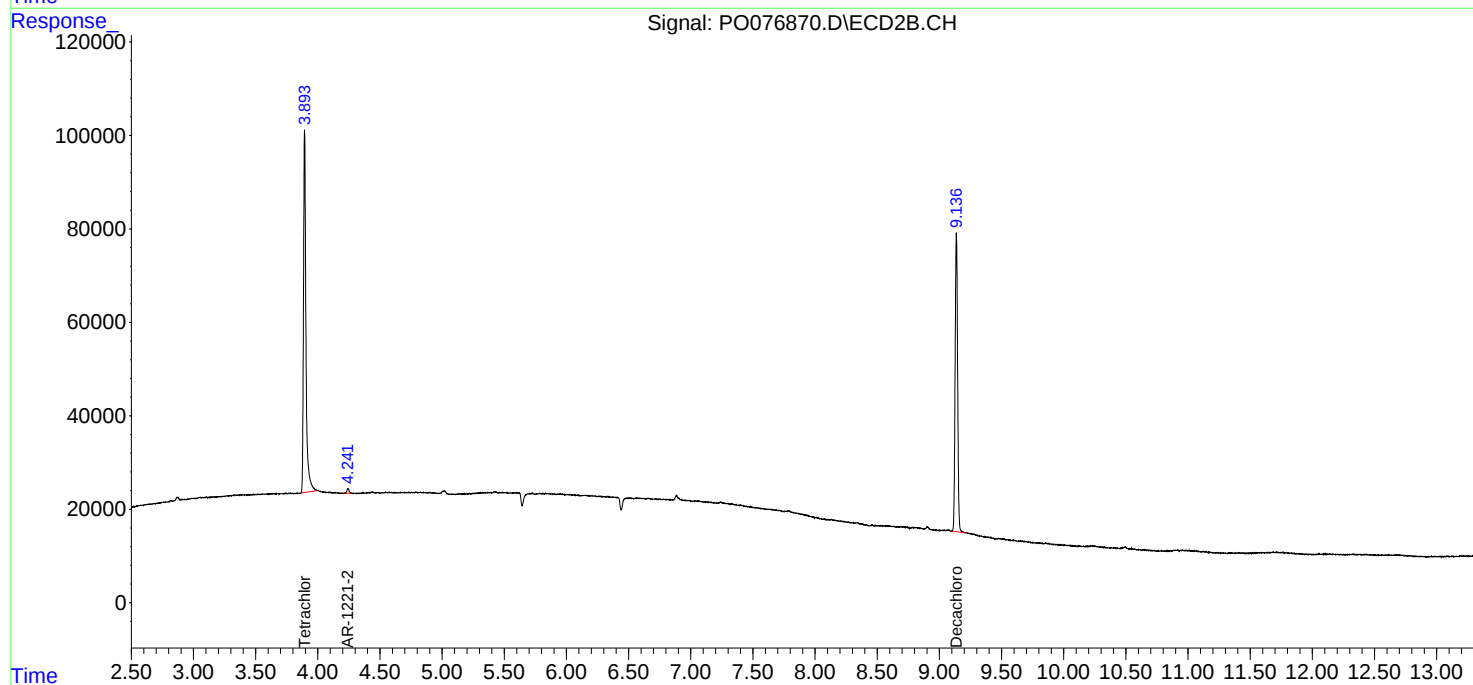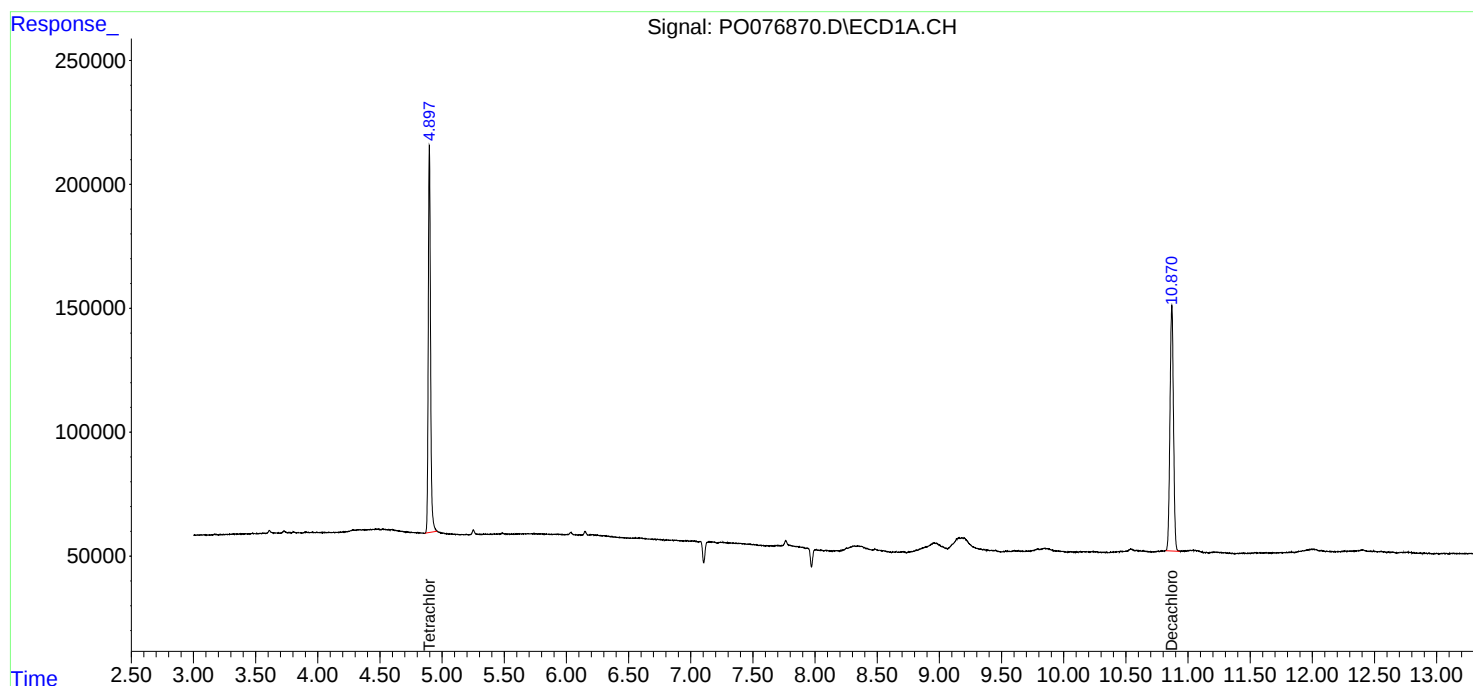


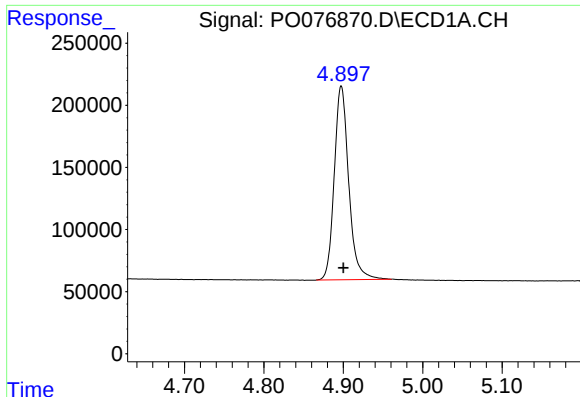

#1 Tetrachloro-m-xylene


R.T.: 4.897 min
Delta R.T.: -0.003 min
Response: 1971915
Conc: 21.20 ng/ml

Instrument :
ECD_O
ClientSampleId :

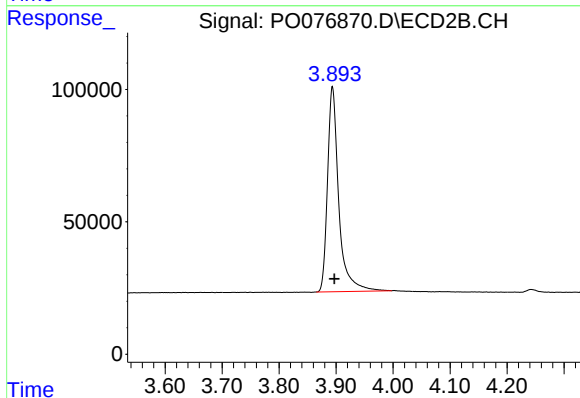


#1 Tetrachloro-m-xylene

R.T.: 3.894 min
Delta R.T.: -0.003 min
Response: 1064210
Conc: 21.21 ng/ml

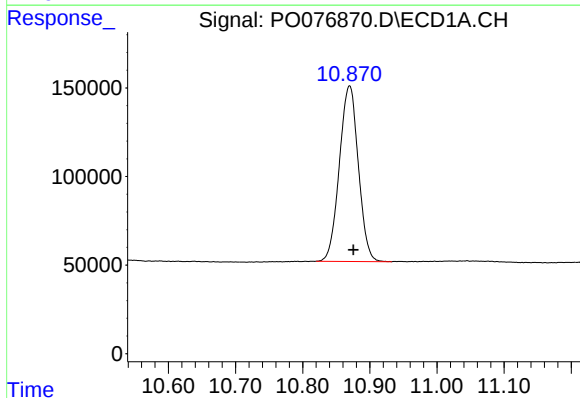


#2 Decachlorobiphenyl

R.T.: 10.870 min
Delta R.T.: -0.006 min
Response: 1942857
Conc: 20.98 ng/ml

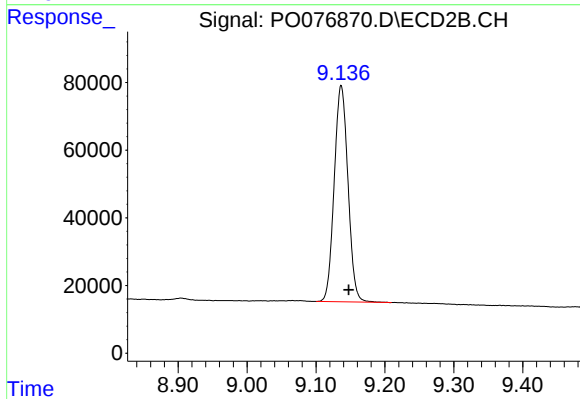

#2 Decachlorobiphenyl


R.T.: 9.137 min
Delta R.T.: -0.011 min
Response: 885862
Conc: 18.26 ng/ml

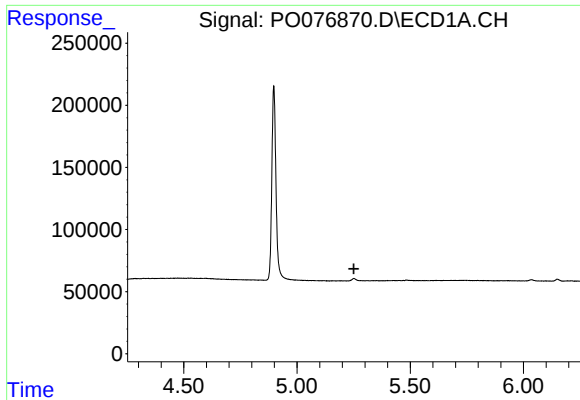

#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 5.251 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

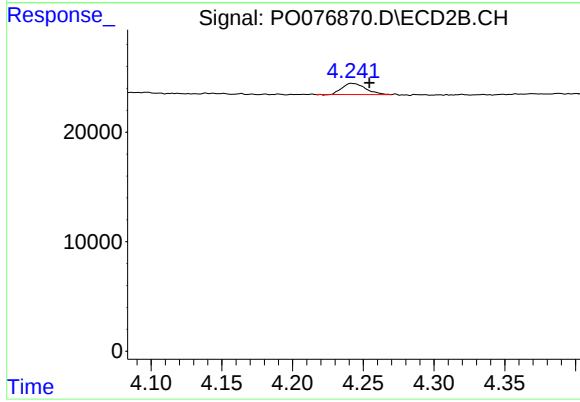

#9 AR-1221-2

R.T.: 4.242 min
Delta R.T.: -0.013 min
Response: 11808
Conc: 33.48 ng/ml