

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040821\
 Data File : P0076875.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Apr 2021 12:41
 Operator : DD\AJ
 Sample : M1972-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ETGI-371

Manual Integrations
 APPROVED

Ankita
 4/9/2021 8:44:27 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 14:59:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.895	3.893	2131897	1136995	22.920	22.657
2) SA Decachlor...	10.865	9.135	1557521	734639	16.816	15.139m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040821\
Data File : P0076875.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Apr 2021 12:41
Operator : DD\AJ
Sample : M1972-02
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ETGI-371


Manual Integrations
APPROVED

Ankita
4/9/2021 8:44:27 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 14:59:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

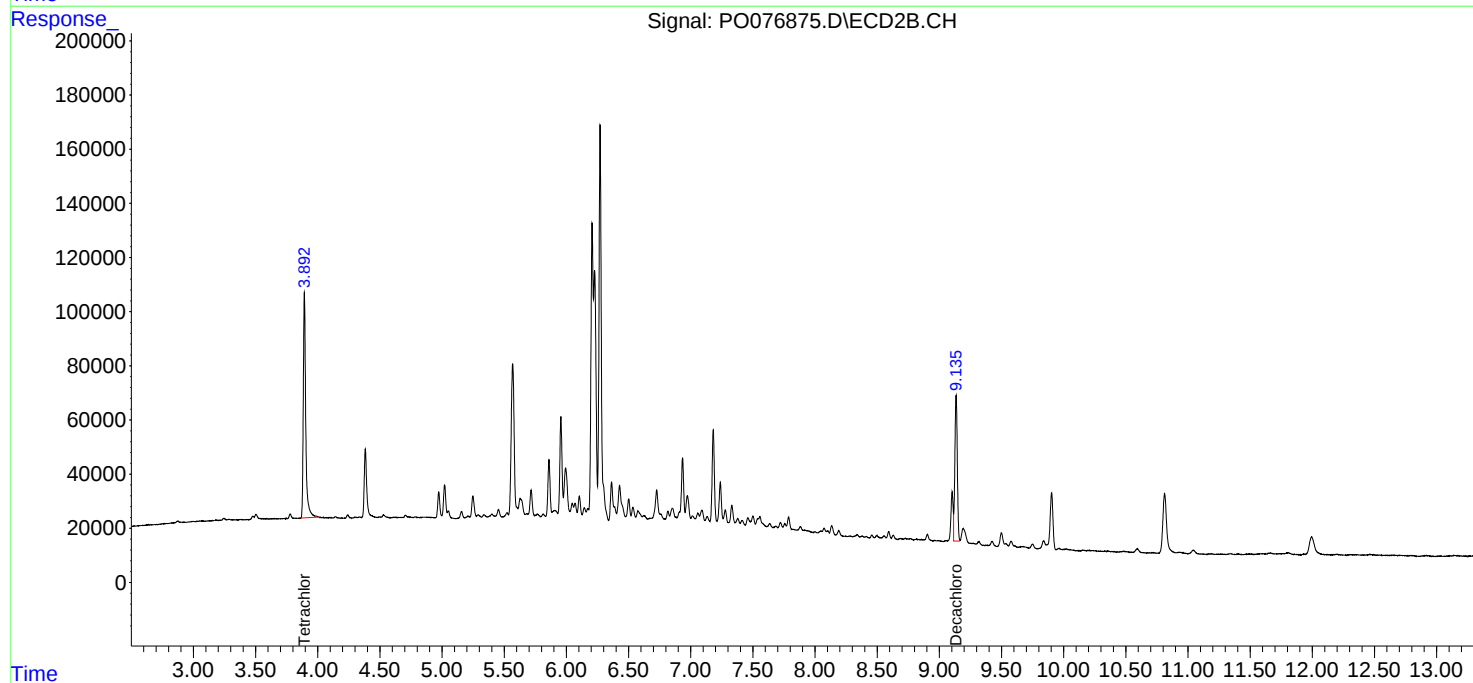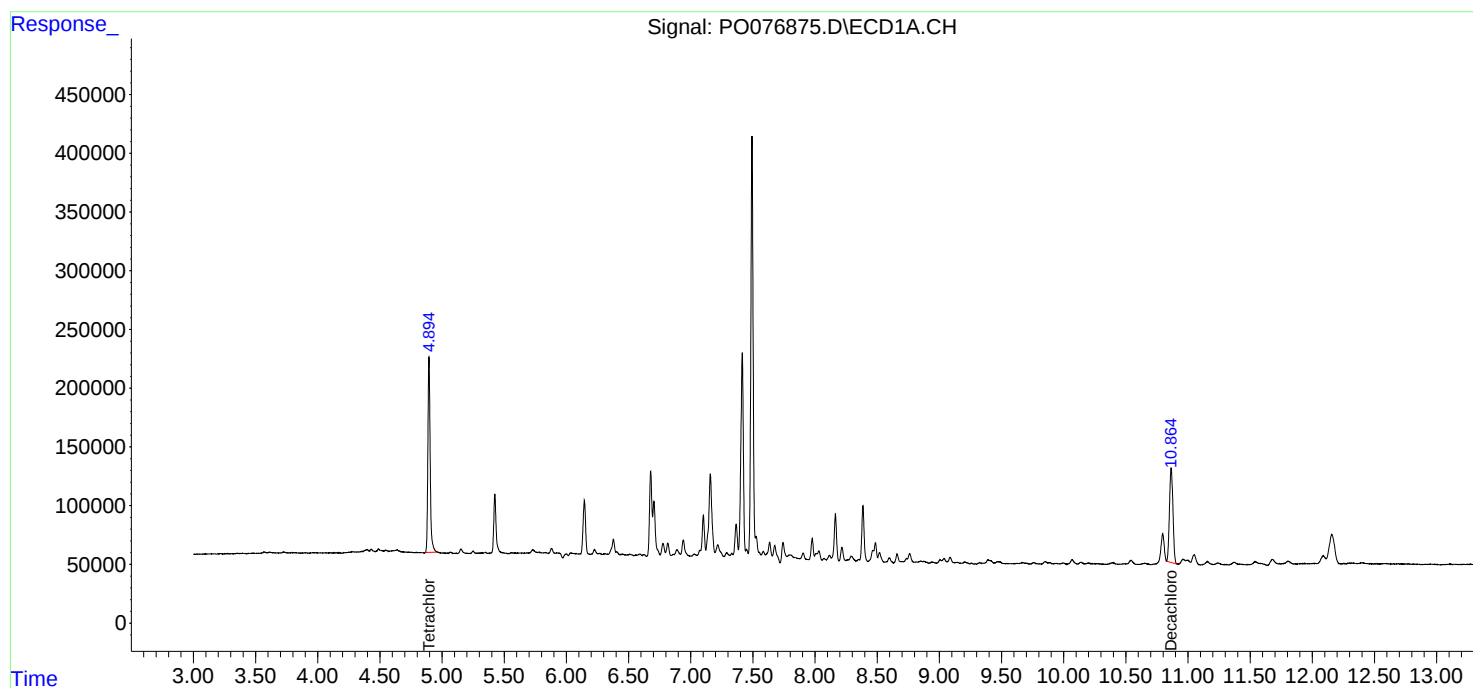

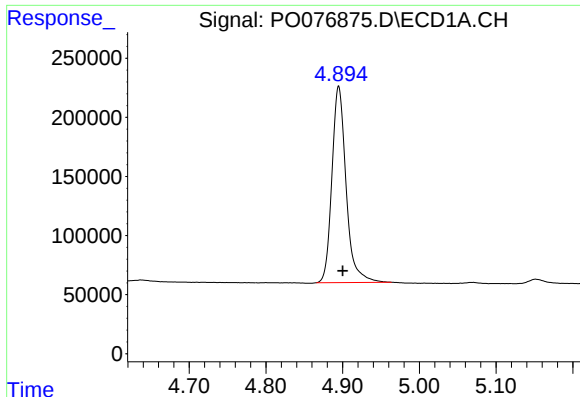


#1 Tetrachloro-m-xylene

R.T.: 4.895 min
Delta R.T.: -0.005 min
Response: 2131897
Conc: 22.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
ETGI-371


Manual Integrations
APPROVED

Ankita
4/9/2021 8:44:27 AM

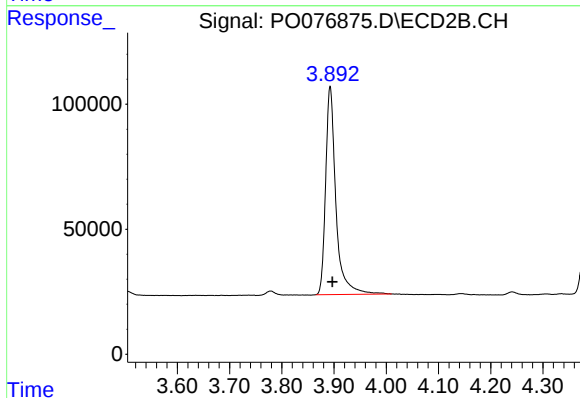


#1 Tetrachloro-m-xylene

R.T.: 3.893 min
Delta R.T.: -0.004 min
Response: 1136995
Conc: 22.66 ng/ml

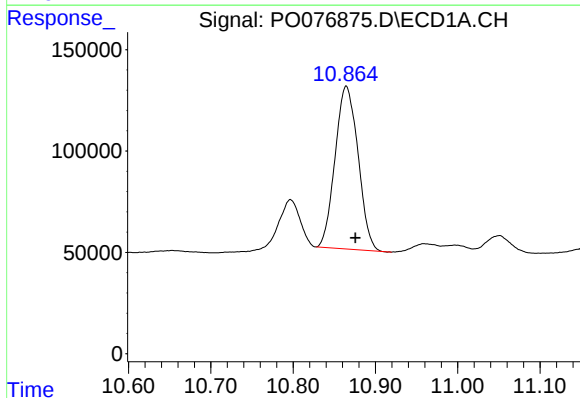

#2 Decachlorobiphenyl

R.T.: 10.865 min
Delta R.T.: -0.011 min
Response: 1557521
Conc: 16.82 ng/ml

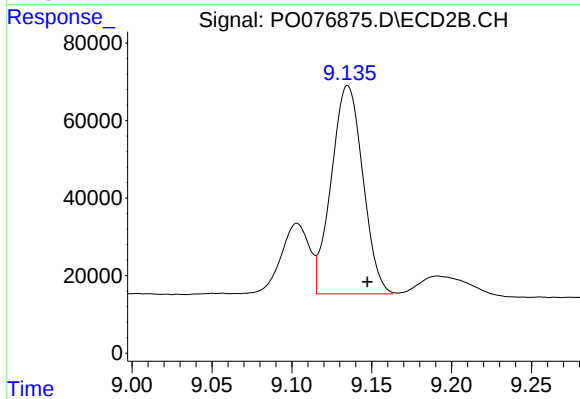

#2 Decachlorobiphenyl

R.T.: 9.135 min
Delta R.T.: -0.013 min
Response: 734639
Conc: 15.14 ng/ml m