

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040821\
 Data File : P0076878.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Apr 2021 13:32
 Operator : DD\AJ
 Sample : M1980-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 B8

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 15:01:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.896	3.893	2026212	1057880	21.784	21.081
2) SA Decachlor...	10.866	9.136	1976855	894080	21.344	18.425

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040821\
Data File : P0076878.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Apr 2021 13:32
Operator : DD\AJ
Sample : M1980-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
B8

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 15:01:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

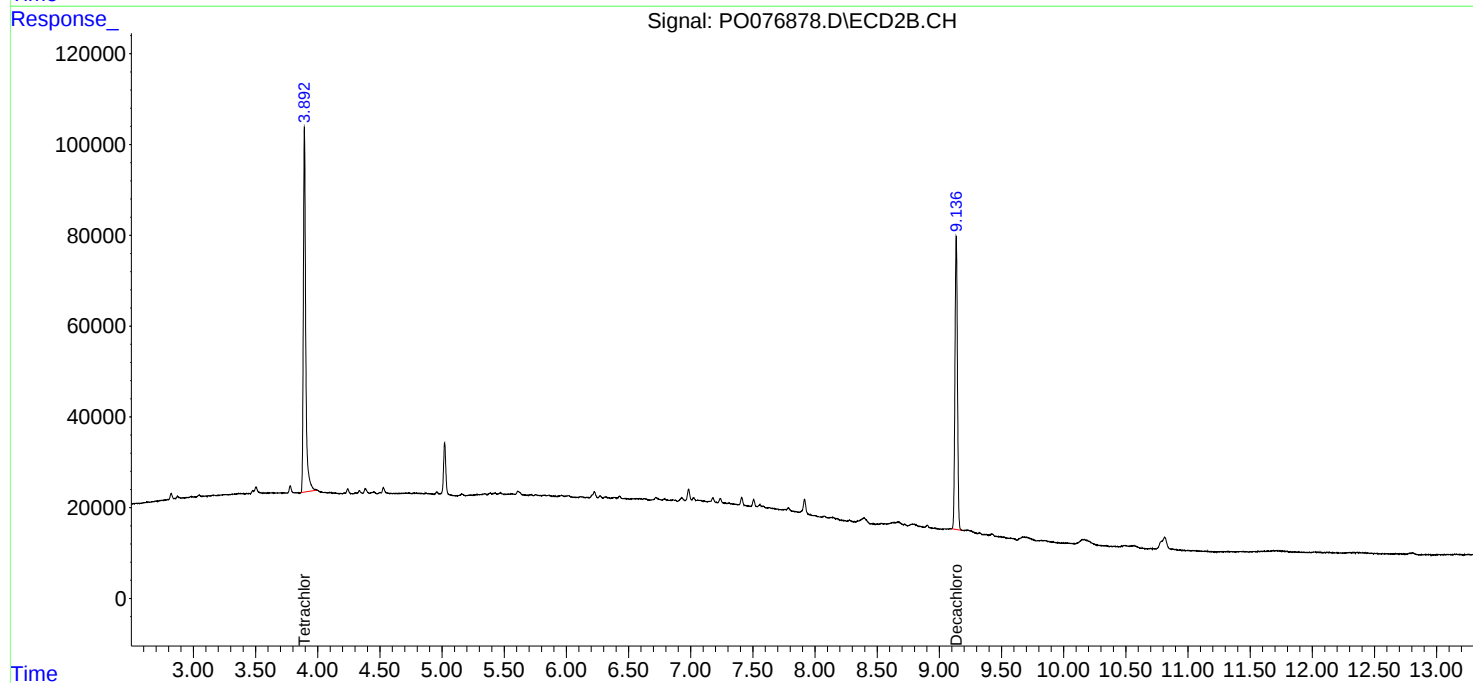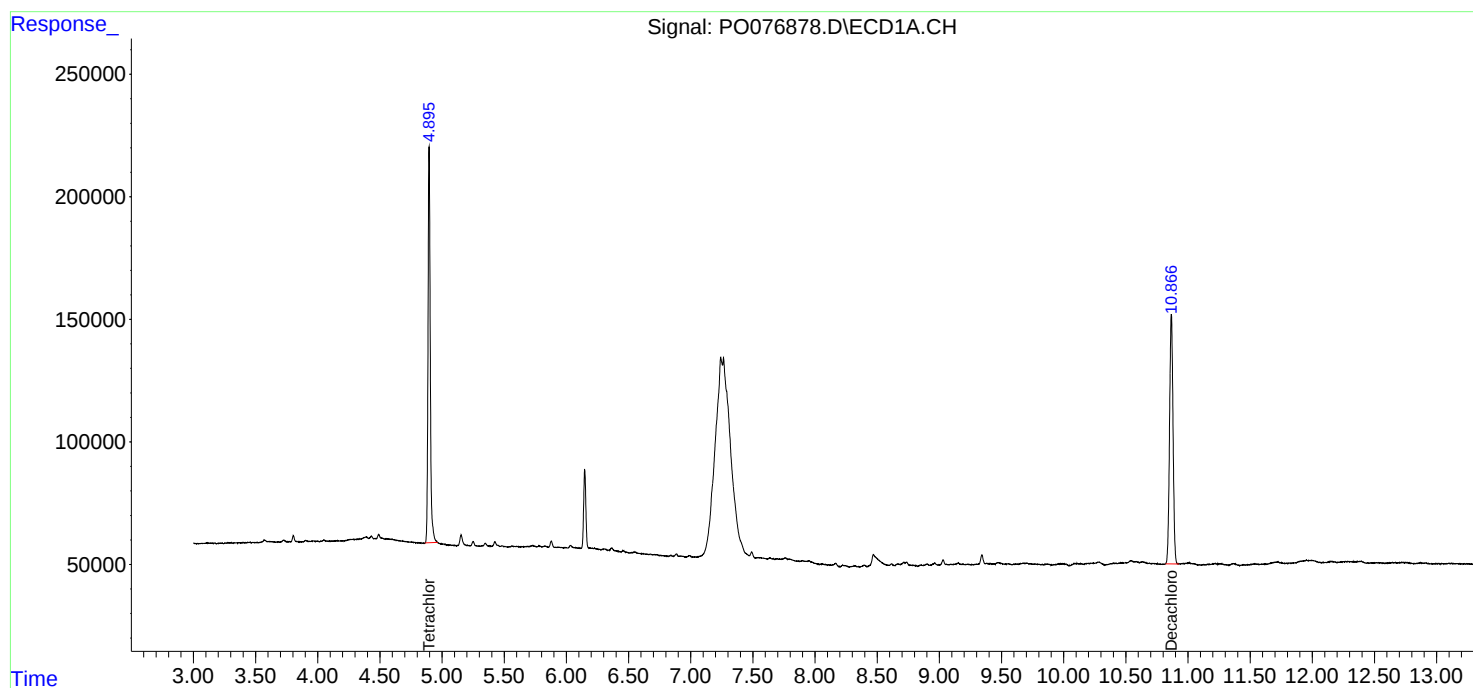


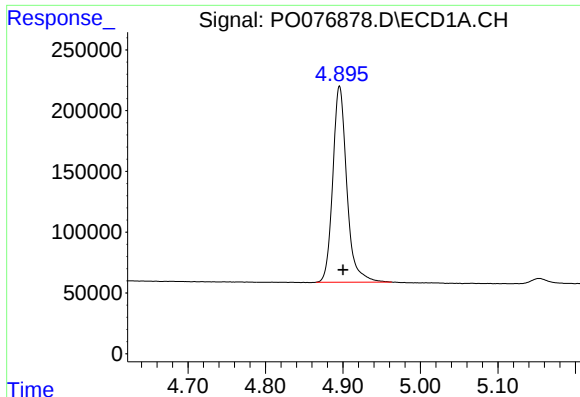

#1 Tetrachloro-m-xylene


R.T.: 4.896 min
Delta R.T.: -0.004 min
Response: 2026212
Conc: 21.78 ng/ml

Instrument :
ECD_O
ClientSampleId :
B8

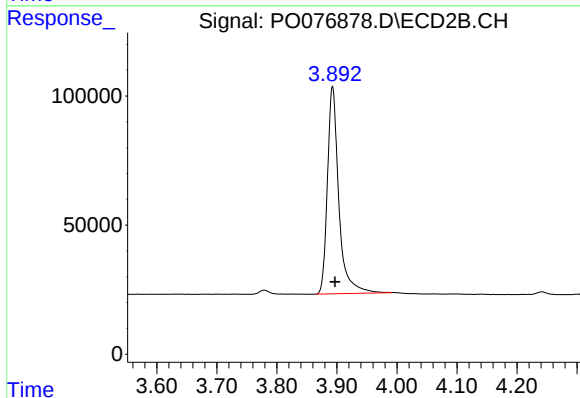


#1 Tetrachloro-m-xylene

R.T.: 3.893 min
Delta R.T.: -0.004 min
Response: 1057880
Conc: 21.08 ng/ml

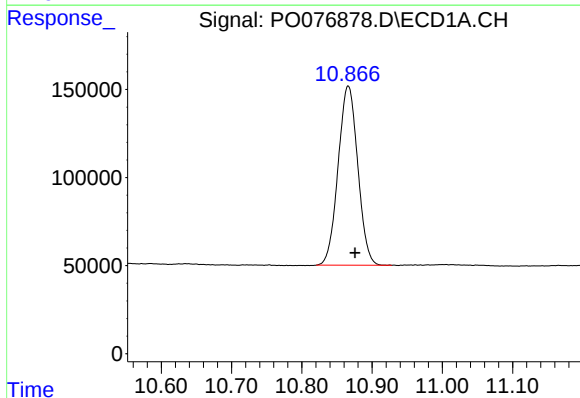

#2 Decachlorobiphenyl

R.T.: 10.866 min
Delta R.T.: -0.010 min
Response: 1976855
Conc: 21.34 ng/ml

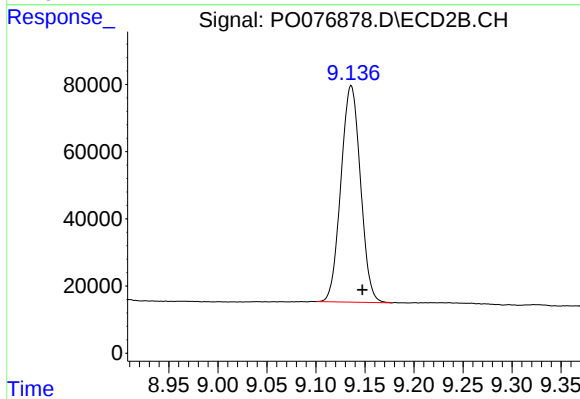

#2 Decachlorobiphenyl

R.T.: 9.136 min
Delta R.T.: -0.011 min
Response: 894080
Conc: 18.42 ng/ml