

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040823\
 Data File : P0094014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2023 16:09
 Operator : YP/AJ
 Sample : 02224-05
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OU3-FC-BACKFILL-03

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/10/2023
 Supervised By :Ankita Jodhani 04/10/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 01:31:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.416	3.621	70742412	26056672	18.924	20.462
2) SA Decachlor...	10.235	8.638	49764322	22584300	22.247m	22.589m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040823\
Data File : PO094014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2023 16:09
Operator : YP/AJ
Sample : 02224-05
Misc :
ALS Vial : 70 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OU3-FC-BACKFILL-03


Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 04/10/2023
Supervised By : Ankita Jodhani 04/10/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 01:31:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

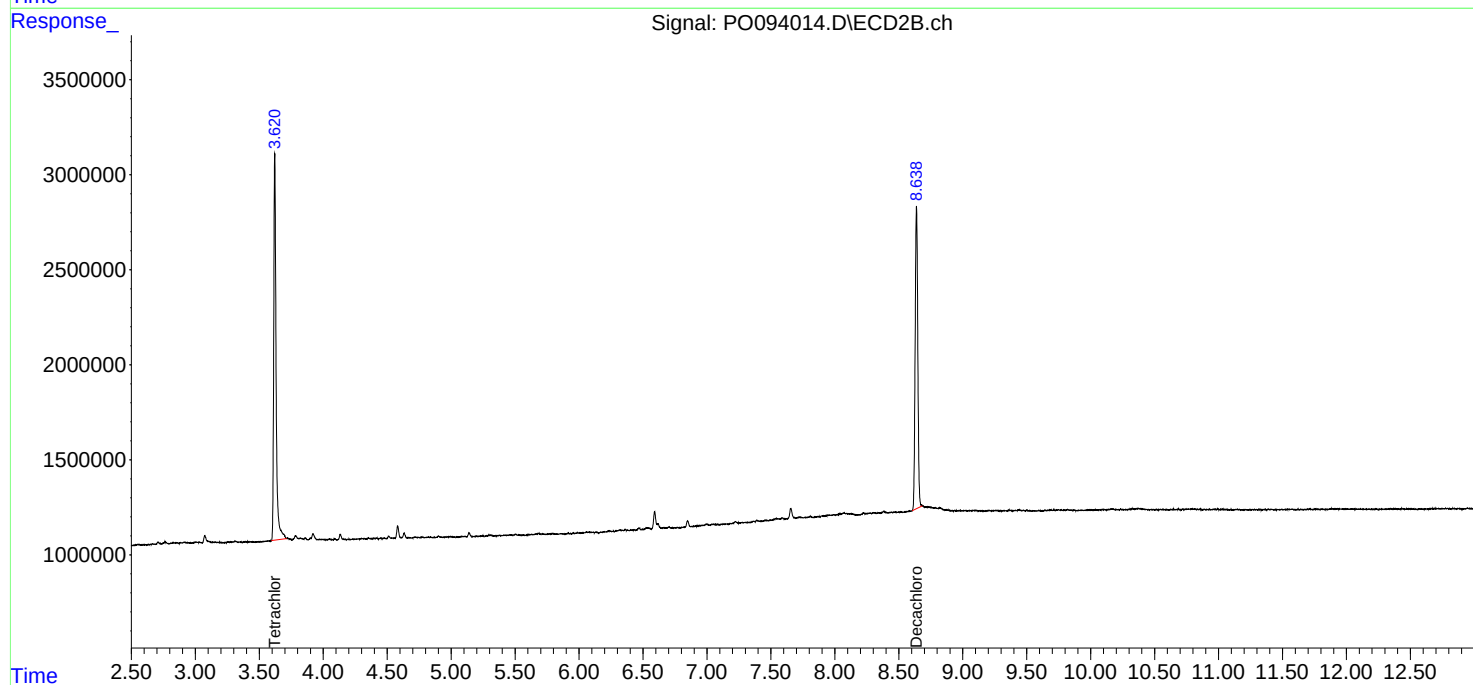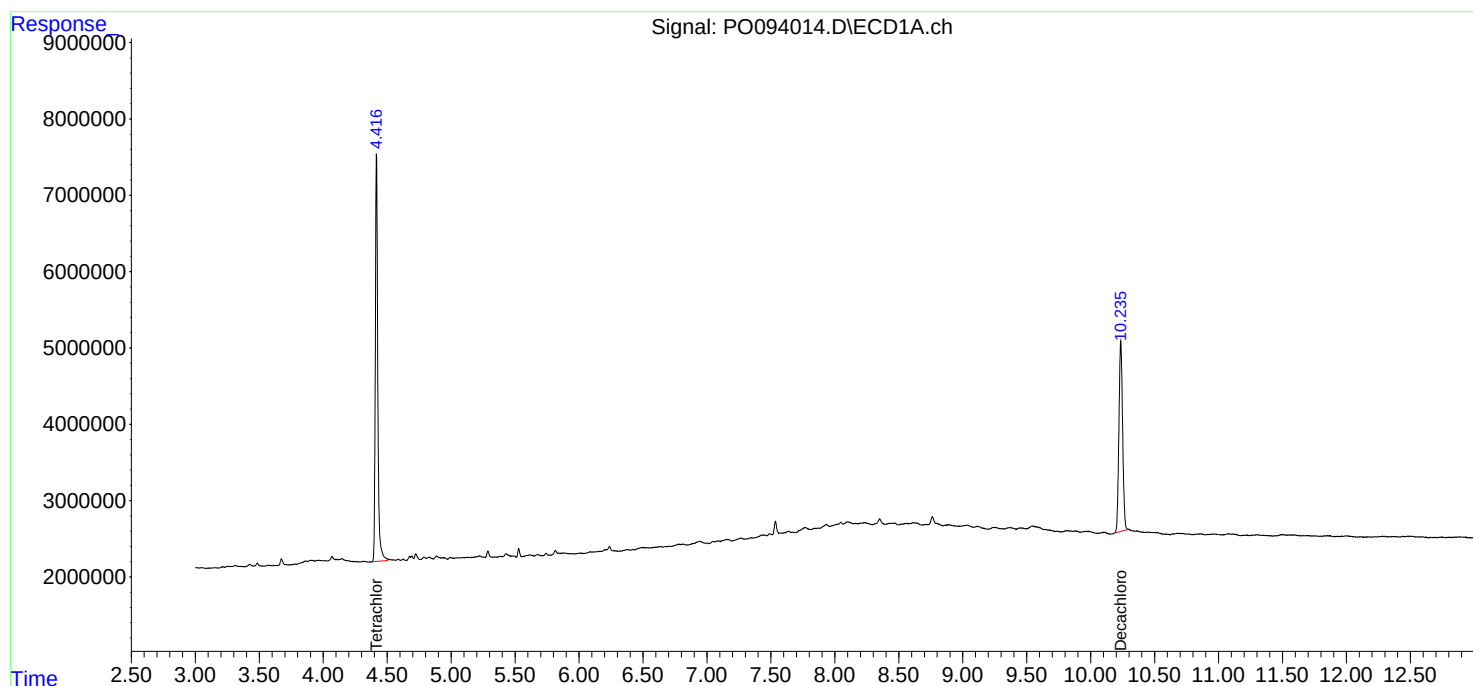

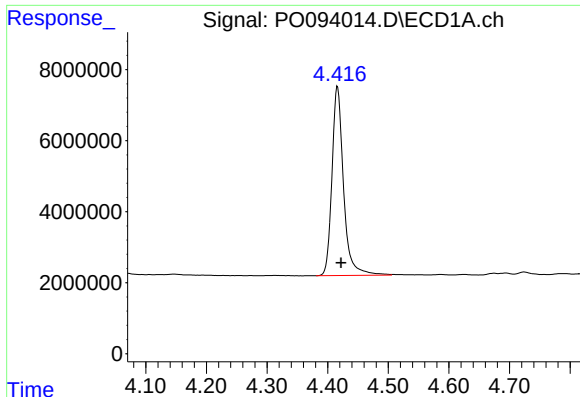


#1 Tetrachloro-m-xylene

R.T.: 4.416 min
Delta R.T.: -0.006 min
Response: 70742412
Conc: 18.92 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU3-FC-BACKFILL-03


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2023
Supervised By :Ankita Jodhani 04/10/2023

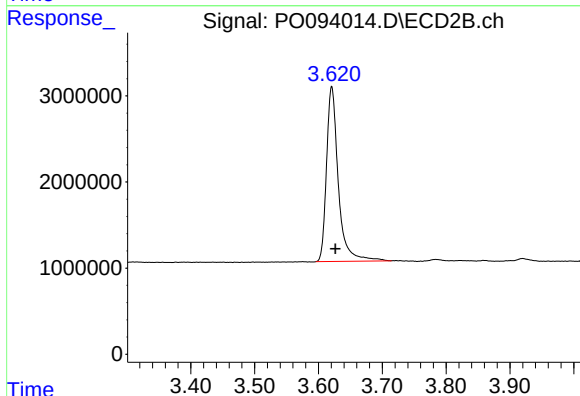


#1 Tetrachloro-m-xylene

R.T.: 3.621 min
Delta R.T.: -0.006 min
Response: 26056672
Conc: 20.46 ng/ml

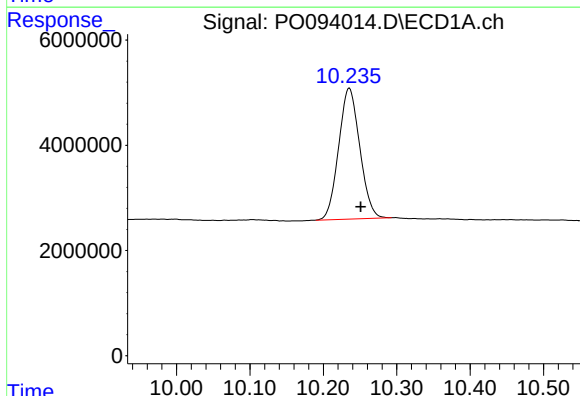

#2 Decachlorobiphenyl

R.T.: 10.235 min
Delta R.T.: -0.016 min
Response: 49764322
Conc: 22.25 ng/ml m

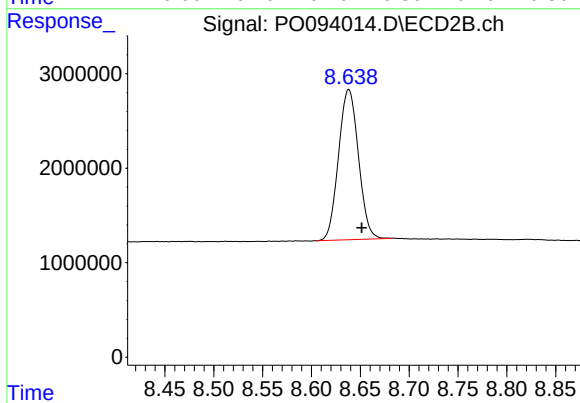

#2 Decachlorobiphenyl

R.T.: 8.638 min
Delta R.T.: -0.014 min
Response: 22584300
Conc: 22.59 ng/ml m