

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040823\
 Data File : P0094015.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2023 16:27
 Operator : YP/AJ
 Sample : 02224-07
 Misc :
 ALS Vial : 71 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OU3-FC-BACKFILL-04

Manual Integrations
 APPROVED

Reviewed By :Yogesh
 Patel

04/10/2023

Supervised By :Ankita
 Jodhani
 04/10/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 01:32:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.417	3.622	74070694	27587820	19.814	21.664
2) SA Decachlor...	10.237	8.639	53957367	24120264	24.121m	24.125

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040823\
Data File : PO094015.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2023 16:27
Operator : YP/AJ
Sample : 02224-07
Misc :
ALS Vial : 71 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OU3-FC-BACKFILL-04


Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel
04/10/2023
Supervised By :Ankita
Jodhani
04/10/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 01:32:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

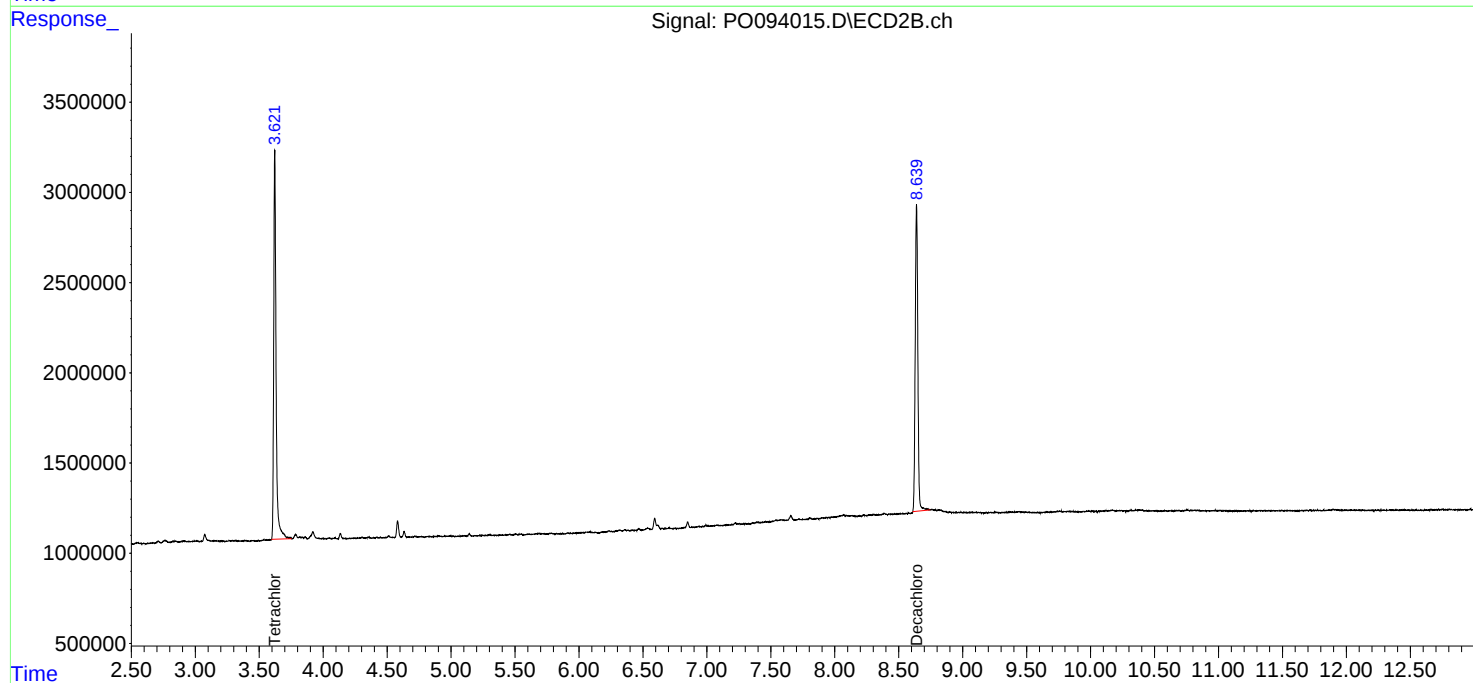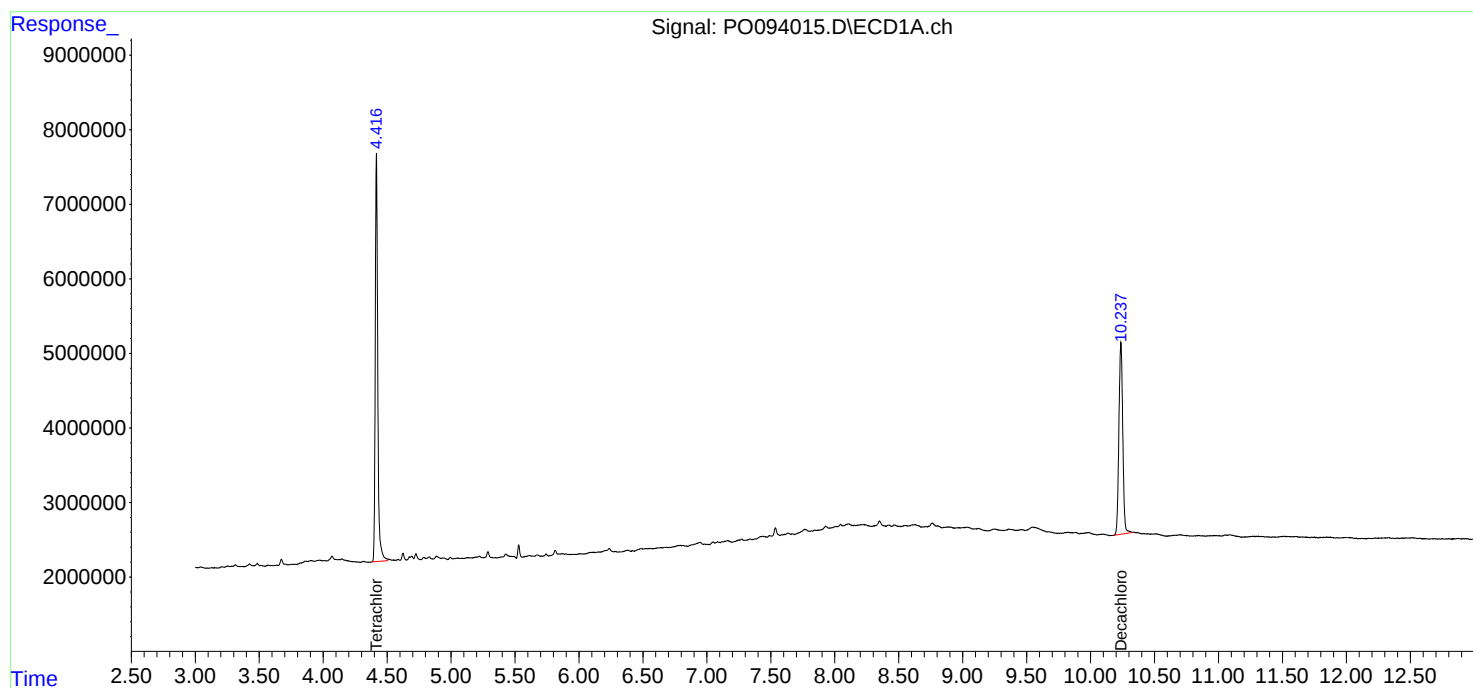

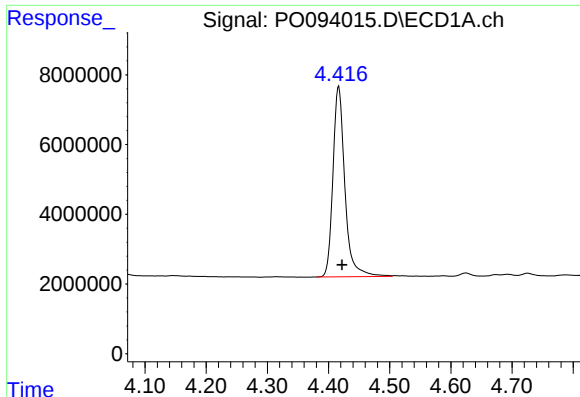

#1 Tetrachloro-m-xylene


R.T.: 4.417 min
Delta R.T.: -0.005 min
Response: 74070694
Conc: 19.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU3-FC-BACKFILL-04

Manual Integrations
APPROVED


Reviewed By :Yogesh
Patel
04/10/2023

Supervised By :Ankita
Jodhani
04/10/2023

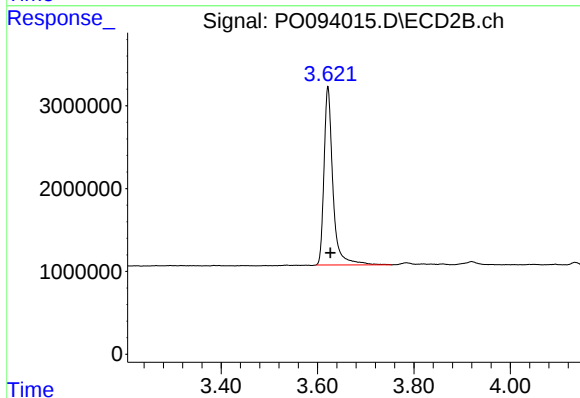


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.005 min
Response: 27587820
Conc: 21.66 ng/ml

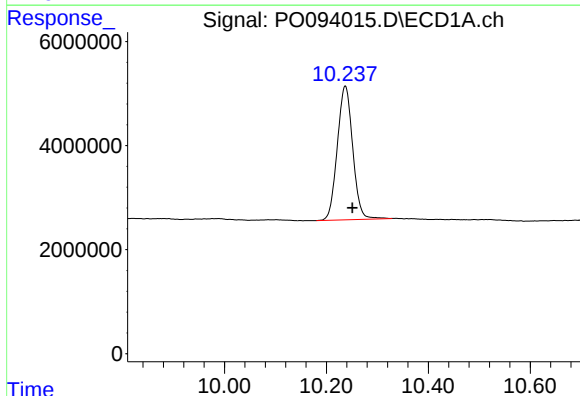

#2 Decachlorobiphenyl

R.T.: 10.237 min
Delta R.T.: -0.014 min
Response: 53957367
Conc: 24.12 ng/ml m

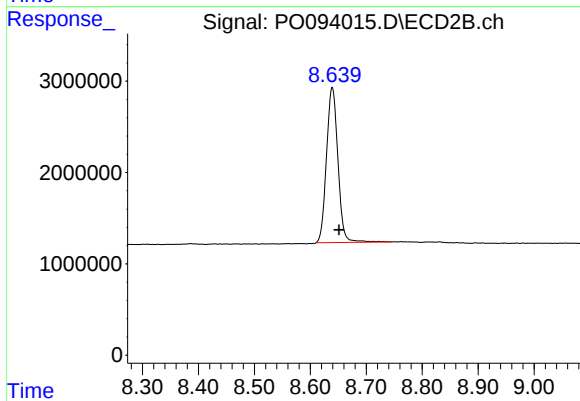

#2 Decachlorobiphenyl

R.T.: 8.639 min
Delta R.T.: -0.012 min
Response: 24120264
Conc: 24.13 ng/ml