

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040825\
Data File : P0110306.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2025 14:12
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 14:20:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	3.690	3.687	165.6E6	91042032	18.193	17.361
2) SA Decachlor...	8.739	8.691	141.3E6	37124521	18.373	15.302

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040825\
Data File : PO110306.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2025 14:12
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 14:20:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 19 02:52:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

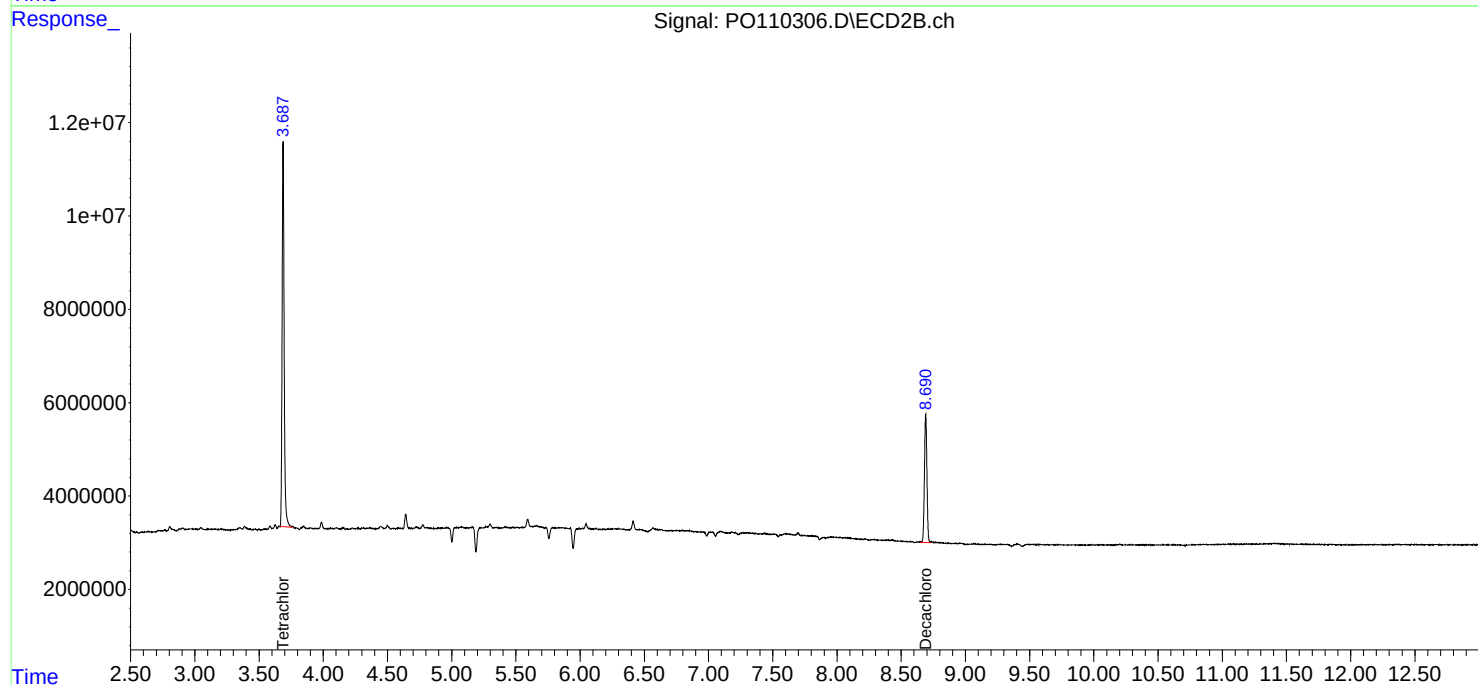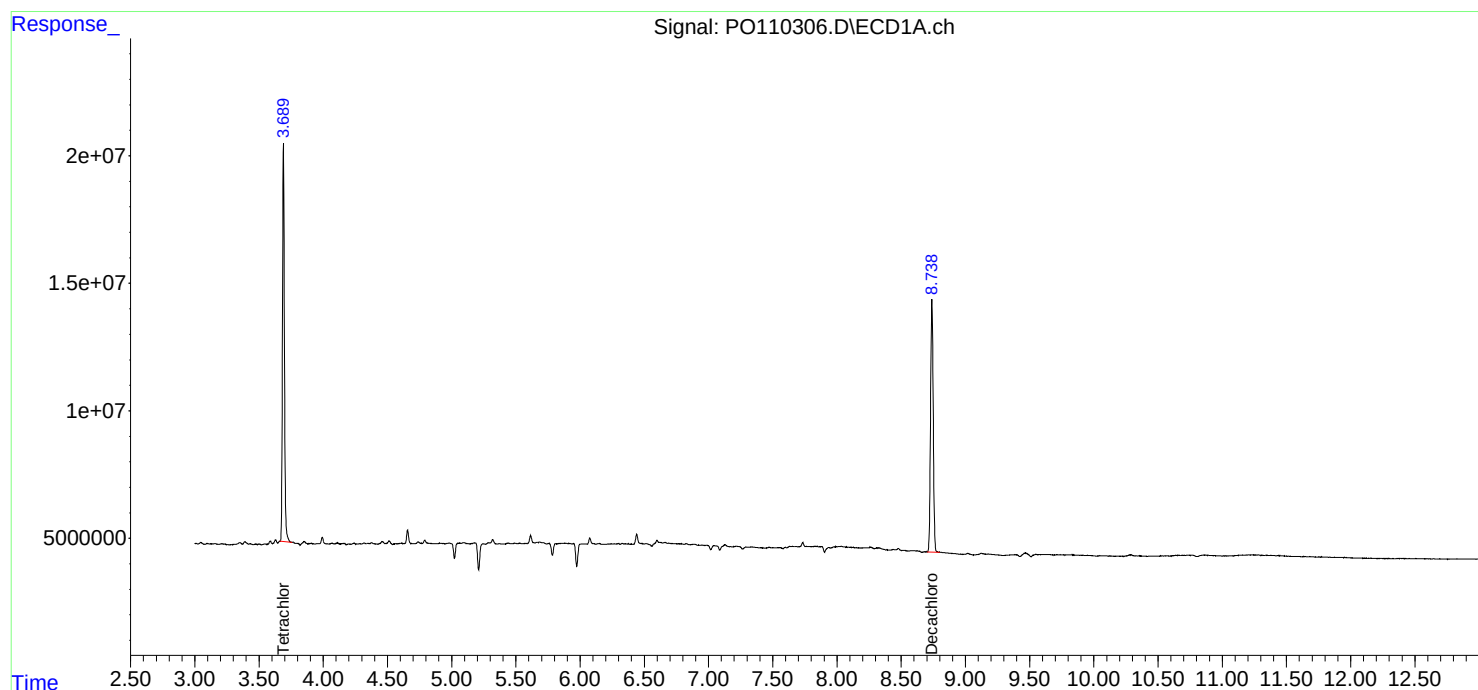


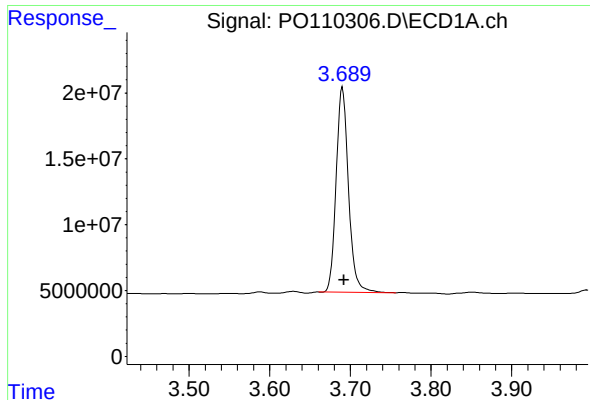

#1 Tetrachloro-m-xylene


R.T.: 3.690 min
Delta R.T.: -0.002 min
Response: 165584494
Conc: 18.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

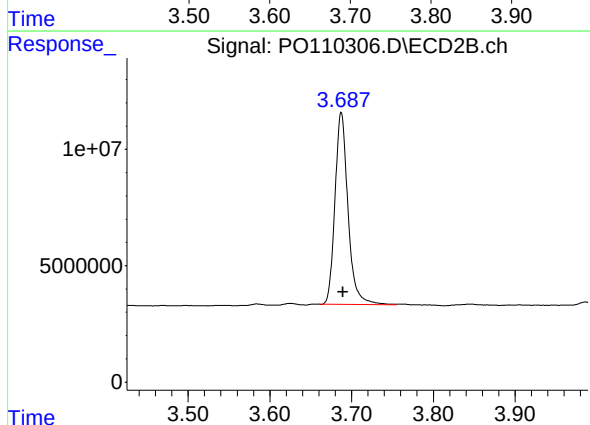


#1 Tetrachloro-m-xylene

R.T.: 3.687 min
Delta R.T.: -0.002 min
Response: 91042032
Conc: 17.36 ng/ml

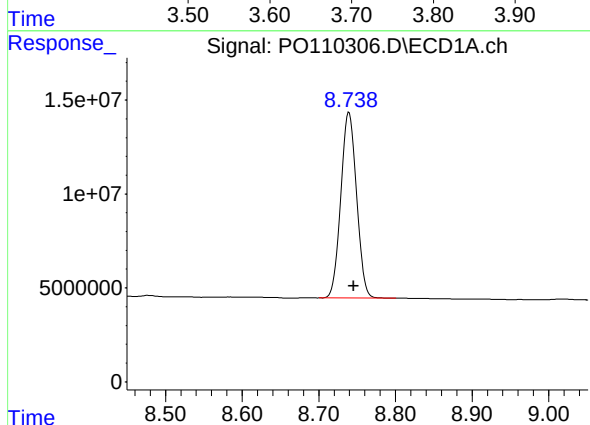

#2 Decachlorobiphenyl

R.T.: 8.739 min
Delta R.T.: -0.006 min
Response: 141264866
Conc: 18.37 ng/ml

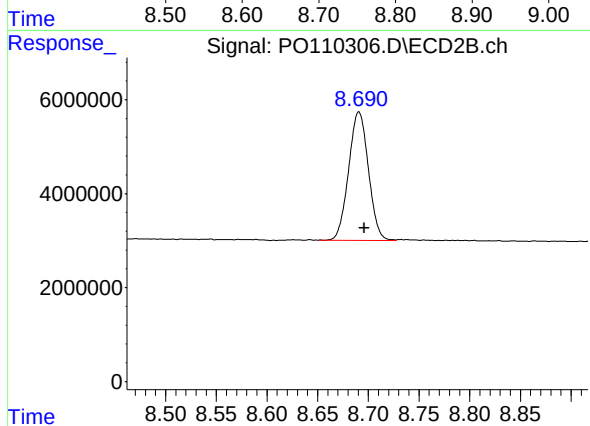

#2 Decachlorobiphenyl

R.T.: 8.691 min
Delta R.T.: -0.005 min
Response: 37124521
Conc: 15.30 ng/ml