

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040920\
 Data File : P0067768.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Apr 2020 9:45
 Operator : DD\AJ
 Sample : PB128100TB
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 09 13:11:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 03 16:04:09 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.933	3.943	582343	853636	24.454	25.469
2)	SA Decachlor...	10.917	9.230	752320	887289	22.099	21.460
Target Compounds							
28)	L6 AR-1254-3	7.788	0.000	14859	0	7.160	N.D. #
29)	L6 AR-1254-4	0.000	6.946	0	35046	N.D.	14.538 #
32)	L7 AR-1260-2	0.000	6.946	0	35046	N.D.	13.649 #
38)	L8 AR-1262-3	9.441	0.000	108628	0	52.204	N.D. #
39)	L8 AR-1262-4	9.487	0.000	13542	0	8.558	N.D. #
41)	L9 AR-1268-1	9.441	0.000	108628	0	29.397	N.D. #
42)	L9 AR-1268-2	9.487	0.000	13542	0	3.907	N.D. #
43)	L9 AR-1268-3	9.784	0.000	57124	0	19.672	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040920\
Data File : P0067768.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Apr 2020 9:45
Operator : DD\AJ
Sample : PB128100TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 09 13:11:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040120.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 03 16:04:09 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

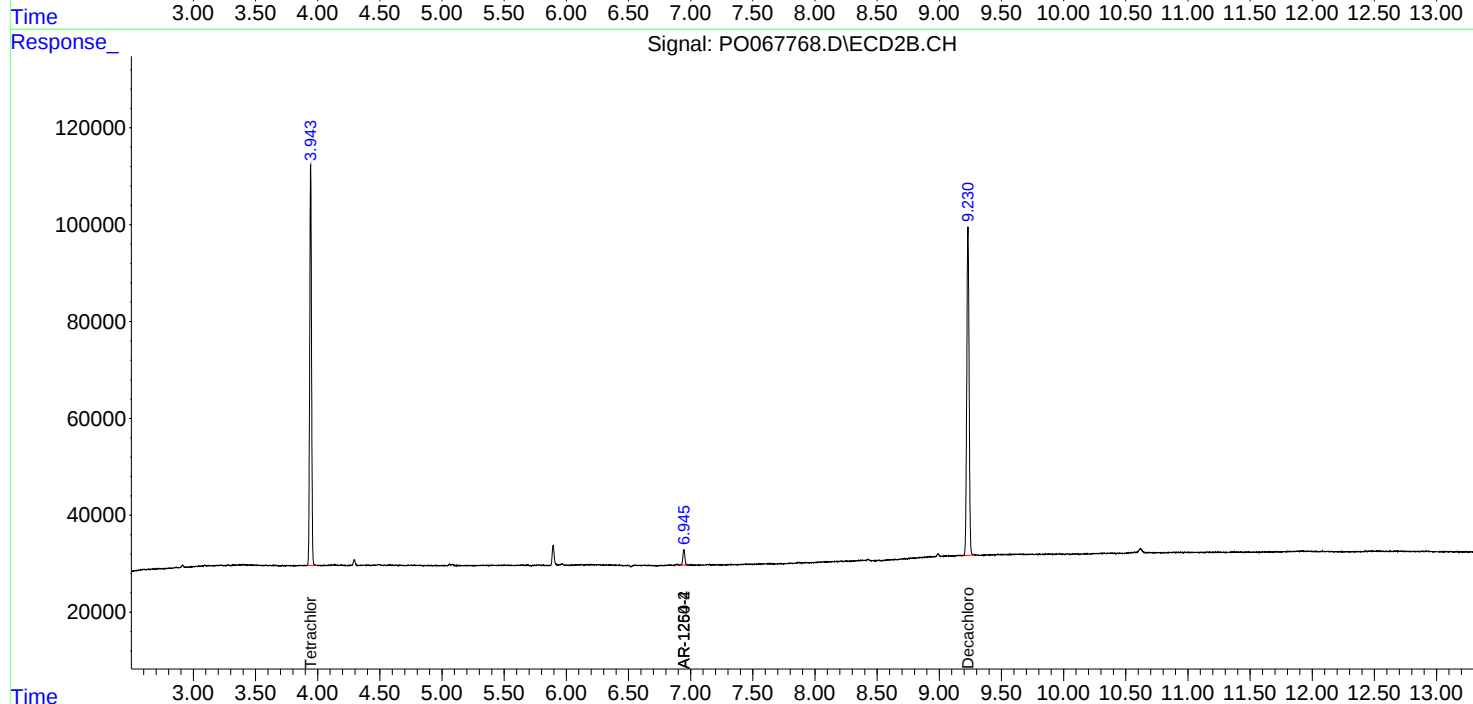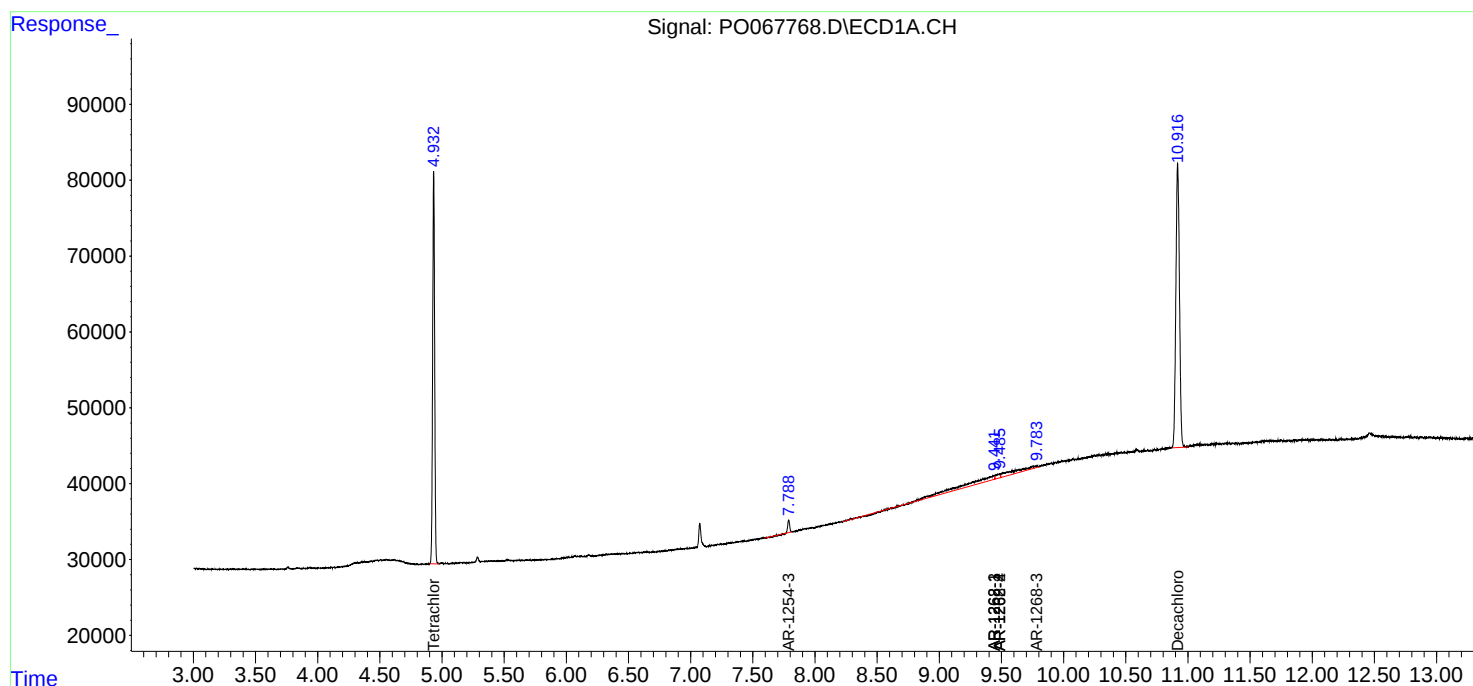


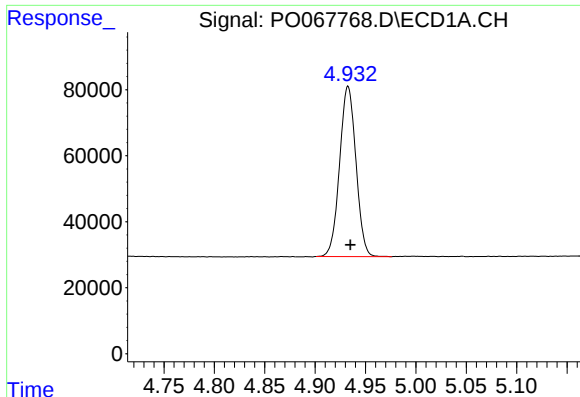

#1 Tetrachloro-m-xylene


R.T.: 4.933 min
Delta R.T.: -0.002 min
Response: 582343
Conc: 24.45 ng/ml

Instrument :
ECD_O
ClientSampleId :

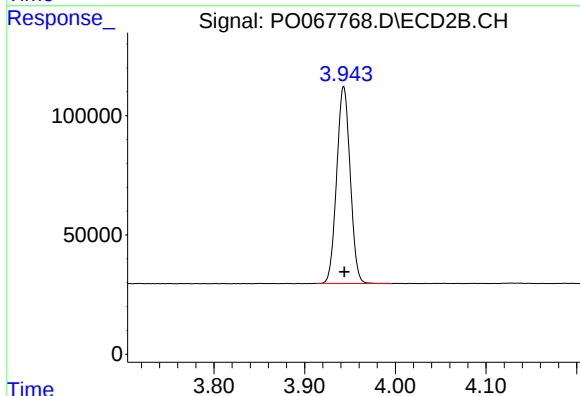


#1 Tetrachloro-m-xylene

R.T.: 3.943 min
Delta R.T.: 0.000 min
Response: 853636
Conc: 25.47 ng/ml

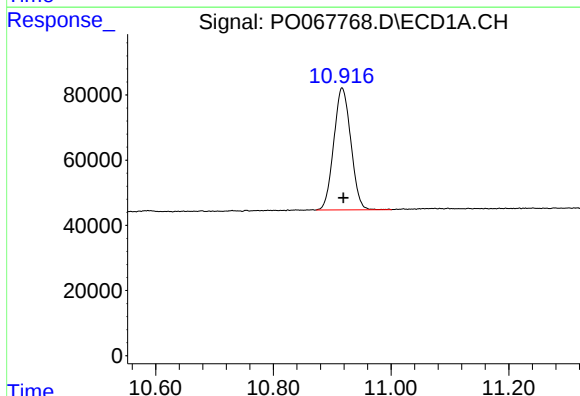


#2 Decachlorobiphenyl

R.T.: 10.917 min
Delta R.T.: -0.002 min
Response: 752320
Conc: 22.10 ng/ml

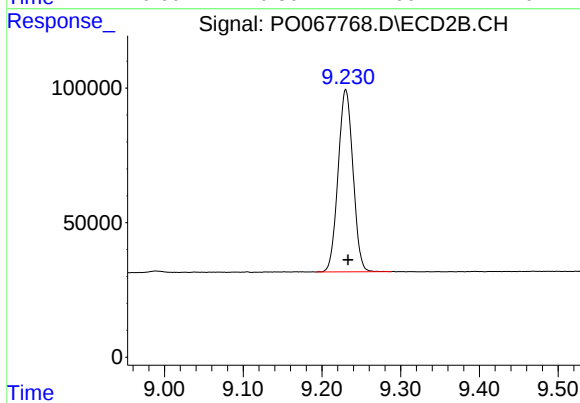

#2 Decachlorobiphenyl


R.T.: 9.230 min
Delta R.T.: -0.003 min
Response: 887289
Conc: 21.46 ng/ml

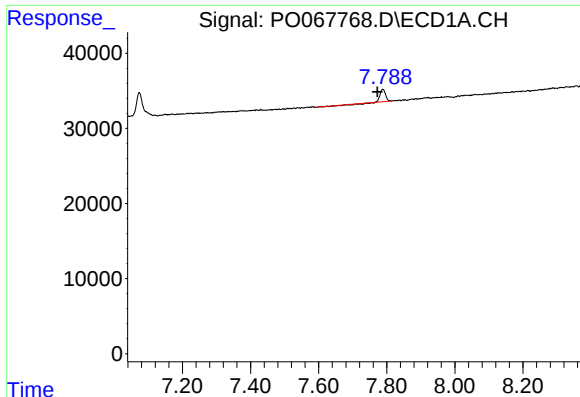

#28 AR-1254-3


R.T.: 7.788 min
Delta R.T.: 0.015 min
Response: 14859
Conc: 7.16 ng/ml

Instrument :
ECD_O
ClientSampleId :

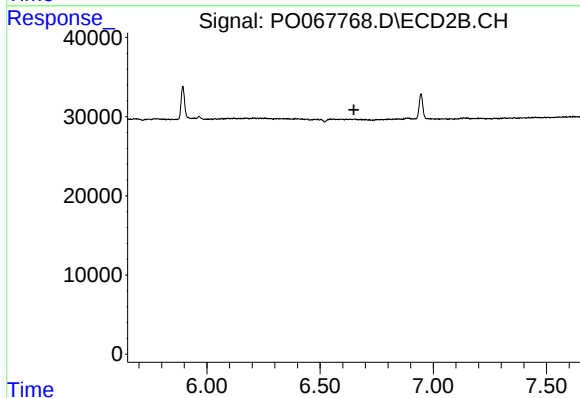


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.649 min
Response: 0
Conc: N.D.

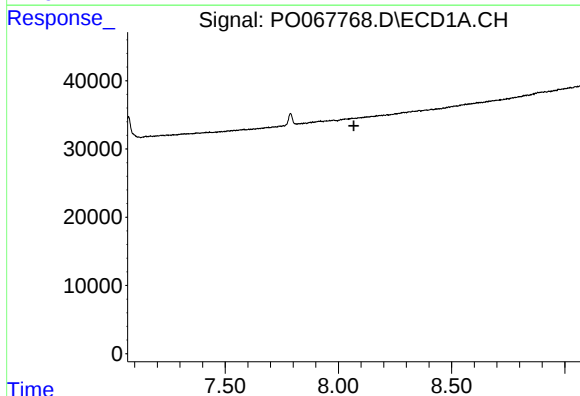


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 8.068 min
Response: 0
Conc: N.D.

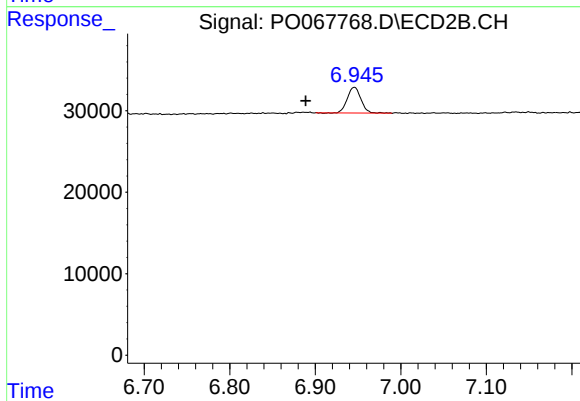

#29 AR-1254-4


R.T.: 6.946 min
Delta R.T.: 0.057 min
Response: 35046
Conc: 14.54 ng/ml

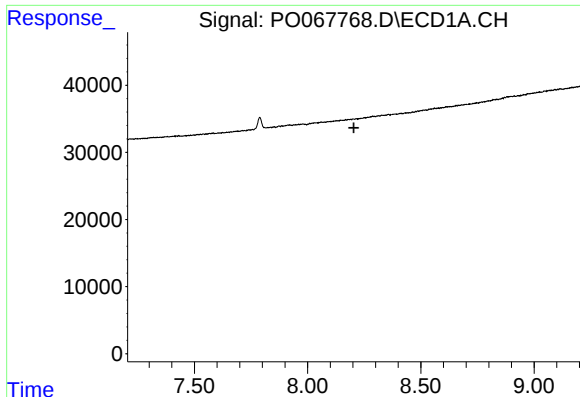

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

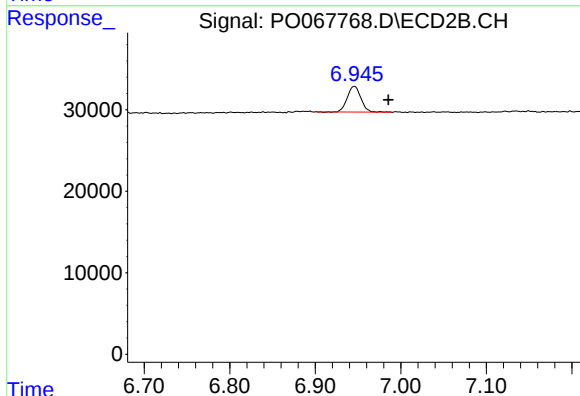


#32 AR-1260-2

R.T.: 6.946 min
Delta R.T.: -0.040 min
Response: 35046
Conc: 13.65 ng/ml

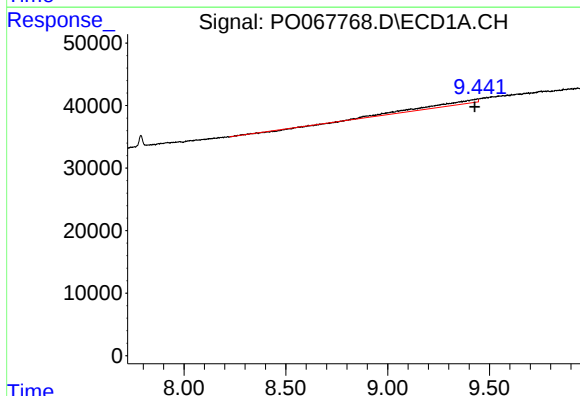


#38 AR-1262-3

R.T.: 9.441 min
Delta R.T.: 0.013 min
Response: 108628
Conc: 52.20 ng/ml

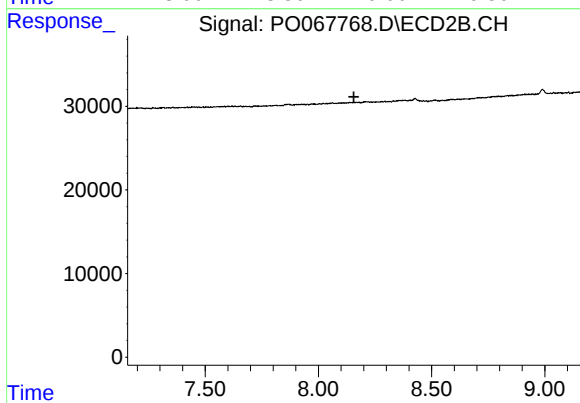

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.157 min
Response: 0
Conc: N.D.

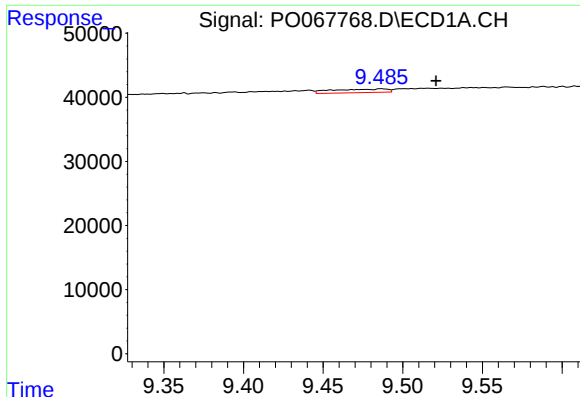

#39 AR-1262-4


R.T.: 9.487 min
Delta R.T.: -0.034 min
Response: 13542
Conc: 8.56 ng/ml

Instrument :
ECD_O
ClientSampleId :

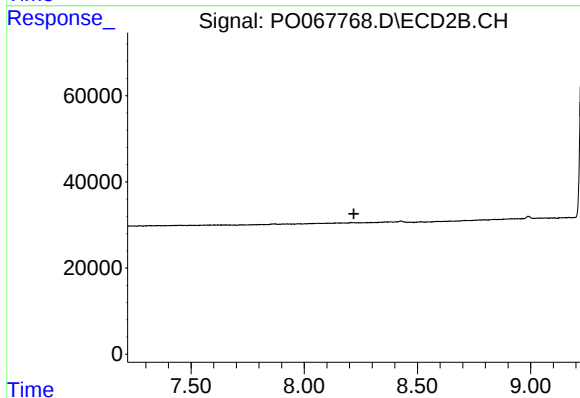


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.219 min
Response: 0
Conc: N.D.

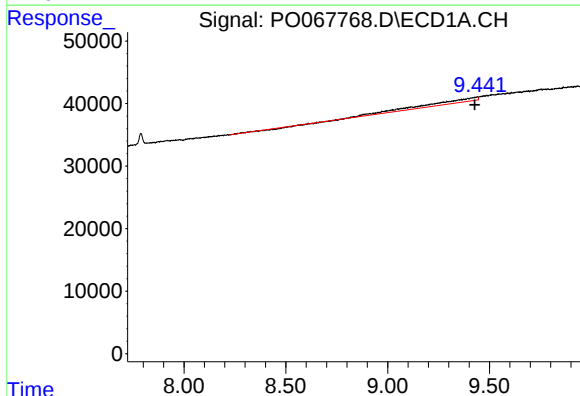


#41 AR-1268-1

R.T.: 9.441 min
Delta R.T.: 0.013 min
Response: 108628
Conc: 29.40 ng/ml

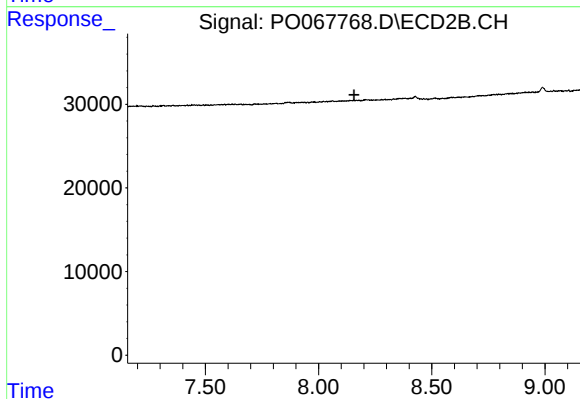

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 8.156 min
Response: 0
Conc: N.D.

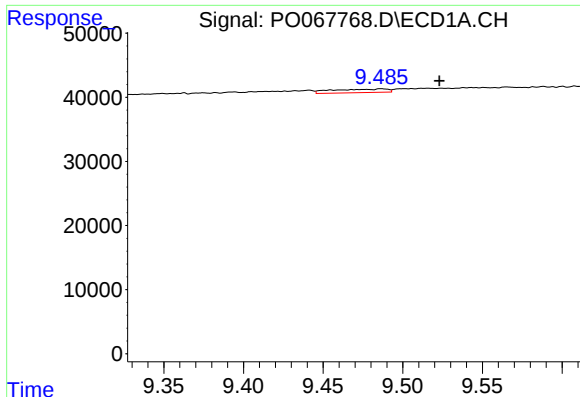

#42 AR-1268-2


R.T.: 9.487 min
Delta R.T.: -0.036 min
Response: 13542
Conc: 3.91 ng/ml

Instrument :
ECD_O
ClientSampleId :

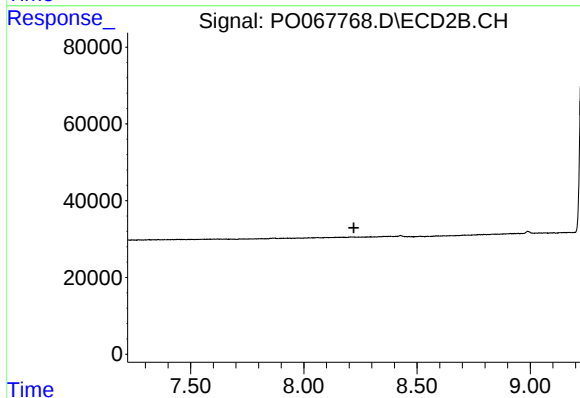


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.221 min
Response: 0
Conc: N.D.

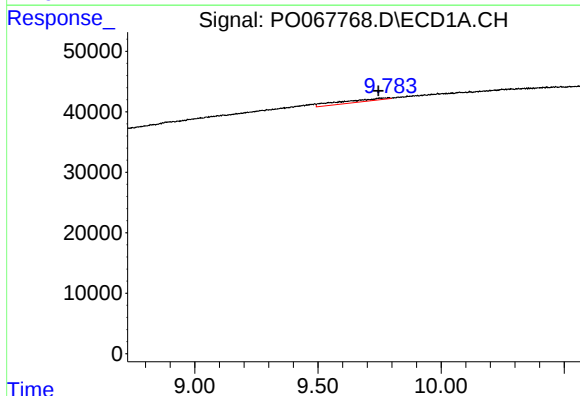

#43 AR-1268-3

R.T.: 9.784 min
Delta R.T.: 0.038 min
Response: 57124
Conc: 19.67 ng/ml

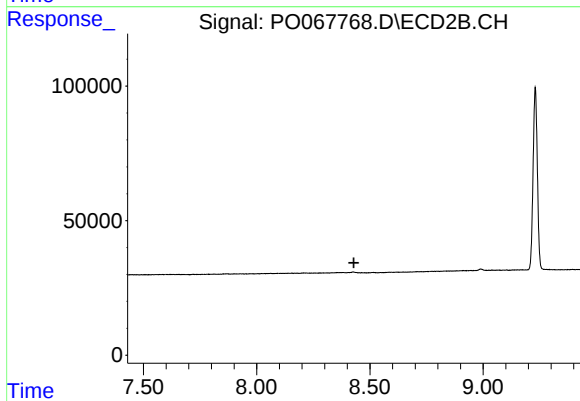

#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 8.430 min
Response: 0
Conc: N.D.