

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0040921\
 Data File : P0076886.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Apr 2021 13:55
 Operator : AJ/MA
 Sample : M1967-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SED-1A

Manual Integrations
 APPROVED

Ankita
 4/12/2021 4:17:16 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 10 08:17:16 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.898	3.896	2228590	1170951	23.960	23.334
2) SA Decachlor...	10.864	9.135	1837108	847211	19.835	17.459
Target Compounds						
26) L6 AR-1254-1	7.130	6.001	75318	57908	23.696	22.093m
27) L6 AR-1254-2	7.358	6.160	173698	38094	33.901	16.635m#
28) L6 AR-1254-3	7.740	6.576	108390	104735	19.670m	29.634m#
29) L6 AR-1254-4	8.034	6.815	52417	26594	13.313m	12.672
30) L6 AR-1254-5	8.463	7.239	151199	81587	34.378	25.027 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO040921\
Data File : PO076886.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Apr 2021 13:55
Operator : AJ/MA
Sample : M1967-01
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
SED-1A


Manual Integrations
APPROVED

Ankita
4/12/2021 4:17:16 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 10 08:17:16 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

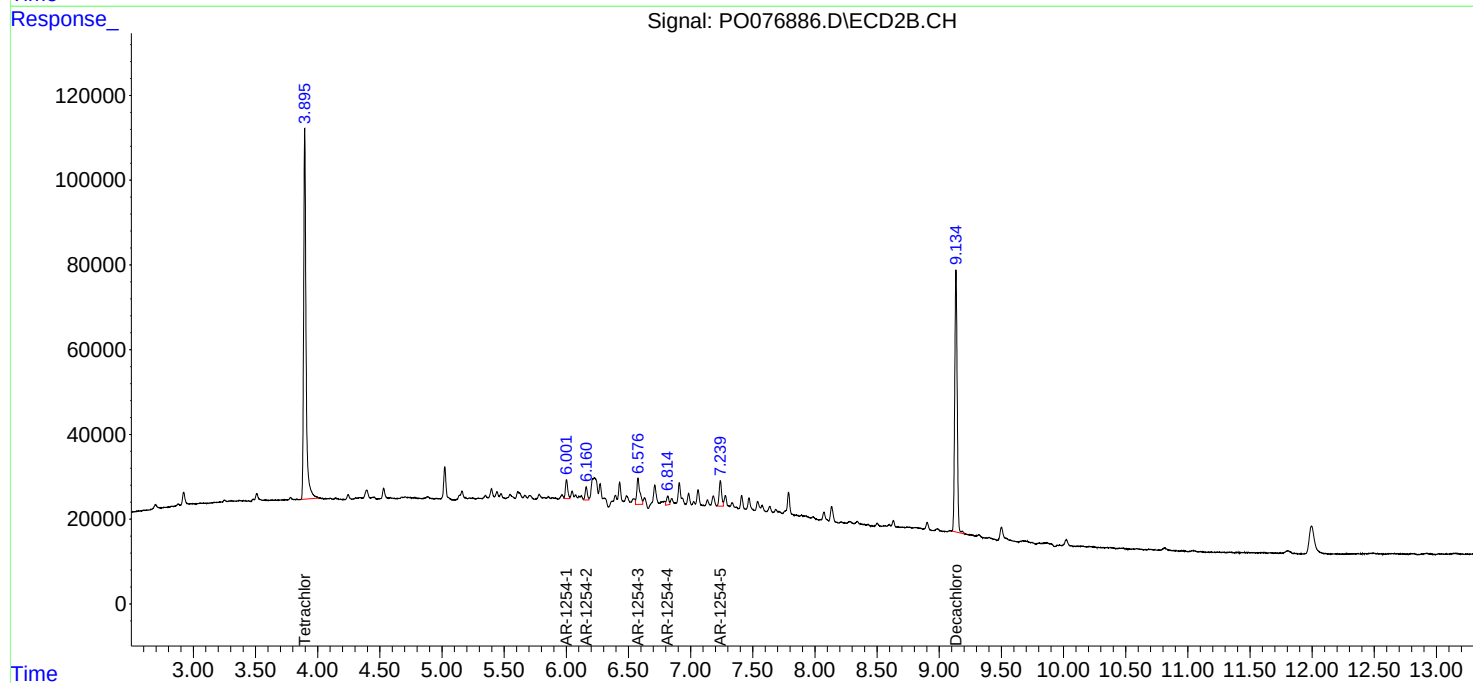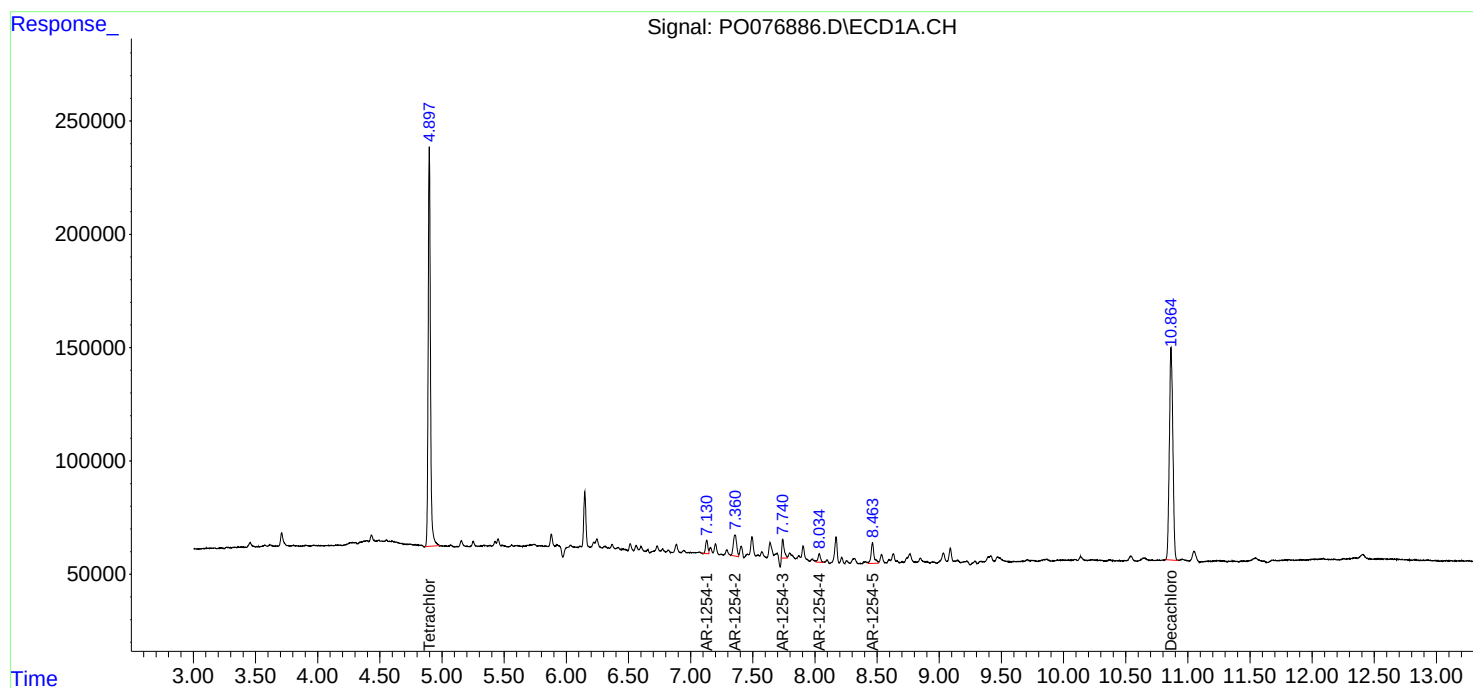

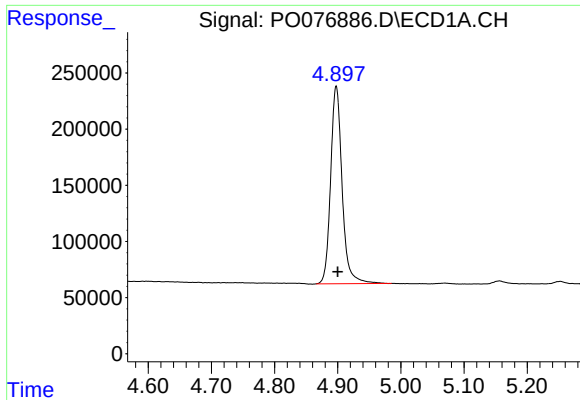


#1 Tetrachloro-m-xylene

R.T.: 4.898 min
Delta R.T.: -0.002 min
Response: 2228590
Conc: 23.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
SED-1A


Manual Integrations
APPROVED

Ankita
4/12/2021 4:17:16 PM

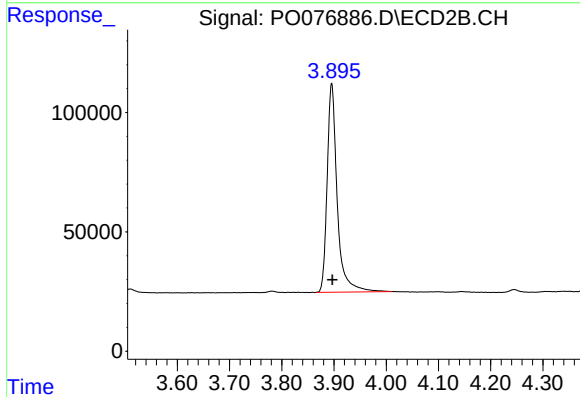


#1 Tetrachloro-m-xylene

R.T.: 3.896 min
Delta R.T.: -0.001 min
Response: 1170951
Conc: 23.33 ng/ml

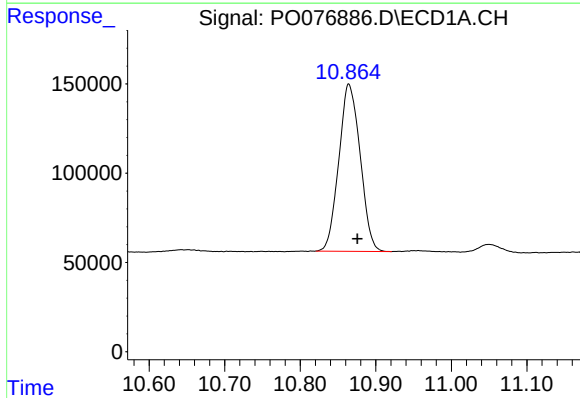


#2 Decachlorobiphenyl

R.T.: 10.864 min
Delta R.T.: -0.011 min
Response: 1837108
Conc: 19.83 ng/ml

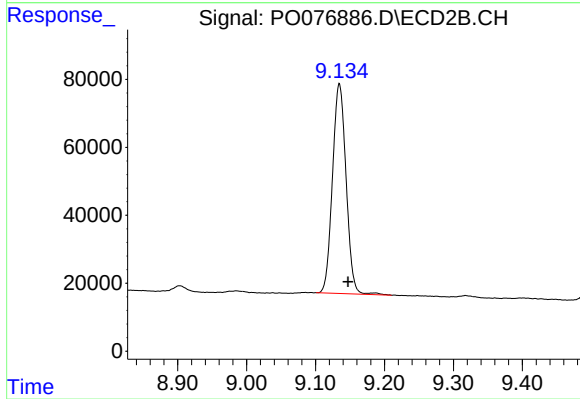

#2 Decachlorobiphenyl

R.T.: 9.135 min
Delta R.T.: -0.013 min
Response: 847211
Conc: 17.46 ng/ml

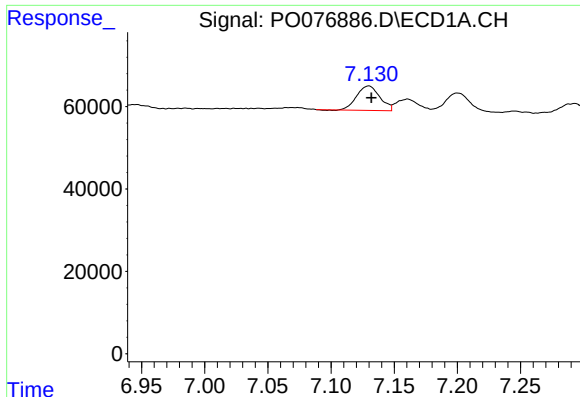


#26 AR-1254-1

R.T.: 7.130 min
Delta R.T.: -0.002 min
Response: 75318
Conc: 23.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
SED-1A


Manual Integrations
APPROVED

Ankita
4/12/2021 4:17:16 PM

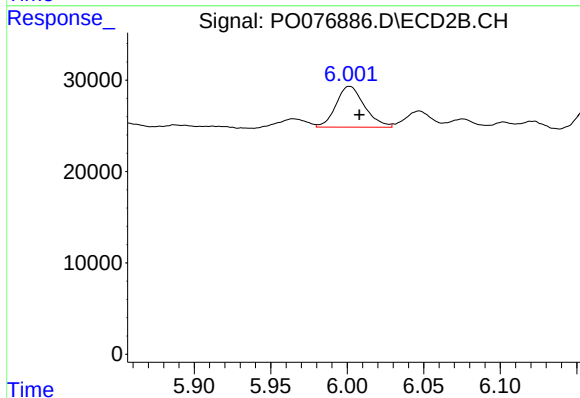


#26 AR-1254-1

R.T.: 6.001 min
Delta R.T.: -0.007 min
Response: 57908
Conc: 22.09 ng/ml m

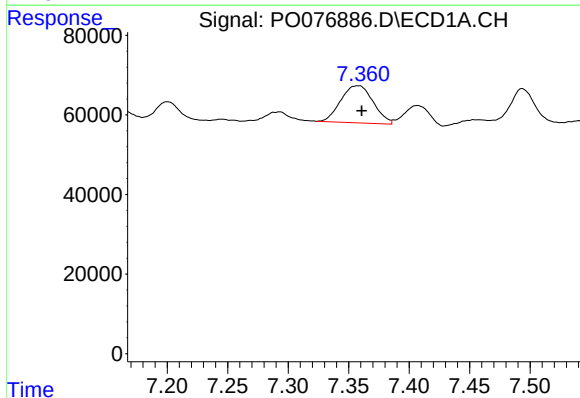


#27 AR-1254-2

R.T.: 7.358 min
Delta R.T.: -0.003 min
Response: 173698
Conc: 33.90 ng/ml

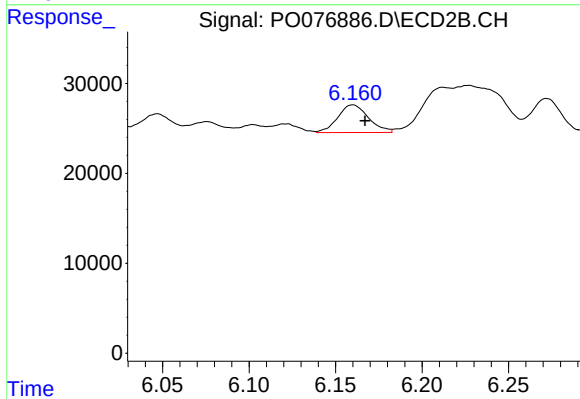

#27 AR-1254-2

R.T.: 6.160 min
Delta R.T.: -0.007 min
Response: 38094
Conc: 16.63 ng/ml m

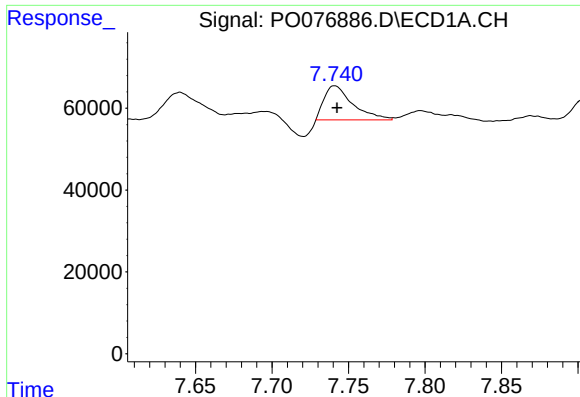


#28 AR-1254-3

R.T.: 7.740 min
Delta R.T.: -0.002 min
Response: 108390
Conc: 19.67 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SED-1A


Manual Integrations
APPROVED

Ankita
4/12/2021 4:17:16 PM

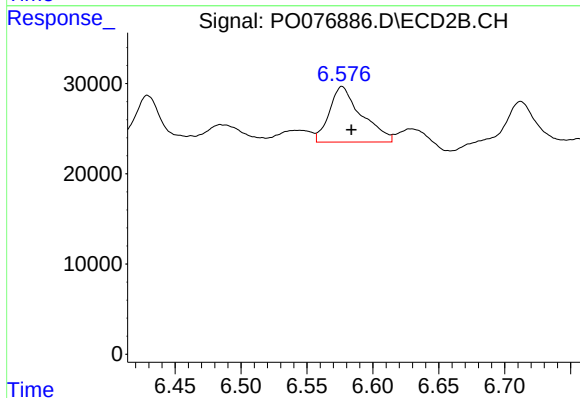


#28 AR-1254-3

R.T.: 6.576 min
Delta R.T.: -0.008 min
Response: 104735
Conc: 29.63 ng/ml m

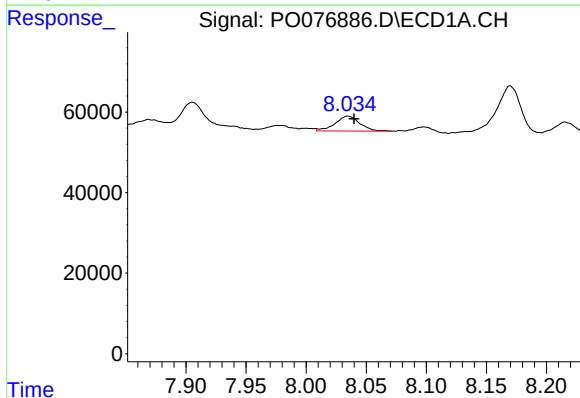


#29 AR-1254-4

R.T.: 8.034 min
Delta R.T.: -0.006 min
Response: 52417
Conc: 13.31 ng/ml m

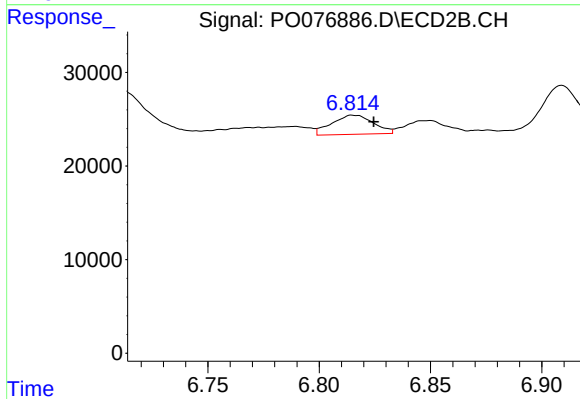

#29 AR-1254-4

R.T.: 6.815 min
Delta R.T.: -0.009 min
Response: 26594
Conc: 12.67 ng/ml

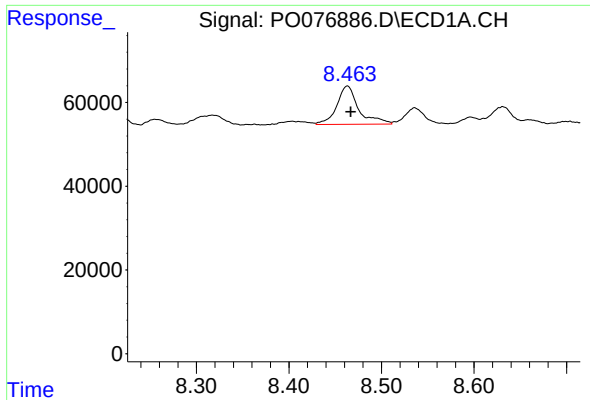


#30 AR-1254-5

R.T.: 8.463 min
Delta R.T.: -0.004 min
Response: 151199
Conc: 34.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
SED-1A

Manual Integrations
APPROVED

Ankita
4/12/2021 4:17:16 PM

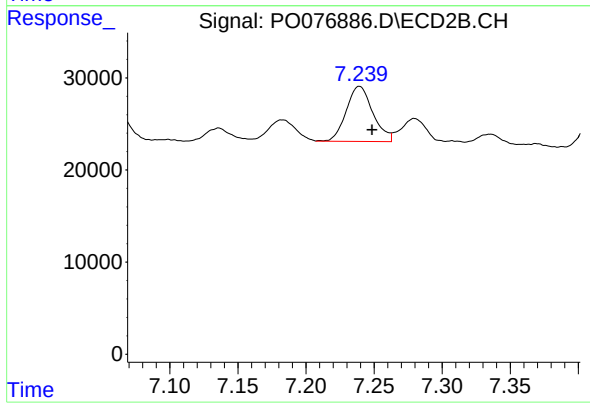

#30 AR-1254-5

R.T.: 7.239 min
Delta R.T.: -0.009 min
Response: 81587
Conc: 25.03 ng/ml