

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041019\
 Data File : P0055119.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Apr 2019 19:50
 Operator : SM/SJ
 Sample : K2342-07
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-11-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 00:59:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.297	3.609	923037	888569	26.597	27.844
2)	SA Decachlor...	9.913	8.579	662641	466906	13.442	14.660
Target Compounds							
7)	L1 AR-1016-5	6.007	0.000	247089	0	185.188	N.D. #
9)	L2 AR-1221-2	4.599	3.907	14142	16083	41.702	53.647 #
23)	L5 AR-1248-3	6.007	0.000	247089	0	154.705	N.D. #
27)	L6 AR-1254-2	6.525	0.000	12041	0	4.218	N.D. #
28)	L6 AR-1254-3	6.899	0.000	17389	0	5.530	N.D. #
31)	L7 AR-1260-1	0.000	6.177	0	1069	N.D.	0.465 #
32)	L7 AR-1260-2	7.305	6.419	12086	8151	3.894	2.961
34)	L7 AR-1260-4	7.879	0.000	7662	0	2.770	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041019\
Data File : P0055119.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Apr 2019 19:50
Operator : SM/SJ
Sample : K2342-07
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP-11-D

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 00:59:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

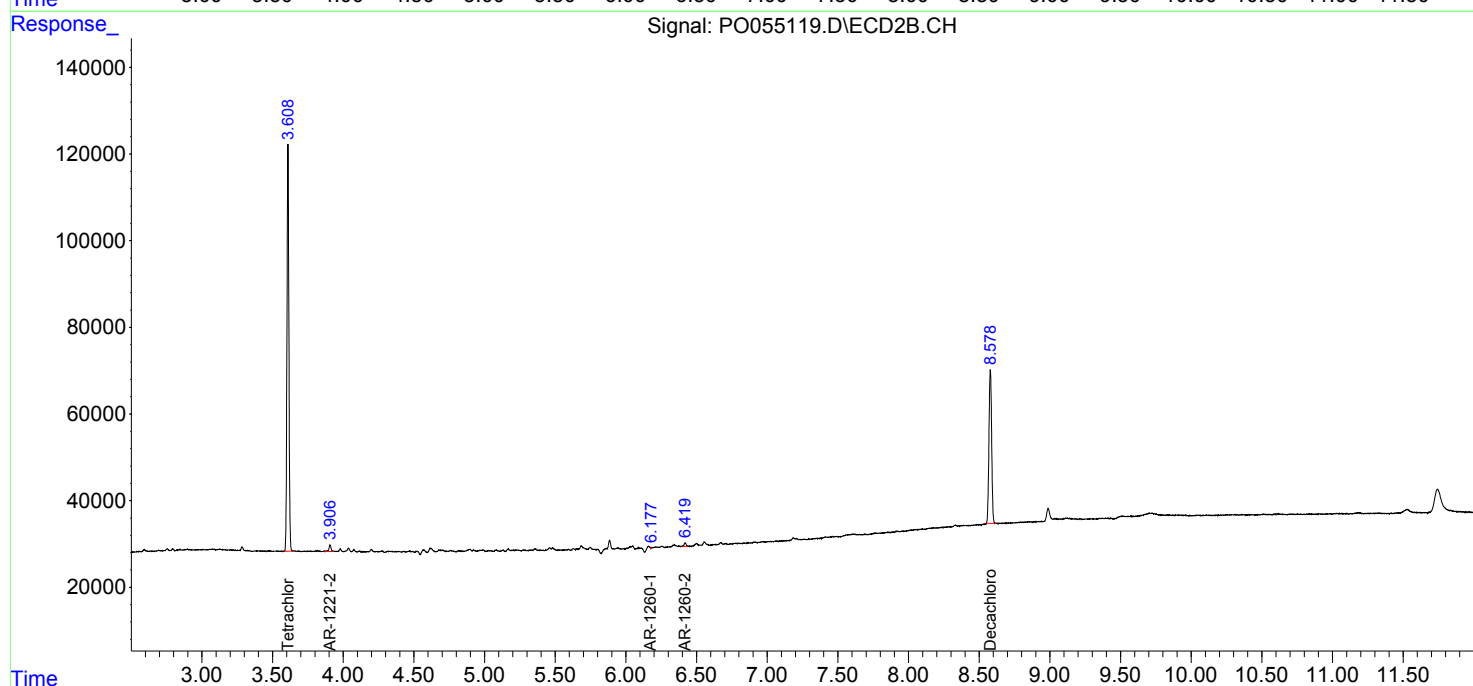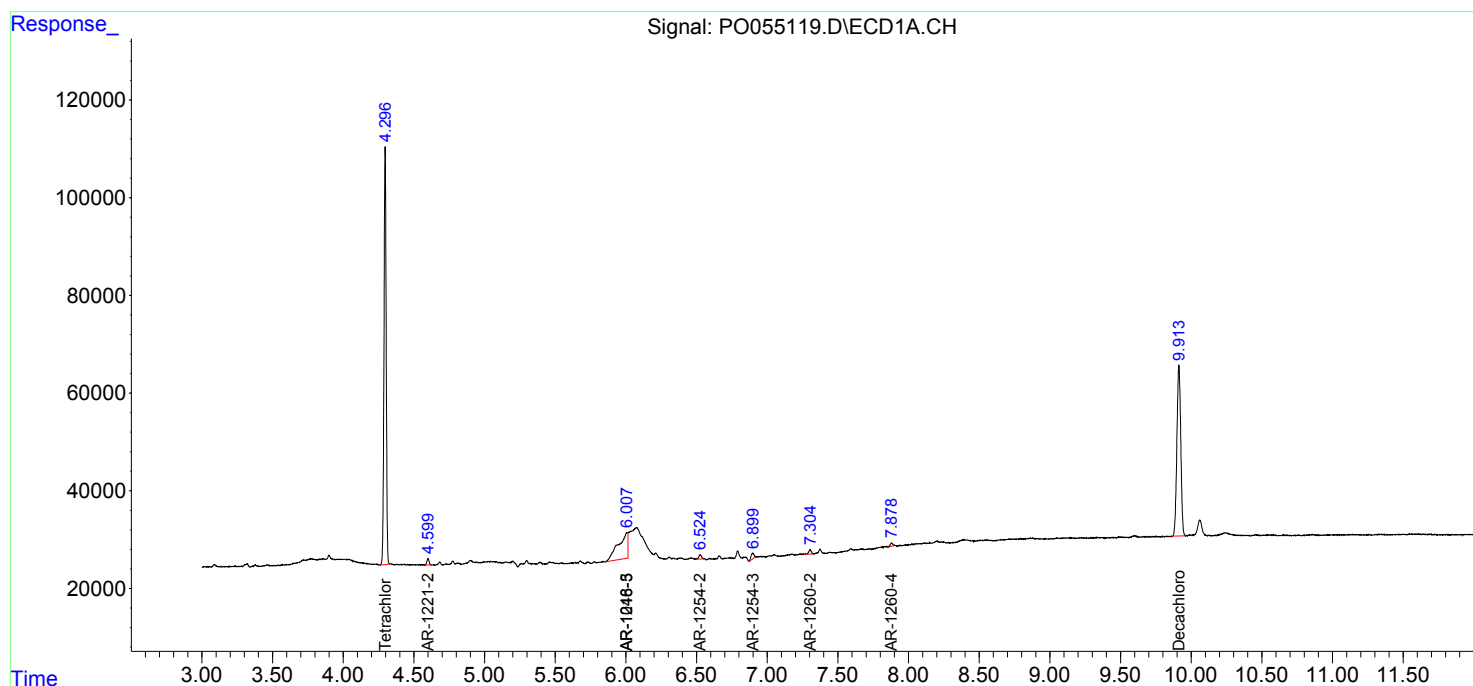


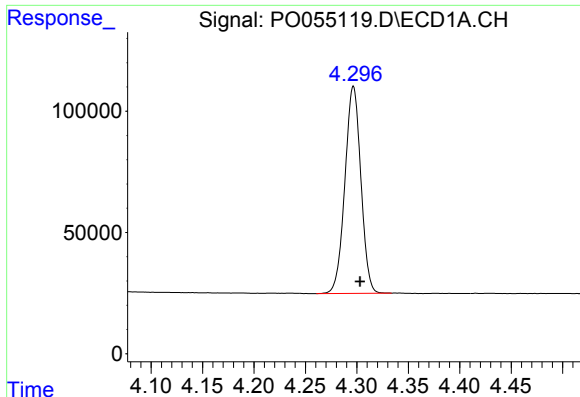

#1 Tetrachloro-m-xylene


R.T.: 4.297 min
Delta R.T.: -0.006 min
Response: 923037
Conc: 26.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-11-D

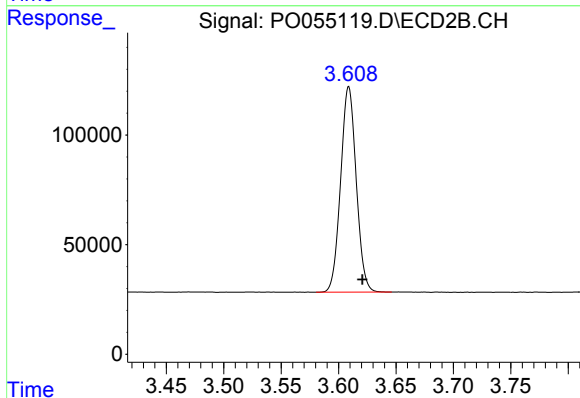


#1 Tetrachloro-m-xylene

R.T.: 3.609 min
Delta R.T.: -0.012 min
Response: 888569
Conc: 27.84 ng/ml

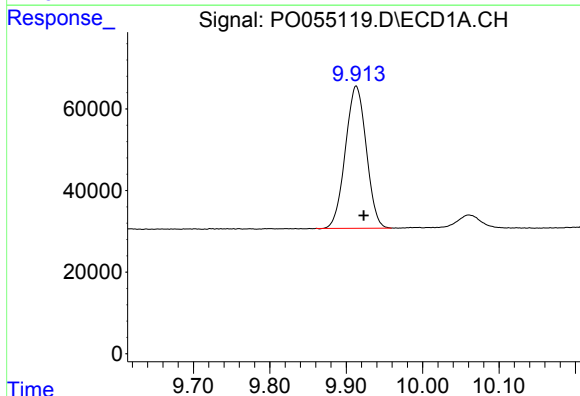


#2 Decachlorobiphenyl

R.T.: 9.913 min
Delta R.T.: -0.010 min
Response: 662641
Conc: 13.44 ng/ml

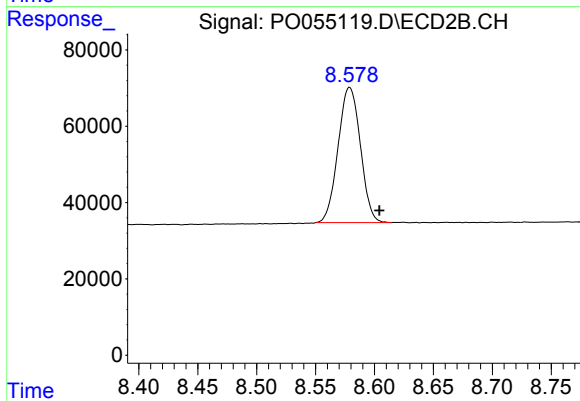

#2 Decachlorobiphenyl


R.T.: 8.579 min
Delta R.T.: -0.025 min
Response: 466906
Conc: 14.66 ng/ml

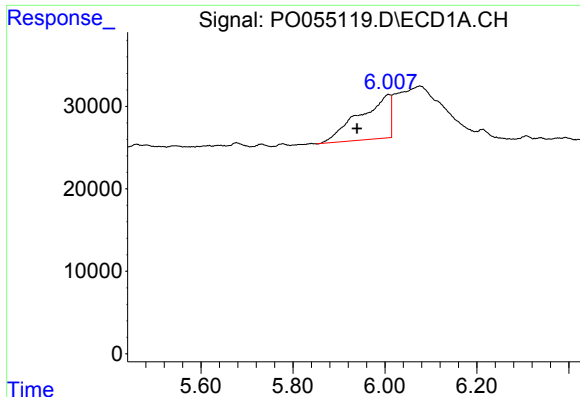

#7 AR-1016-5


R.T.: 6.007 min
Delta R.T.: 0.067 min
Response: 247089
Conc: 185.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-11-D

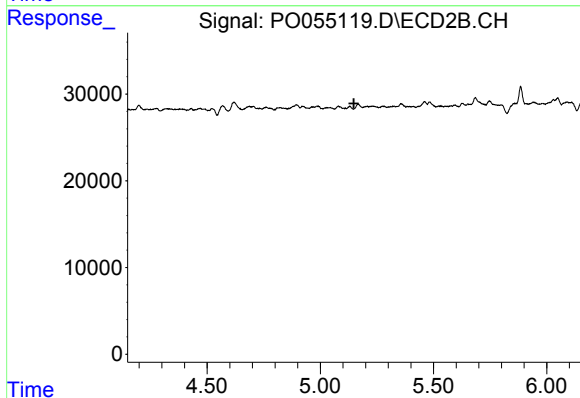


#7 AR-1016-5

R.T.: 0.000 min
Exp R.T. : 5.149 min
Response: 0
Conc: N.D.

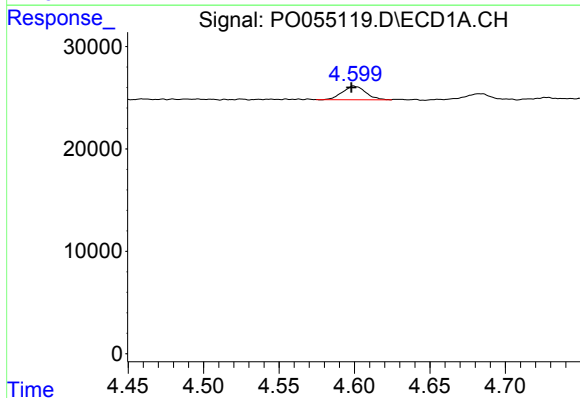


#9 AR-1221-2

R.T.: 4.599 min
Delta R.T.: 0.001 min
Response: 14142
Conc: 41.70 ng/ml

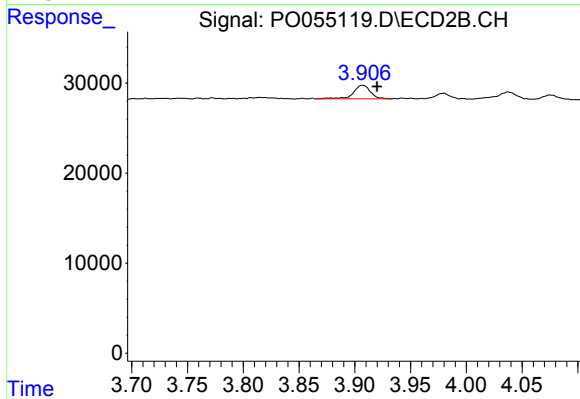

#9 AR-1221-2


R.T.: 3.907 min
Delta R.T.: -0.013 min
Response: 16083
Conc: 53.65 ng/ml

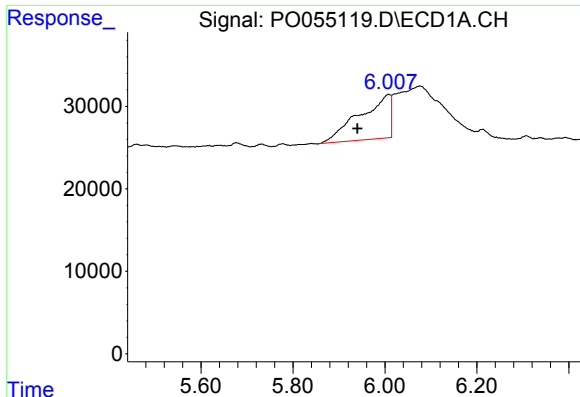

#23 AR-1248-3


R.T.: 6.007 min
Delta R.T.: 0.067 min
Response: 247089
Conc: 154.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-11-D

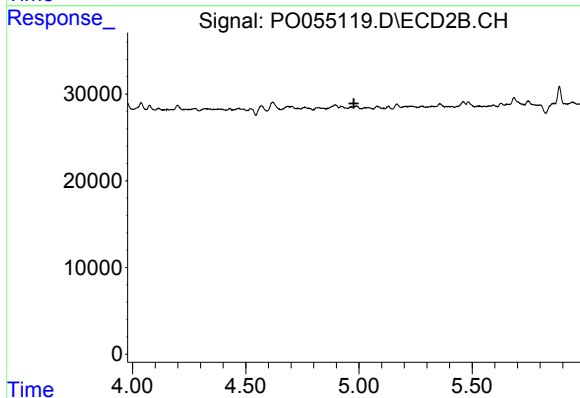


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 4.977 min
Response: 0
Conc: N.D.

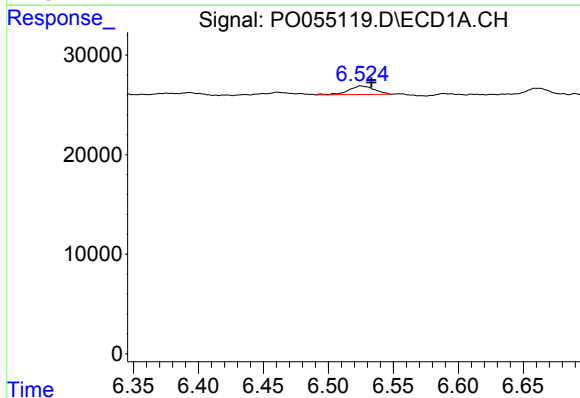


#27 AR-1254-2

R.T.: 6.525 min
Delta R.T.: -0.008 min
Response: 12041
Conc: 4.22 ng/ml

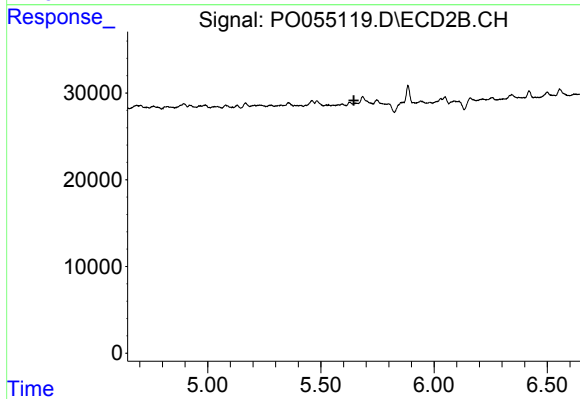

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 5.646 min
Response: 0
Conc: N.D.

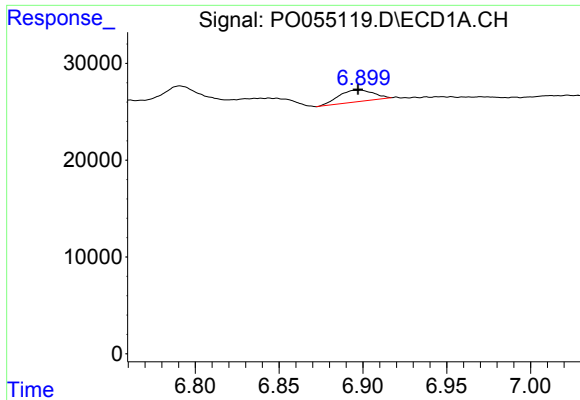

#28 AR-1254-3


R.T.: 6.899 min
Delta R.T.: 0.002 min
Response: 17389
Conc: 5.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-11-D

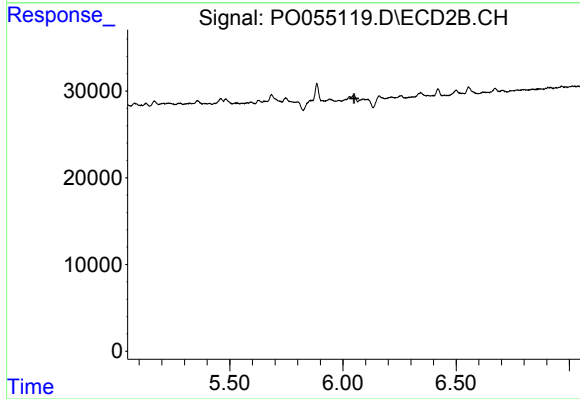


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.049 min
Response: 0
Conc: N.D.

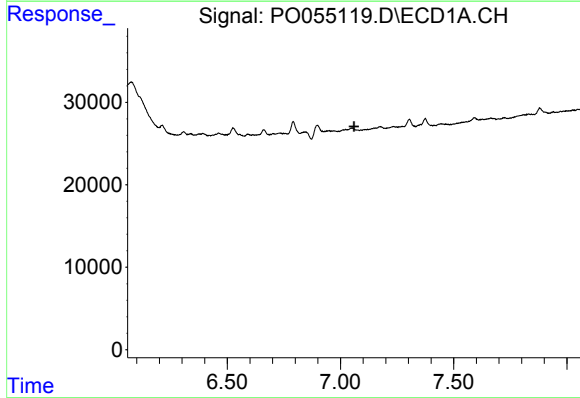


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 7.060 min
Response: 0
Conc: N.D.

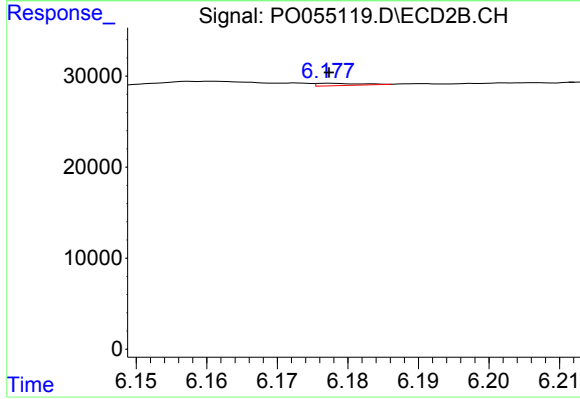

#31 AR-1260-1


R.T.: 6.177 min
Delta R.T.: 0.000 min
Response: 1069
Conc: 0.46 ng/ml

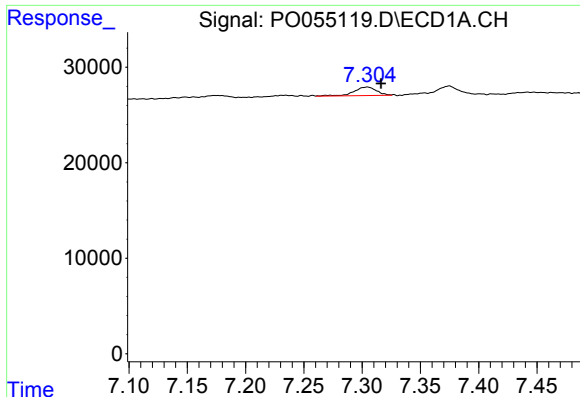

#32 AR-1260-2


R.T.: 7.305 min
Delta R.T.: -0.012 min
Response: 12086
Conc: 3.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-11-D

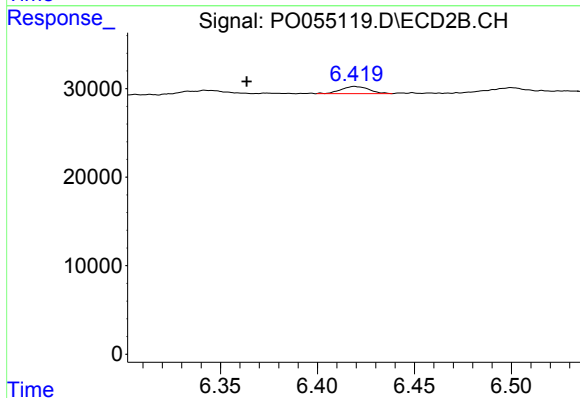


#32 AR-1260-2

R.T.: 6.419 min
Delta R.T.: 0.056 min
Response: 8151
Conc: 2.96 ng/ml

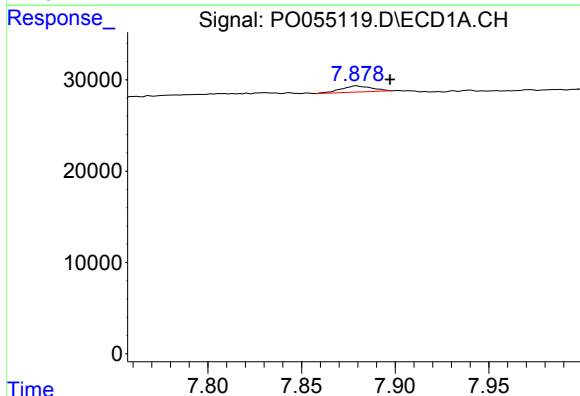

#34 AR-1260-4

R.T.: 7.879 min
Delta R.T.: -0.018 min
Response: 7662
Conc: 2.77 ng/ml

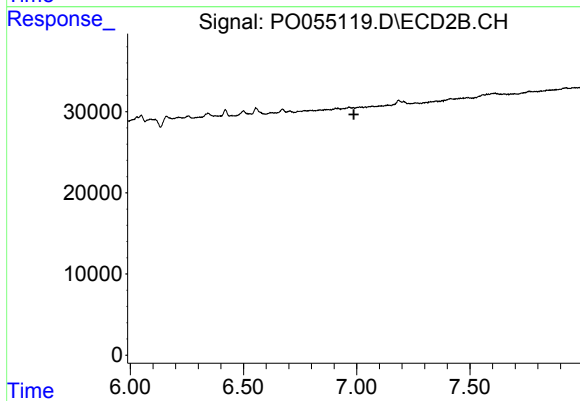

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 6.988 min
Response: 0
Conc: N.D.