

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041019\
 Data File : P0055130.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Apr 2019 22:57
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 01:02:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.296	3.608	979022	941503	28.210	29.503
2) SA Decachlor...	9.912	8.577	1056686	752883	21.435	23.640m

Sohil

4/11/2019 9:16:27 AM

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.



Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041019\
Data File : P0055130.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Apr 2019 22:57
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1


Instrument :
ECD_O
ClientSampleId :
I.BLK

Manual Integrations
APPROVED

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 01:02:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

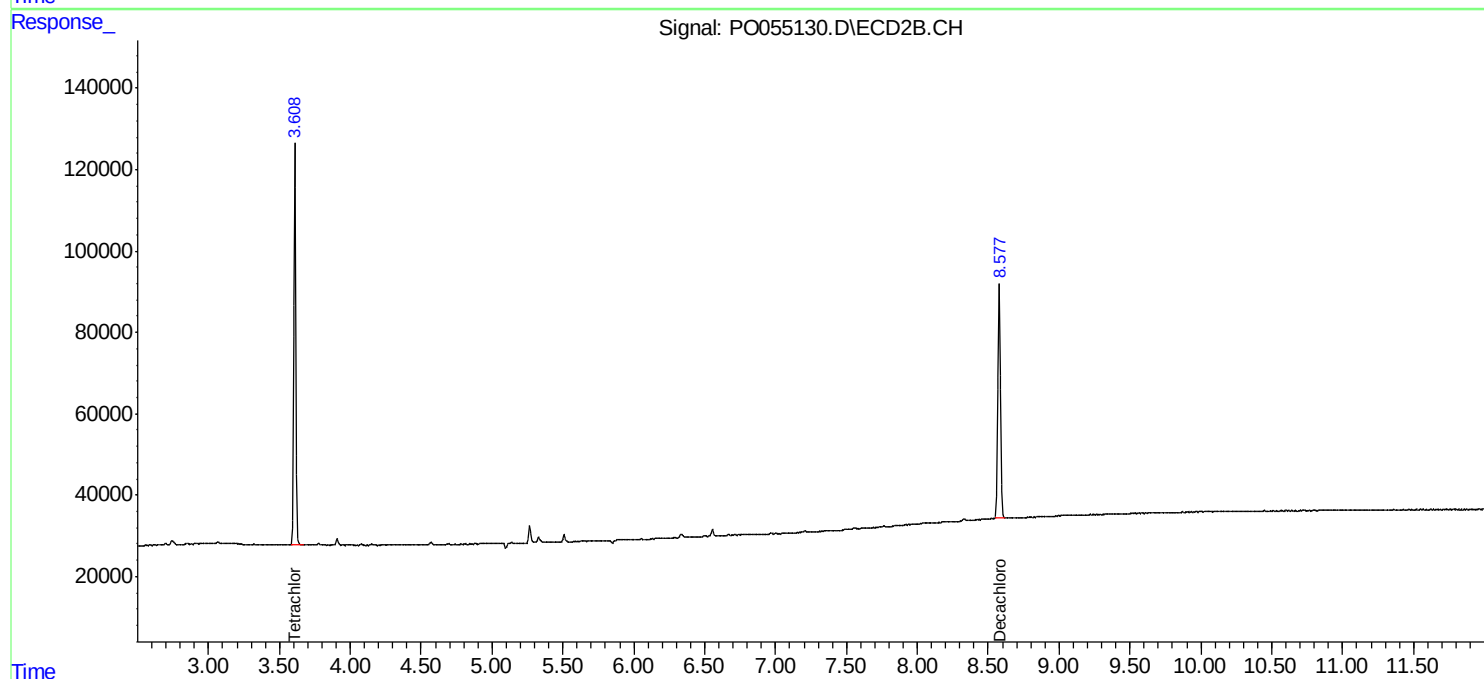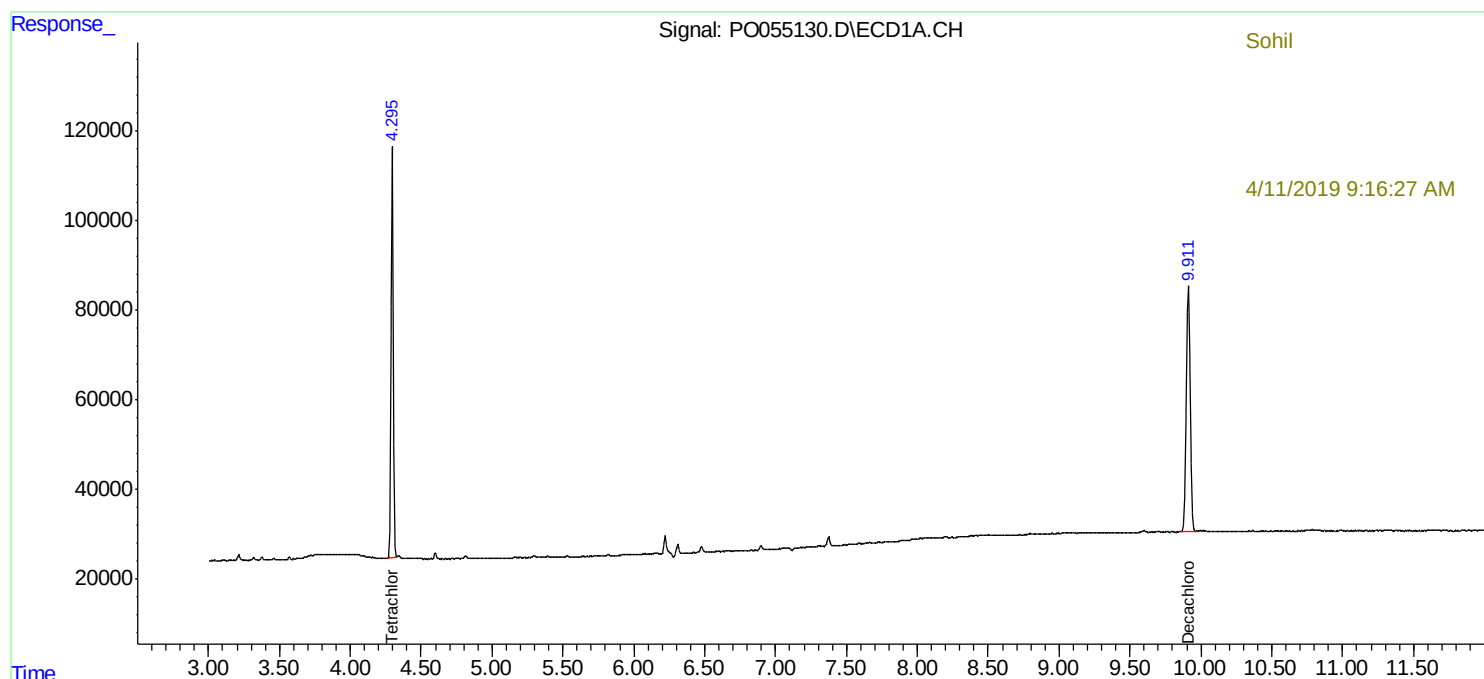

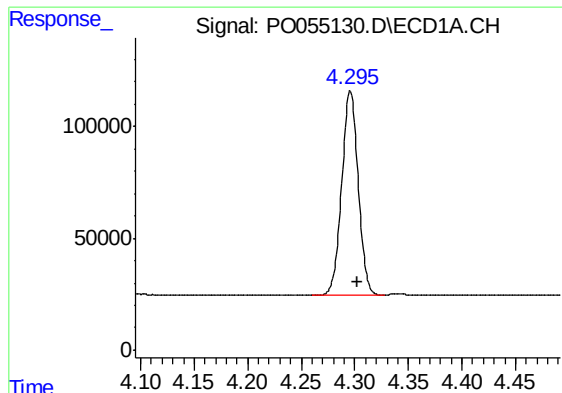


#1 Tetrachloro-m-xylene

R.T.: 4.296 min
Delta R.T.: -0.007 min
Response: 979022
Conc: 28.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

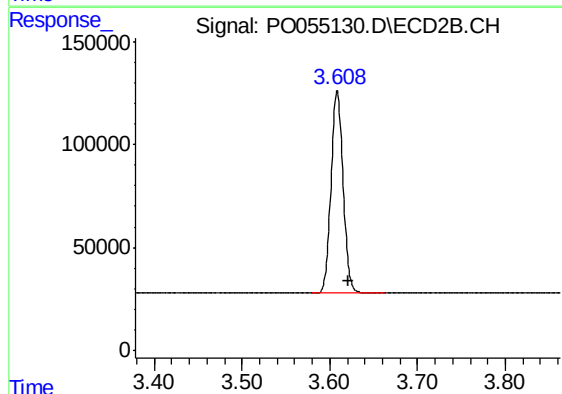

#1 Tetrachloro-m-xylene

R.T.: 3.608 min
Delta R.T.: -0.012 min
Response: 941503
Conc: 29.50 ng/ml


Sohil

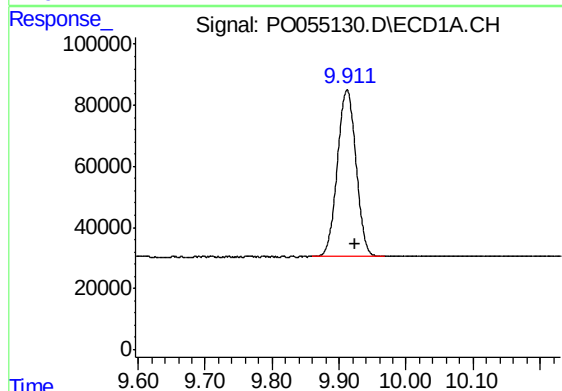

#2 Decachlorobiphenyl

R.T.: 9.912 min
Delta R.T.: -0.011 min
Response: 1056686
Conc: 21.43 ng/ml

4/11/2019 9:16:27 AM

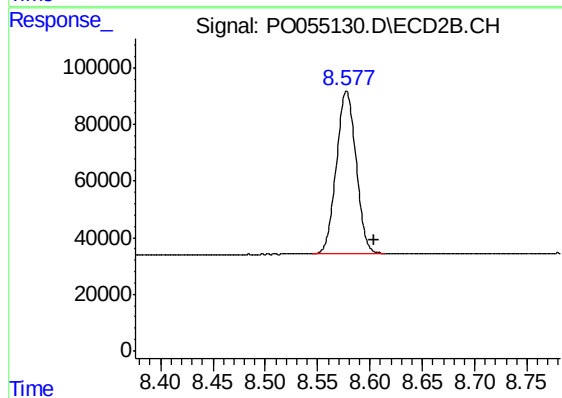

#2 Decachlorobiphenyl

R.T.: 8.577 min
Delta R.T.: -0.027 min
Response: 752883
Conc: 23.64 ng/ml m