

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041019\
 Data File : P0055132.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Apr 2019 23:31
 Operator : SM/SJ
 Sample : IDOC BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 IDOC BL

Manual Integrations
 APPROVED

Sohil
 4/11/2019 9:16:29 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 01:03:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0032519.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Mar 25 17:22:26 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.296	3.609	661261	637964	19.054	19.991
2) SA Decachlor...	9.911	8.577	632752	458391	12.835	14.393m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041019\
Data File : PO055132.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Apr 2019 23:31
Operator : SM/SJ
Sample : IDOC BL
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
IDOC BL


Manual Integrations
APPROVED

Sohil
4/11/2019 9:16:29 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 01:03:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO032519.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Mar 25 17:22:26 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

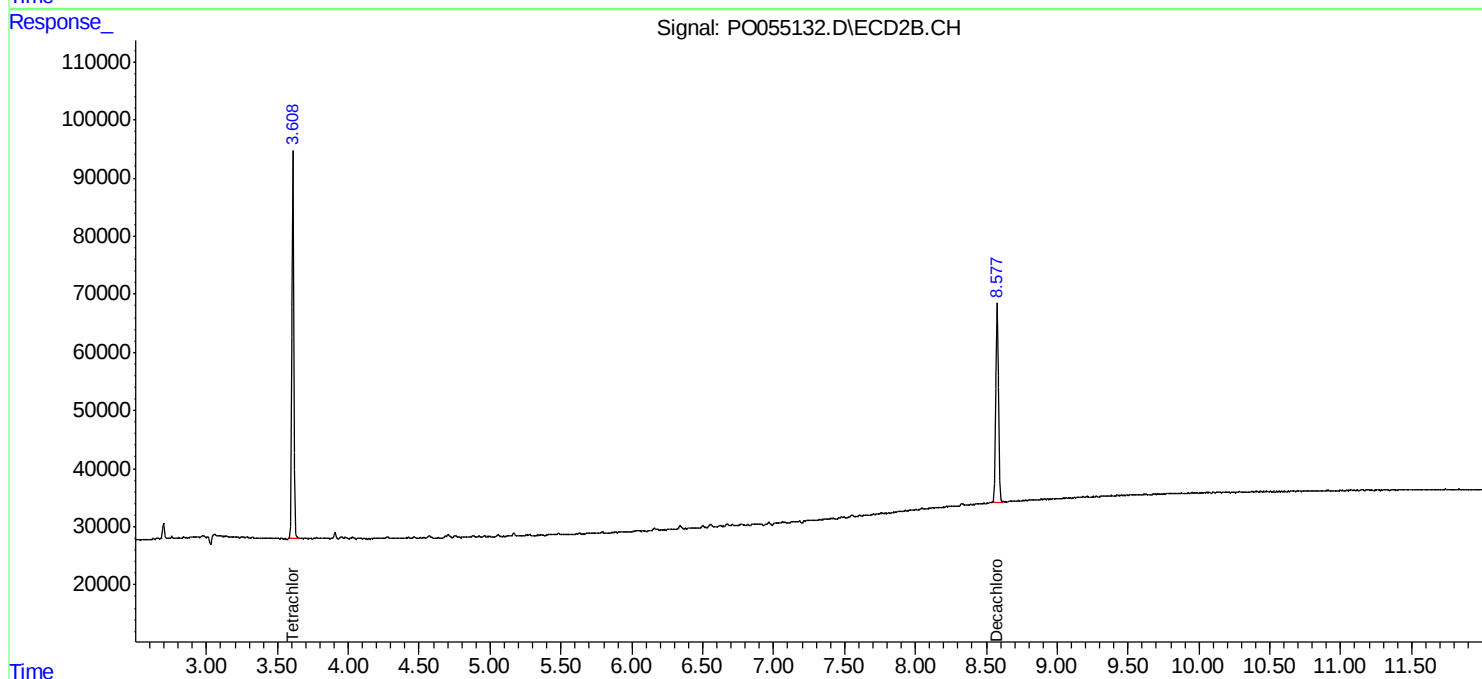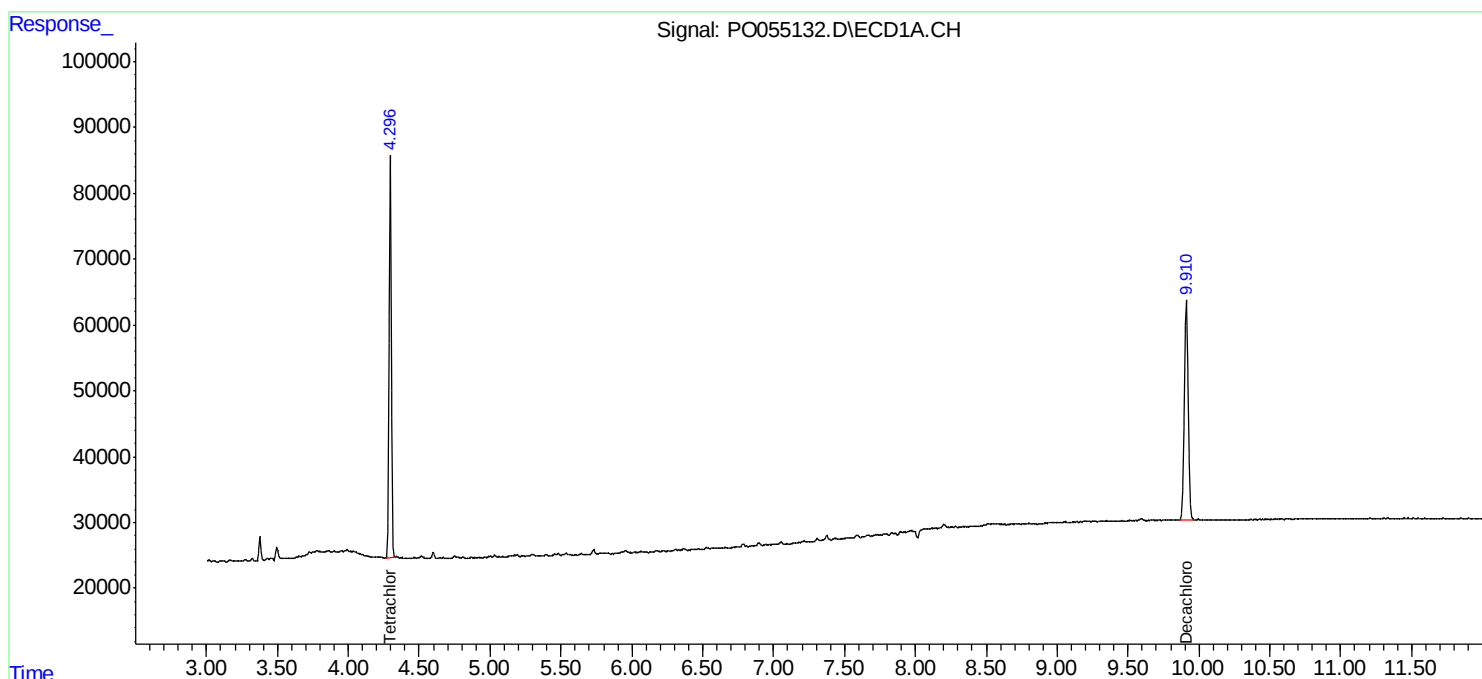

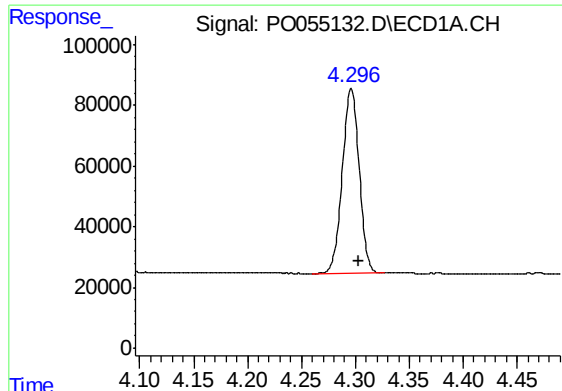


#1 Tetrachloro-m-xylene

R.T.: 4.296 min
Delta R.T.: -0.007 min
Response: 661261
Conc: 19.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
IDOC BL


Manual Integrations
APPROVED

Sohil
4/11/2019 9:16:29 AM

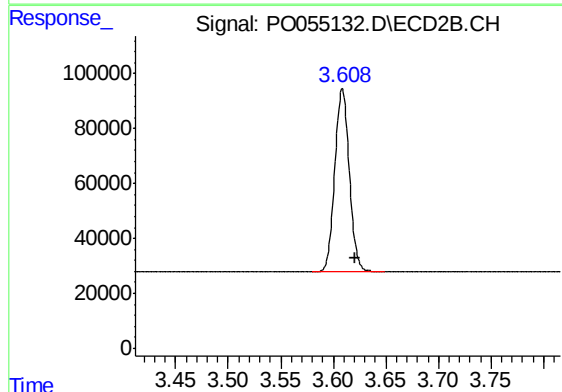


#1 Tetrachloro-m-xylene

R.T.: 3.609 min
Delta R.T.: -0.012 min
Response: 637964
Conc: 19.99 ng/ml

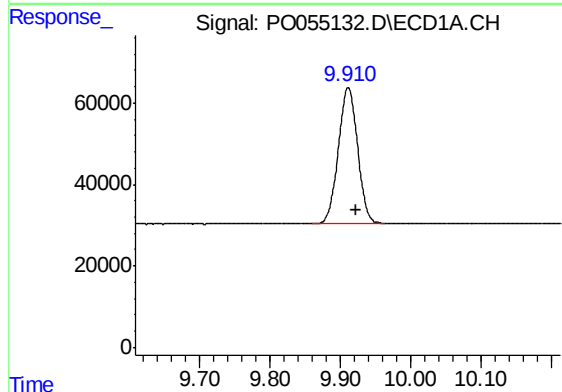

#2 Decachlorobiphenyl

R.T.: 9.911 min
Delta R.T.: -0.012 min
Response: 632752
Conc: 12.84 ng/ml

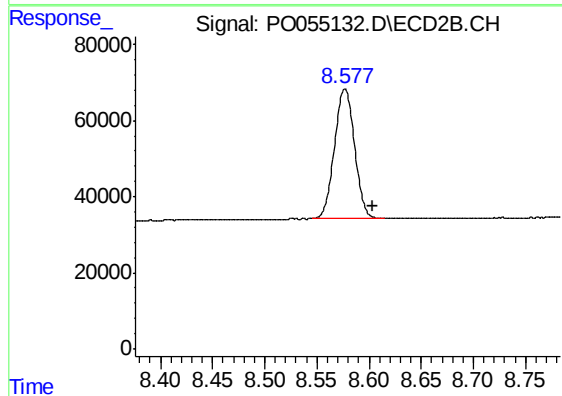

#2 Decachlorobiphenyl

R.T.: 8.577 min
Delta R.T.: -0.027 min
Response: 458391
Conc: 14.39 ng/ml m