

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\P0041023\  
 Data File : P0094029.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 10 Apr 2023 10:21  
 Operator : YP/AJ  
 Sample : 02224-17  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 ECD\_O  
 ClientSampleId :  
 OU3-FC-BACKFILL-09

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Apr 11 01:31:07 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\P0040323.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Tue Apr 04 06:20:55 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|--------|-------|----------|----------|--------|--------|
| -----                       |        |       |          |          |        |        |
| System Monitoring Compounds |        |       |          |          |        |        |
| 1) SA Tetrachlo...          | 4.421  | 3.624 | 69260596 | 25414872 | 18.528 | 19.958 |
| 2) SA Decachlor...          | 10.245 | 8.643 | 52699261 | 23440440 | 23.559 | 23.445 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_O\Data\PO041023\  
Data File : PO094029.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 10 Apr 2023 10:21  
Operator : YP/AJ  
Sample : 02224-17  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
ECD\_O  
ClientSampleId :  
OU3-FC-BACKFILL-09

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Apr 11 01:31:07 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_O\methods\PO040323.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Tue Apr 04 06:20:55 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

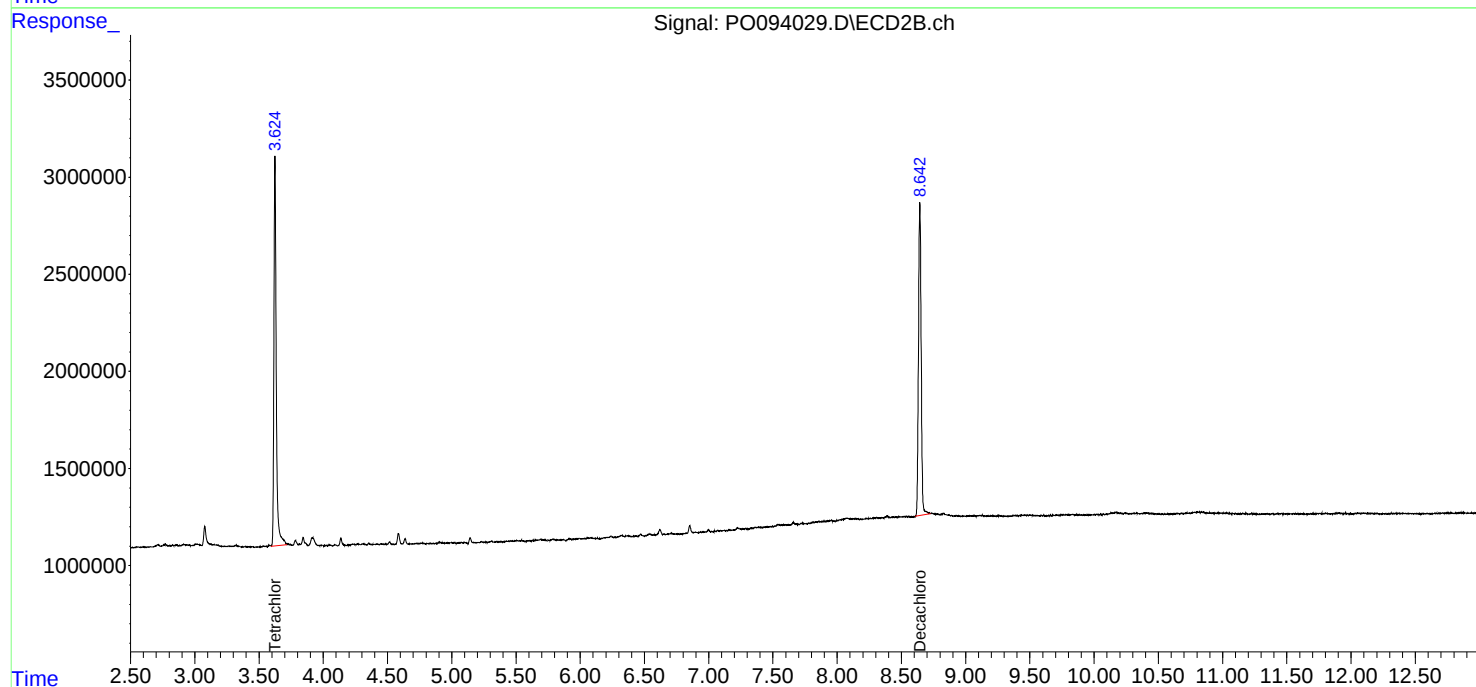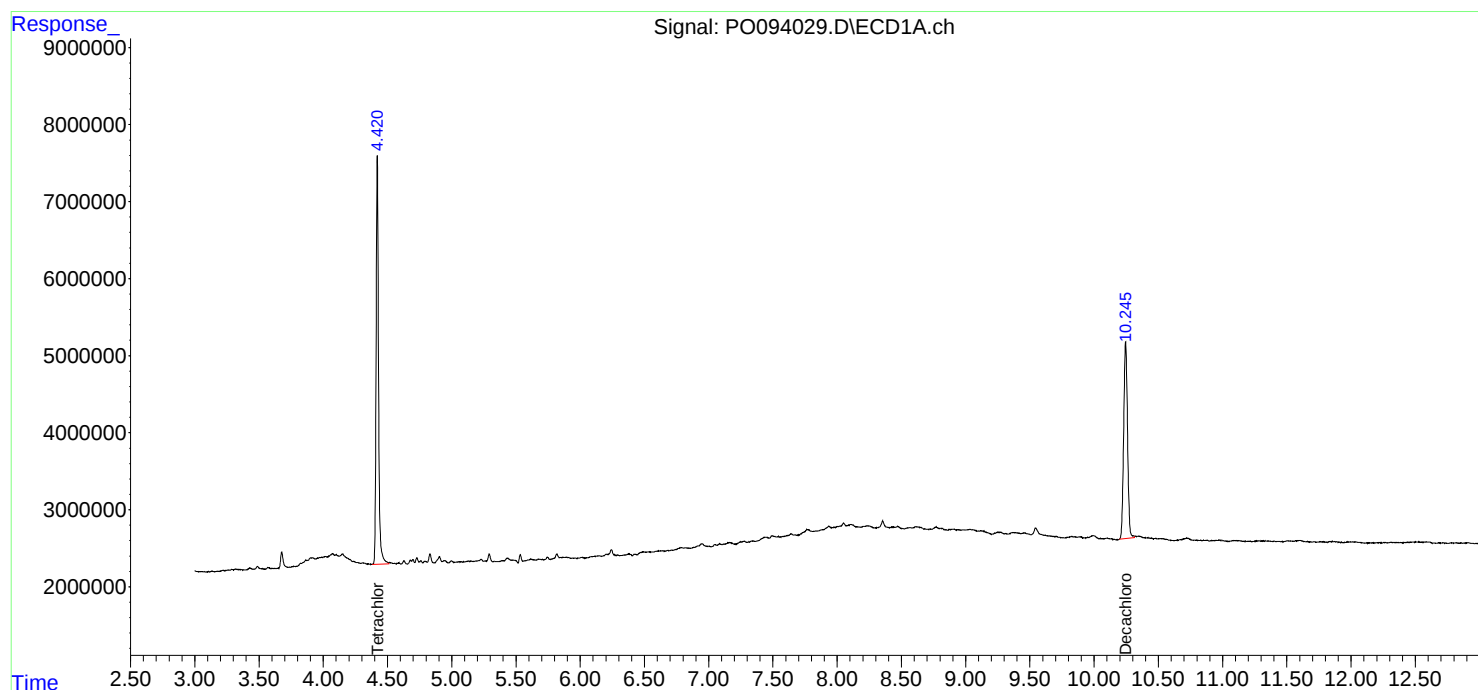


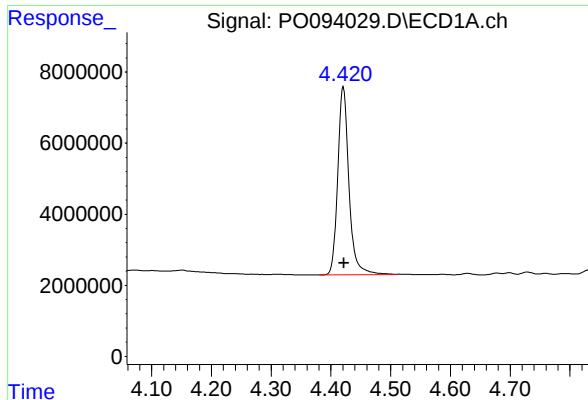

#1 Tetrachloro-m-xylene


R.T.: 4.421 min  
Delta R.T.: -0.001 min  
Response: 69260596  
Conc: 18.53 ng/ml

Instrument :  
ECD\_O  
ClientSampleId :  
OU3-FC-BACKFILL-09

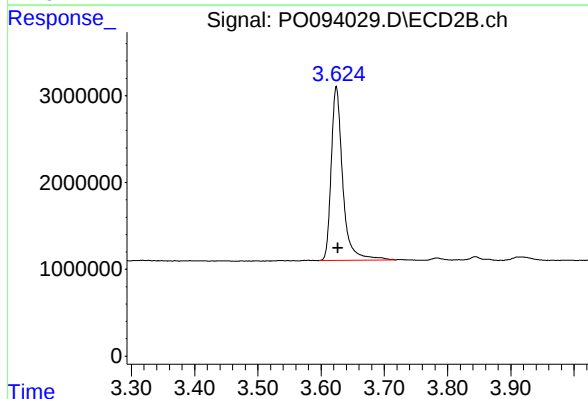


#1 Tetrachloro-m-xylene

R.T.: 3.624 min  
Delta R.T.: -0.003 min  
Response: 25414872  
Conc: 19.96 ng/ml

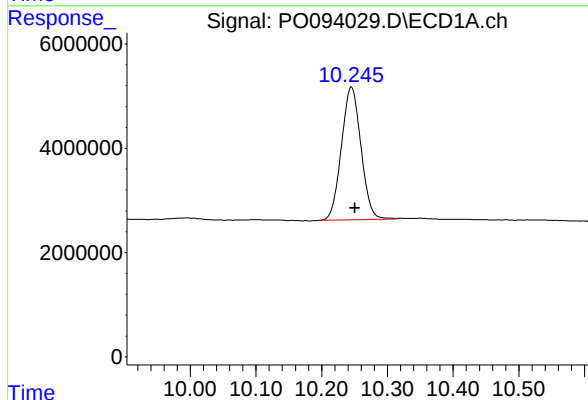

#2 Decachlorobiphenyl

R.T.: 10.245 min  
Delta R.T.: -0.005 min  
Response: 52699261  
Conc: 23.56 ng/ml

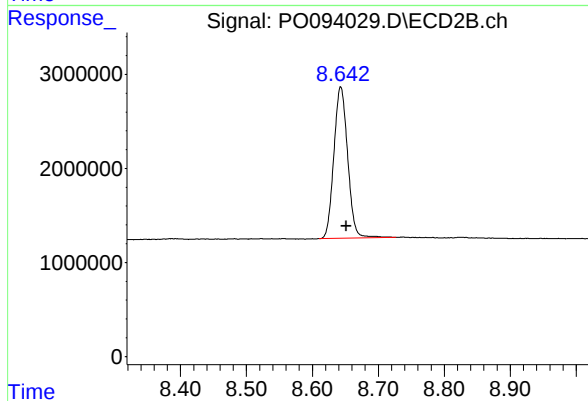

#2 Decachlorobiphenyl

R.T.: 8.643 min  
Delta R.T.: -0.008 min  
Response: 23440440  
Conc: 23.45 ng/ml