

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041023\
 Data File : P0094034.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Apr 2023 11:47
 Operator : YP/AJ
 Sample : 02224-27
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OU3-FC-BACKFILL-14

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 11 01:34:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.420	3.625	69452569	26286312	18.579	20.642
2) SA Decachlor...	10.243	8.644	51176578	22606152	22.878	22.611

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041023\
Data File : PO094034.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Apr 2023 11:47
Operator : YP/AJ
Sample : 02224-27
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OU3-FC-BACKFILL-14

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 11 01:34:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

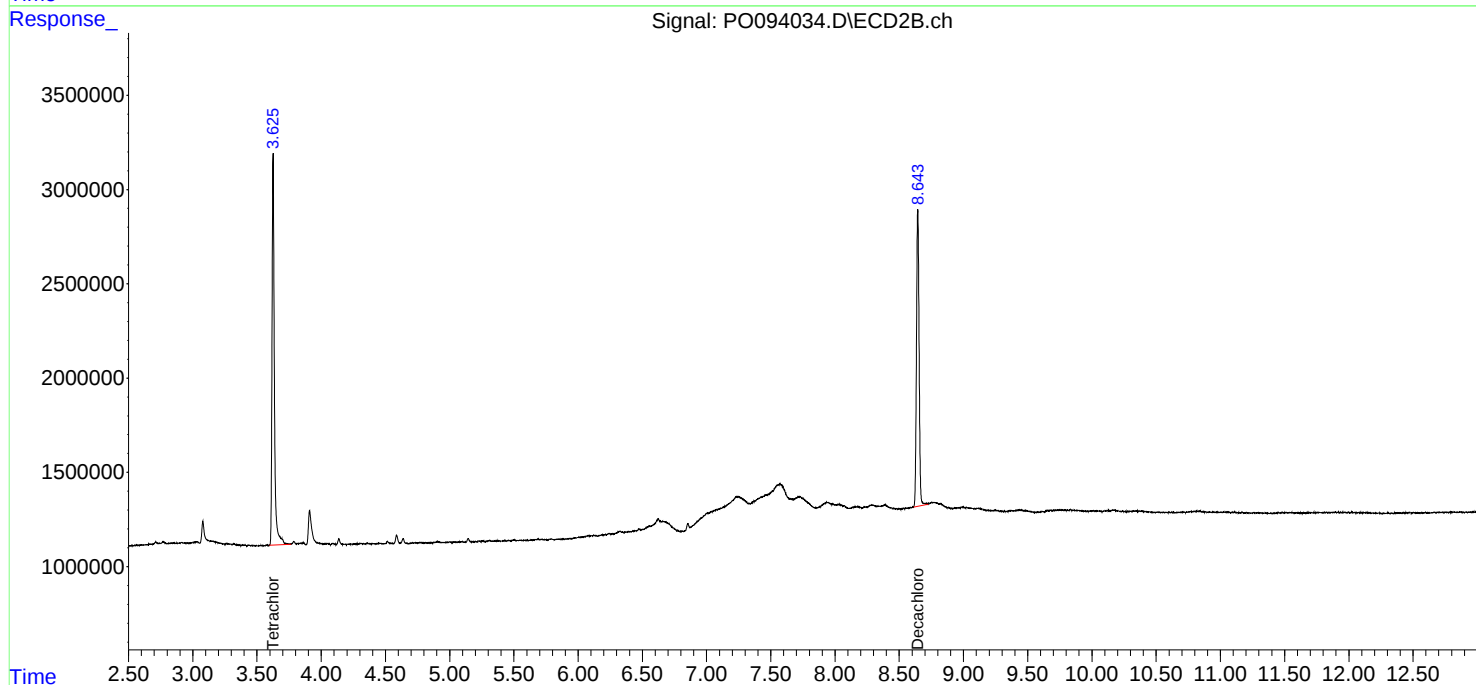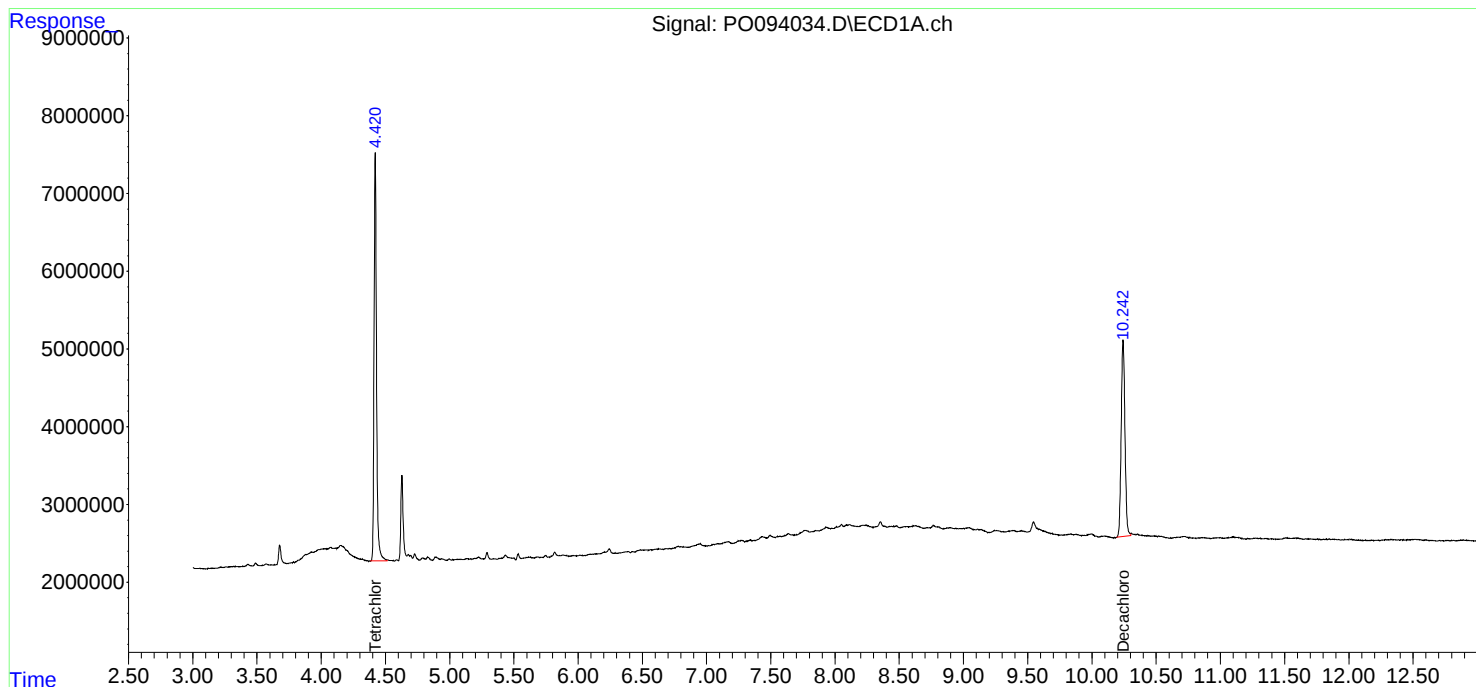


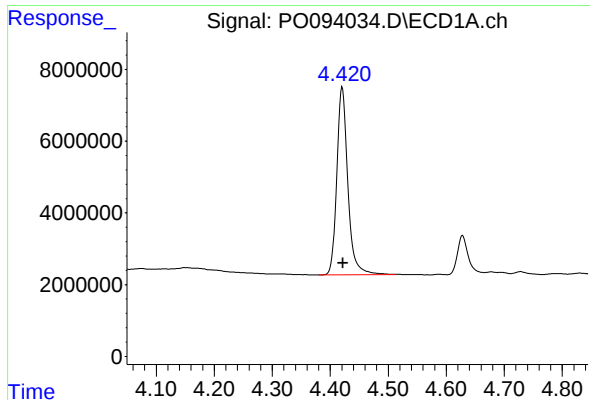

#1 Tetrachloro-m-xylene


R.T.: 4.420 min
Delta R.T.: -0.002 min
Response: 69452569
Conc: 18.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
OU3-FC-BACKFILL-14

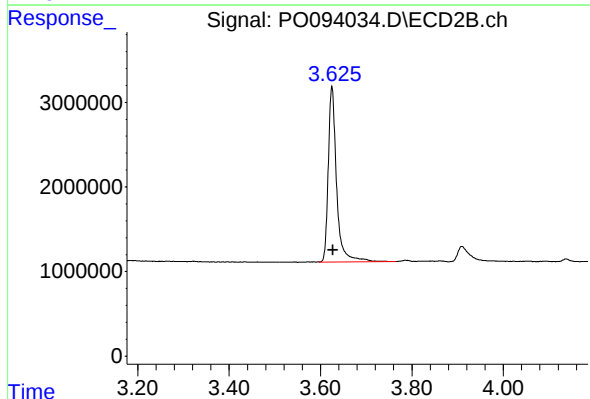


#1 Tetrachloro-m-xylene

R.T.: 3.625 min
Delta R.T.: -0.002 min
Response: 26286312
Conc: 20.64 ng/ml

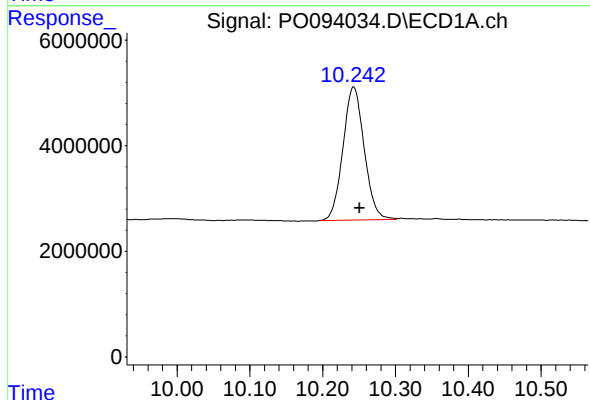

#2 Decachlorobiphenyl

R.T.: 10.243 min
Delta R.T.: -0.008 min
Response: 51176578
Conc: 22.88 ng/ml

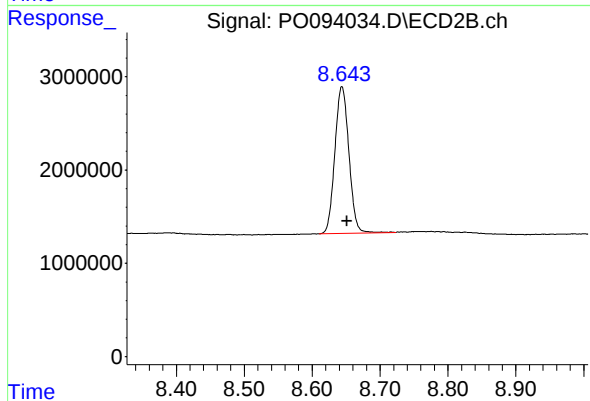

#2 Decachlorobiphenyl

R.T.: 8.644 min
Delta R.T.: -0.008 min
Response: 22606152
Conc: 22.61 ng/ml