

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041123\
 Data File : P0094096.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2023 16:34
 Operator : YP/AJ
 Sample : 02265-01 (Sig #1); PB152032BS (Sig #2)
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 40215

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 02:41:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.419	3.622	68886452	24334616	18.428	19.110
2) SA Decachlor...	10.246	8.643	52907831	23460148	23.652	23.465

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041123\
Data File : PO094096.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2023 16:34
Operator : YP/AJ
Sample : 02265-01 (Sig #1); PB152032BS (Sig #2)
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
40215

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 02:41:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

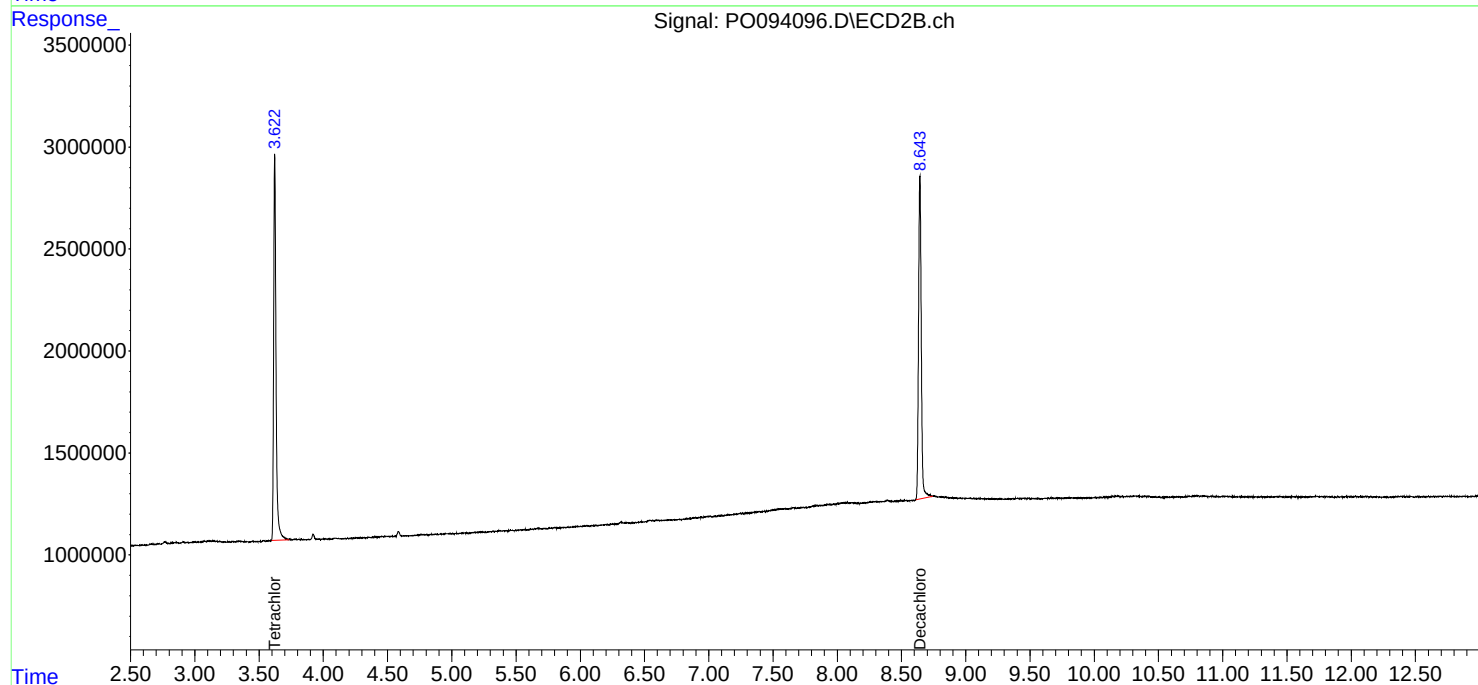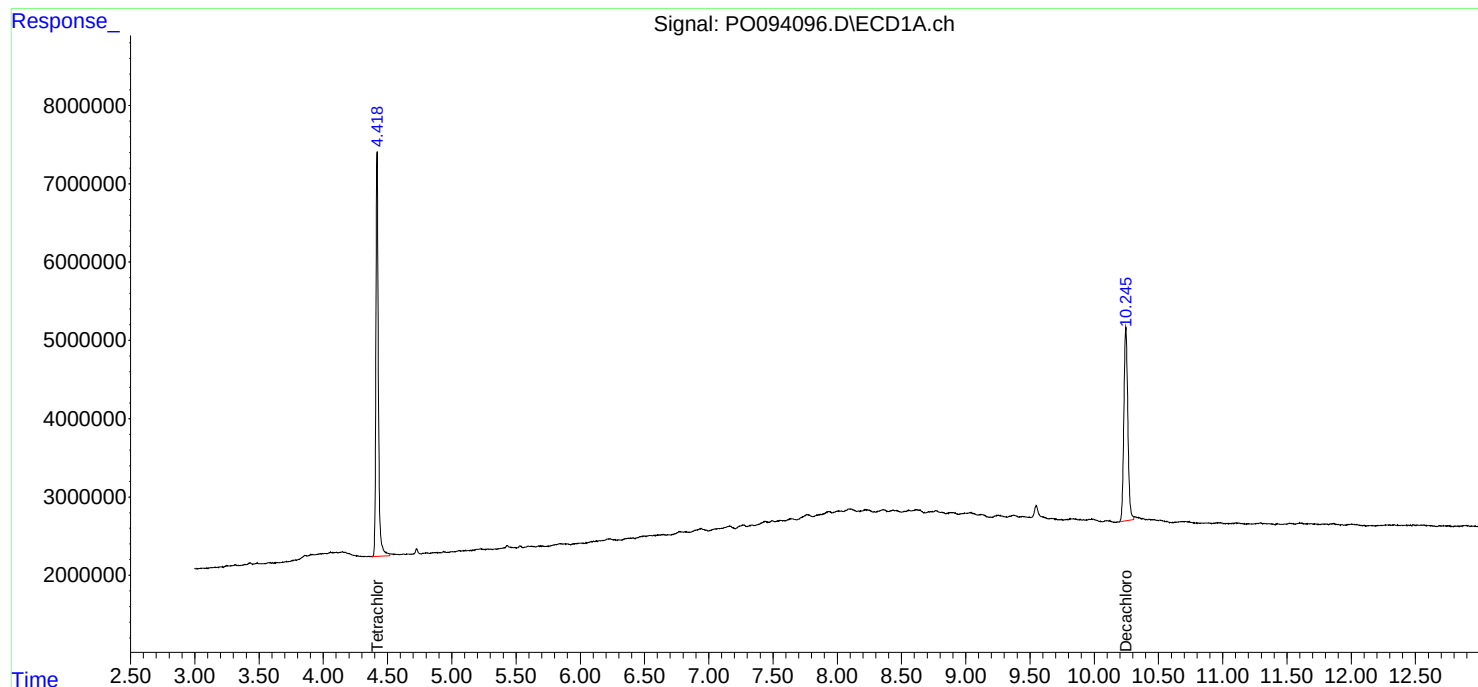


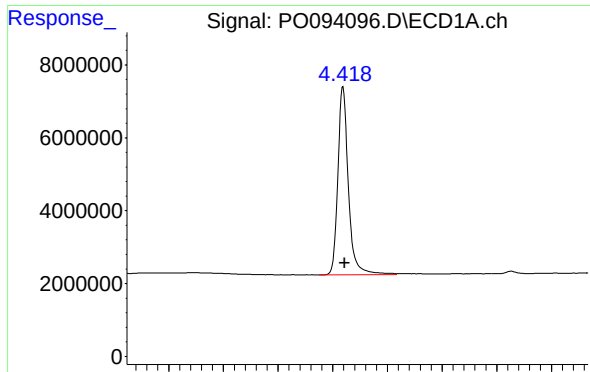

#1 Tetrachloro-m-xylene


R.T.: 4.419 min
Delta R.T.: -0.003 min
Response: 68886452
Conc: 18.43 ng/ml

Instrument :
ECD_O
ClientSampleId :
40215

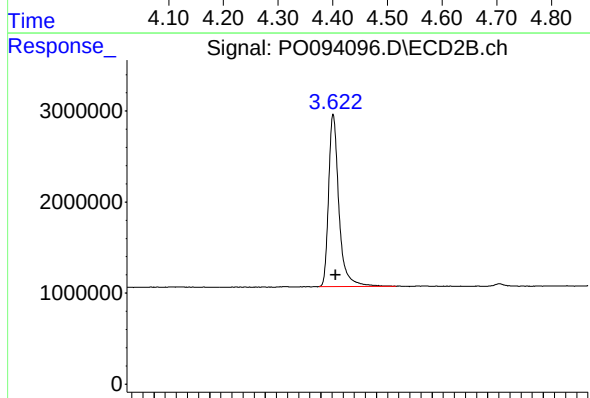


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.005 min
Response: 24334616
Conc: 19.11 ng/ml

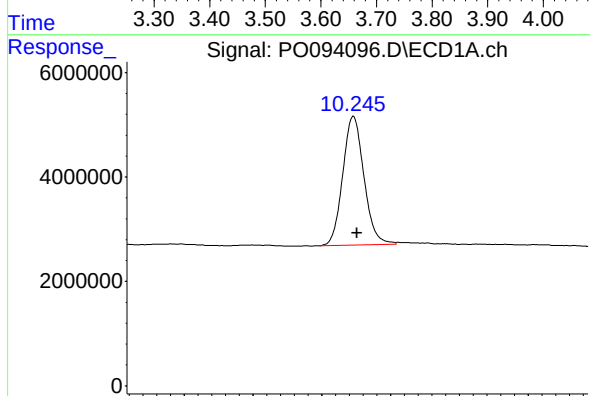

#2 Decachlorobiphenyl

R.T.: 10.246 min
Delta R.T.: -0.005 min
Response: 52907831
Conc: 23.65 ng/ml

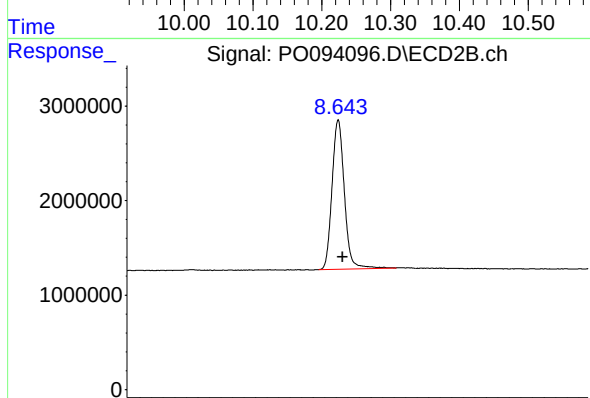

#2 Decachlorobiphenyl

R.T.: 8.643 min
Delta R.T.: -0.008 min
Response: 23460148
Conc: 23.47 ng/ml