

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041124\
 Data File : P0102775.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Apr 2024 23:32
 Operator : YP/AJ
 Sample : P2069-11 10X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AC09-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh
 Patel

04/12/2024

Supervised By :Ankita
 Jodhani

04/12/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 01:46:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0031824.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Mar 19 08:56:28 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.261	3.378	6145071	4071611	1.394	1.415
2) SA Decachlor...	9.793	8.238	4209037	2708076	1.516	1.493m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041124\
Data File : PO102775.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Apr 2024 23:32
Operator : YP/AJ
Sample : P2069-11 10X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AC09-1

Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel



04/12/2024


Supervised By :Ankita
Jodhani

04/12/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 01:46:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO031824.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Mar 19 08:56:28 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

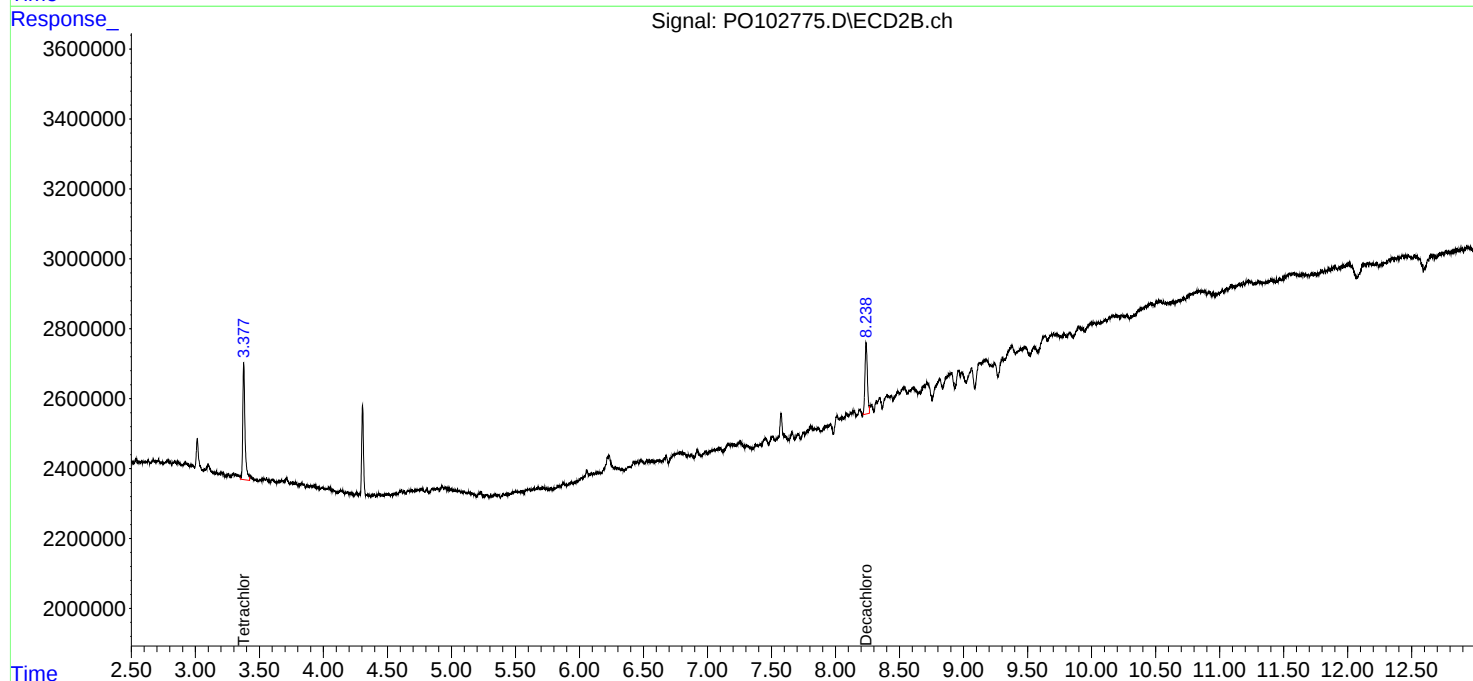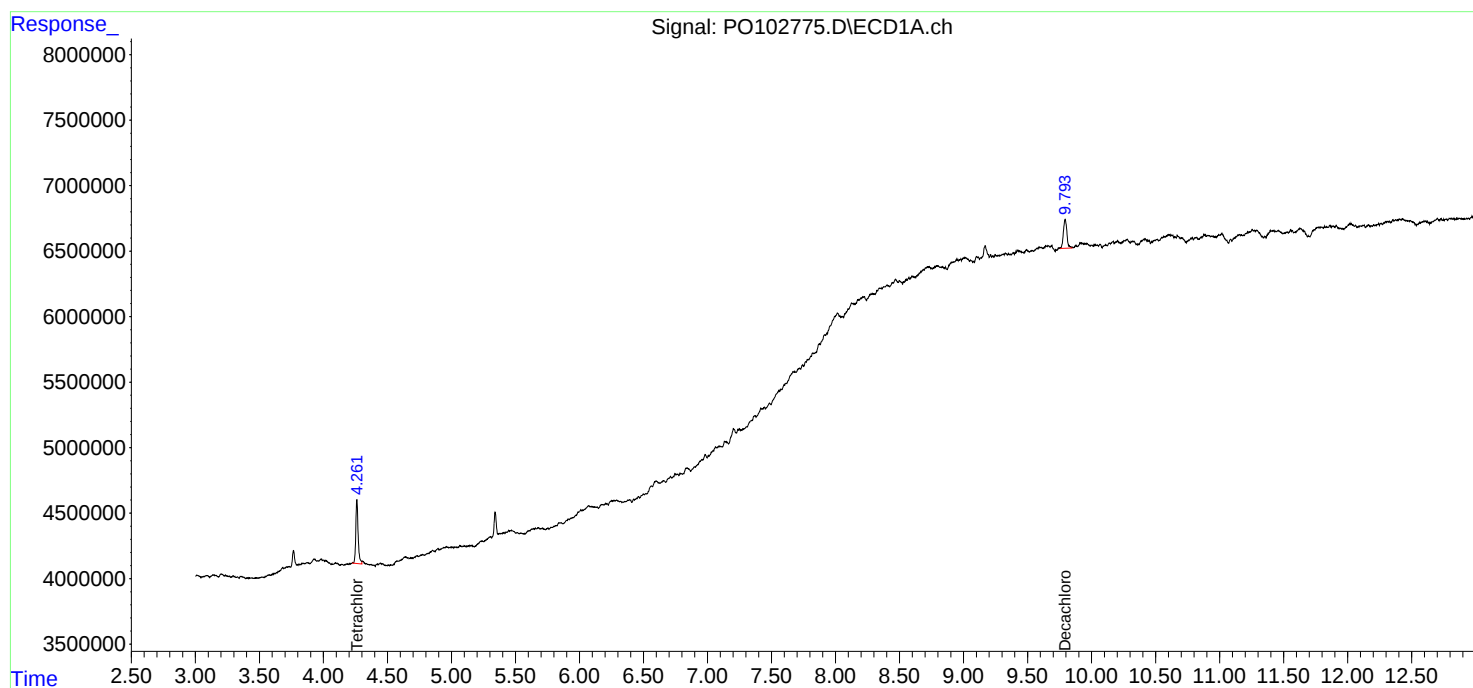

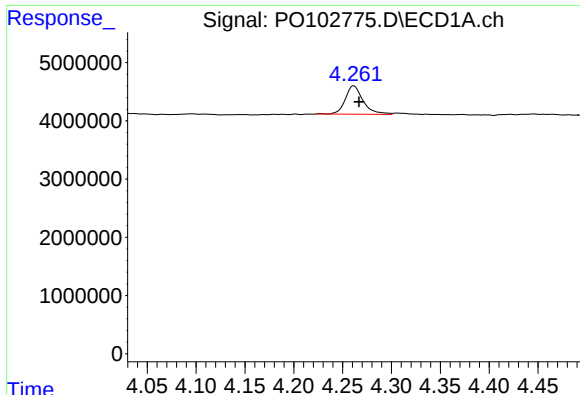

#1 Tetrachloro-m-xylene

R.T.: 4.261 min
Delta R.T.: -0.006 min
Response: 6145071
Conc: 1.39 ng/ml

Instrument :
ECD_O
ClientSampleId :
AC09-1


Manual Integrations
APPROVED

Reviewed By :Yogesh
Patel

04/12/2024


Supervised By :Ankita
Jodhani

04/12/2024

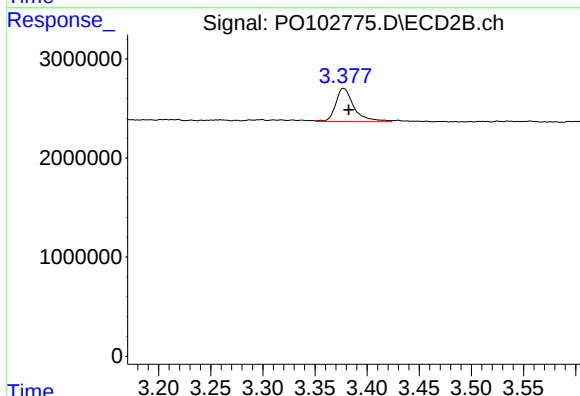


#1 Tetrachloro-m-xylene

R.T.: 3.378 min
Delta R.T.: -0.005 min
Response: 4071611
Conc: 1.42 ng/ml

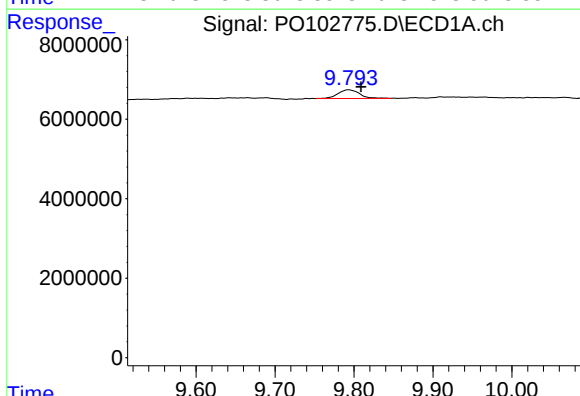

#2 Decachlorobiphenyl

R.T.: 9.793 min
Delta R.T.: -0.016 min
Response: 4209037
Conc: 1.52 ng/ml

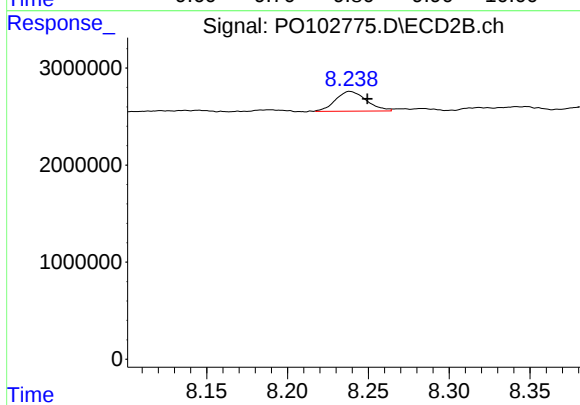

#2 Decachlorobiphenyl

R.T.: 8.238 min
Delta R.T.: -0.011 min
Response: 2708076
Conc: 1.49 ng/ml m