

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041221\
 Data File : P0076915.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Apr 2021 15:26
 Operator : AJ/MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 16:37:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.901	3.897	1987346	1055476	21.366	21.033
2) SA Decachlor...	10.873	9.140	1896767	885999	20.479	18.258
Target Compounds						
9) L2 AR-1221-2	0.000	4.246	0	13140	N.D.	37.261 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041221\
Data File : P0076915.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Apr 2021 15:26
Operator : AJ/MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 16:37:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

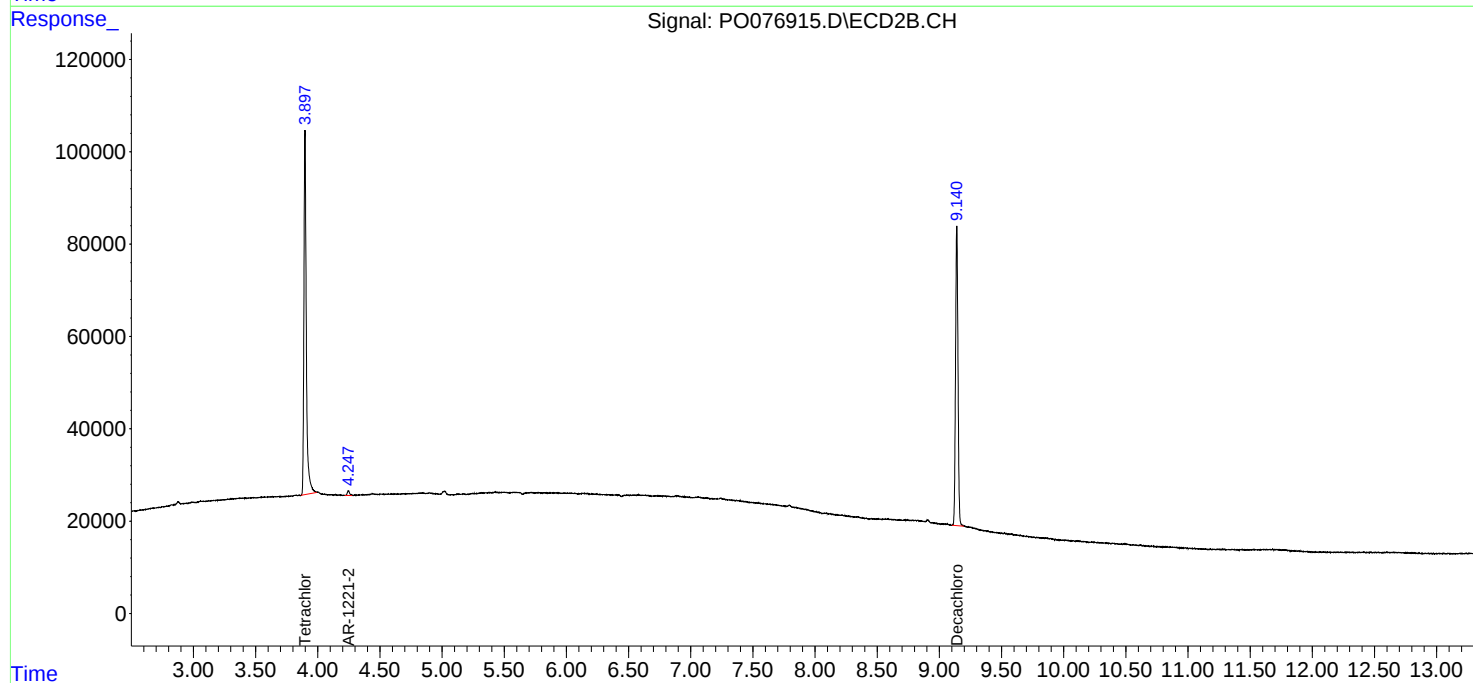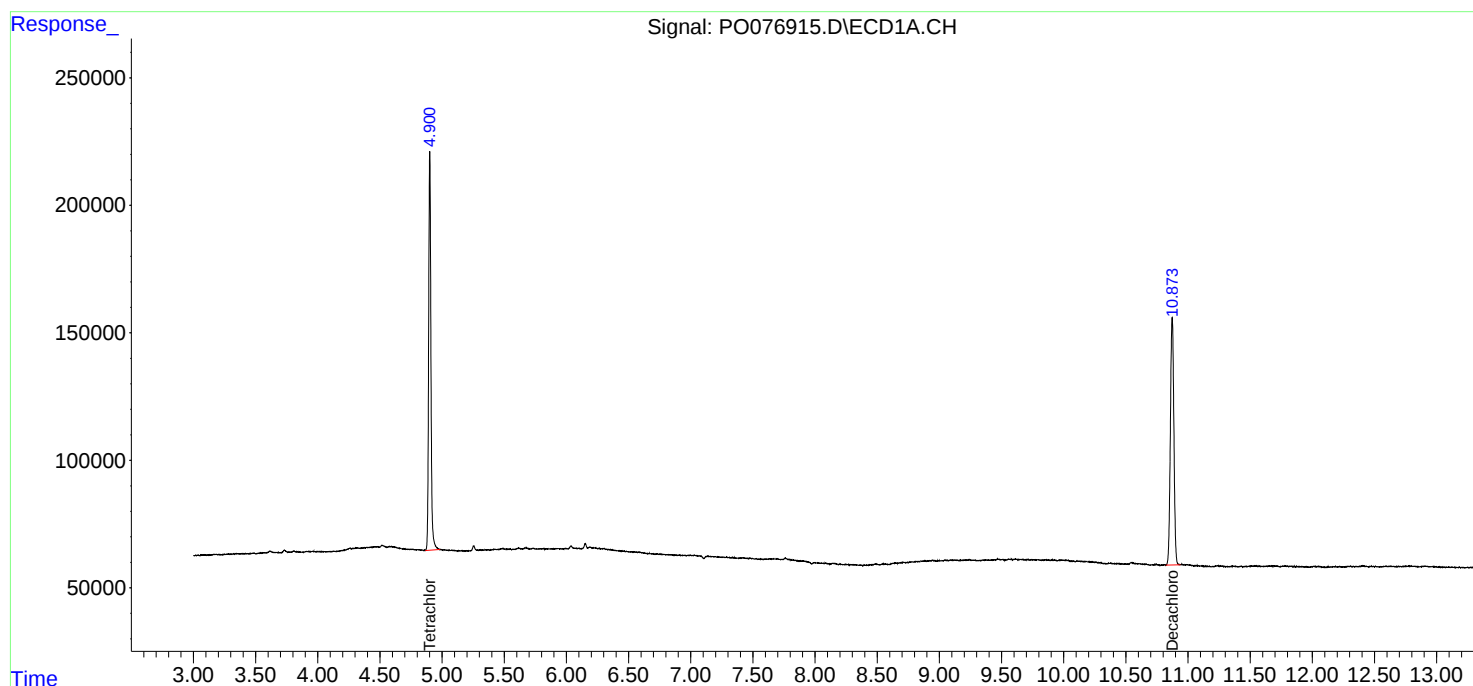


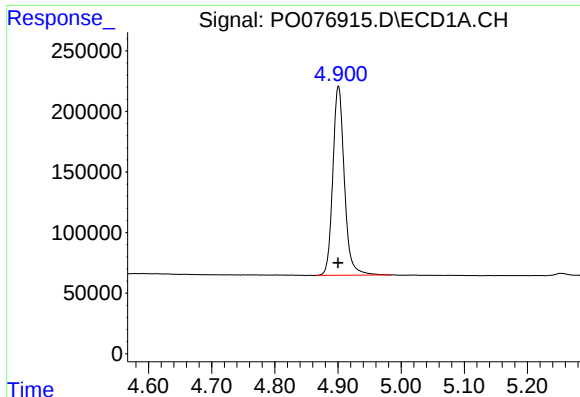

#1 Tetrachloro-m-xylene


R.T.: 4.901 min
Delta R.T.: 0.000 min
Response: 1987346
Conc: 21.37 ng/ml

Instrument :
ECD_O
ClientSampleId :

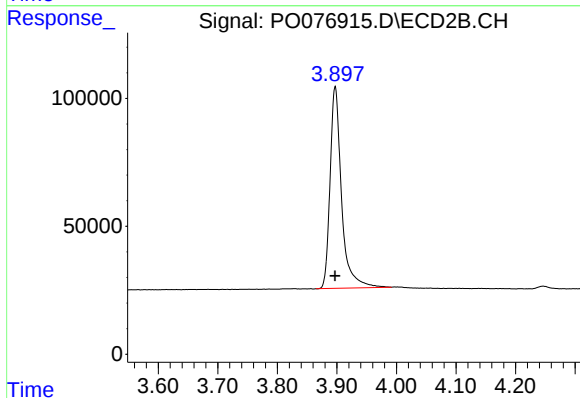


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 1055476
Conc: 21.03 ng/ml

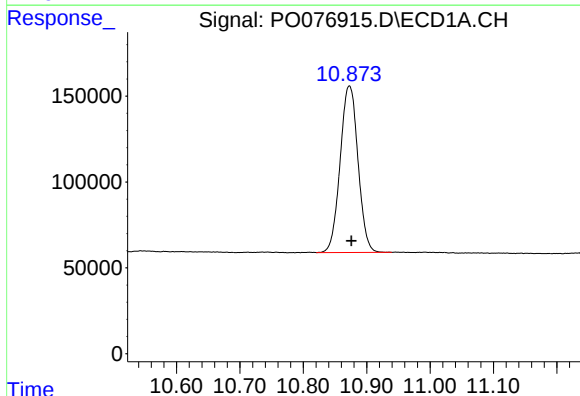


#2 Decachlorobiphenyl

R.T.: 10.873 min
Delta R.T.: -0.003 min
Response: 1896767
Conc: 20.48 ng/ml

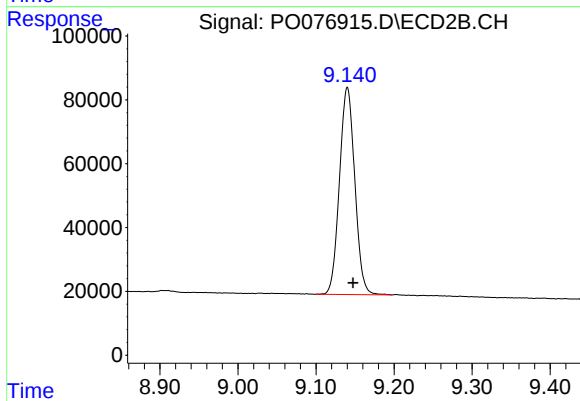

#2 Decachlorobiphenyl


R.T.: 9.140 min
Delta R.T.: -0.007 min
Response: 885999
Conc: 18.26 ng/ml

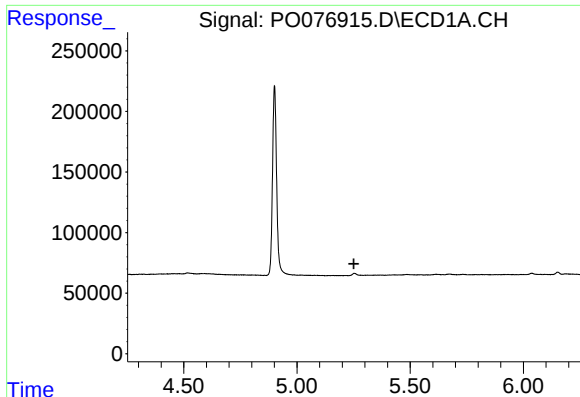

#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 5.251 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

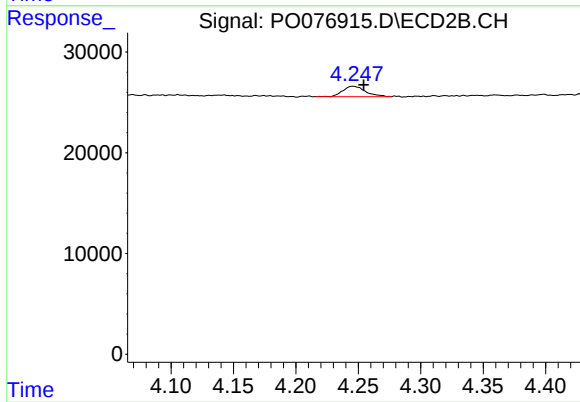

#9 AR-1221-2

R.T.: 4.246 min
Delta R.T.: -0.008 min
Response: 13140
Conc: 37.26 ng/ml