

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0041221\
 Data File : P0076905.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Apr 2021 11:40
 Operator : AJ/MA
 Sample : M1967-09DL 2X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 SB1-ADL

Manual Integrations
 APPROVED

Ankita
 4/13/2021 1:20:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 15:37:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.897	3.894	898168	396451	9.656m	7.900
2) SA Decachlor...	10.867	9.138	1106858	477349	11.951	9.837m
Target Compounds						
21) L5 AR-1248-1	6.219	5.139	1169227	568216	769.720	754.484
22) L5 AR-1248-2	6.513	5.400	1162793	698962	502.351	481.422
23) L5 AR-1248-3	6.730	5.442	1250557	903654	444.702	620.711 #
24) L5 AR-1248-4	7.159	5.626	1355219	744861	402.019	436.286
25) L5 AR-1248-5	7.202	6.046	2388050	975480	692.891	485.348 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041221\
Data File : PO076905.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Apr 2021 11:40
Operator : AJ/MA
Sample : M1967-09DL 2X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB1-ADL


Manual Integrations
APPROVED

Ankita
4/13/2021 1:20:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 15:37:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

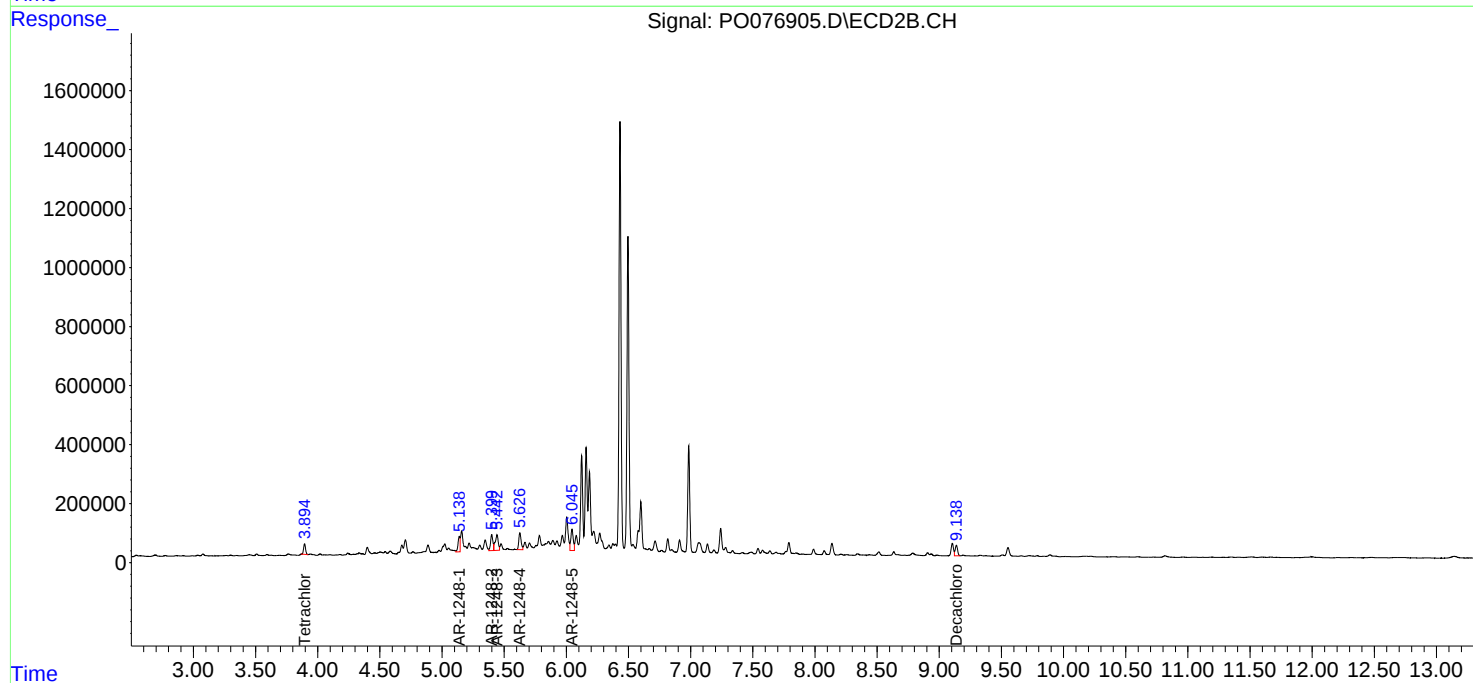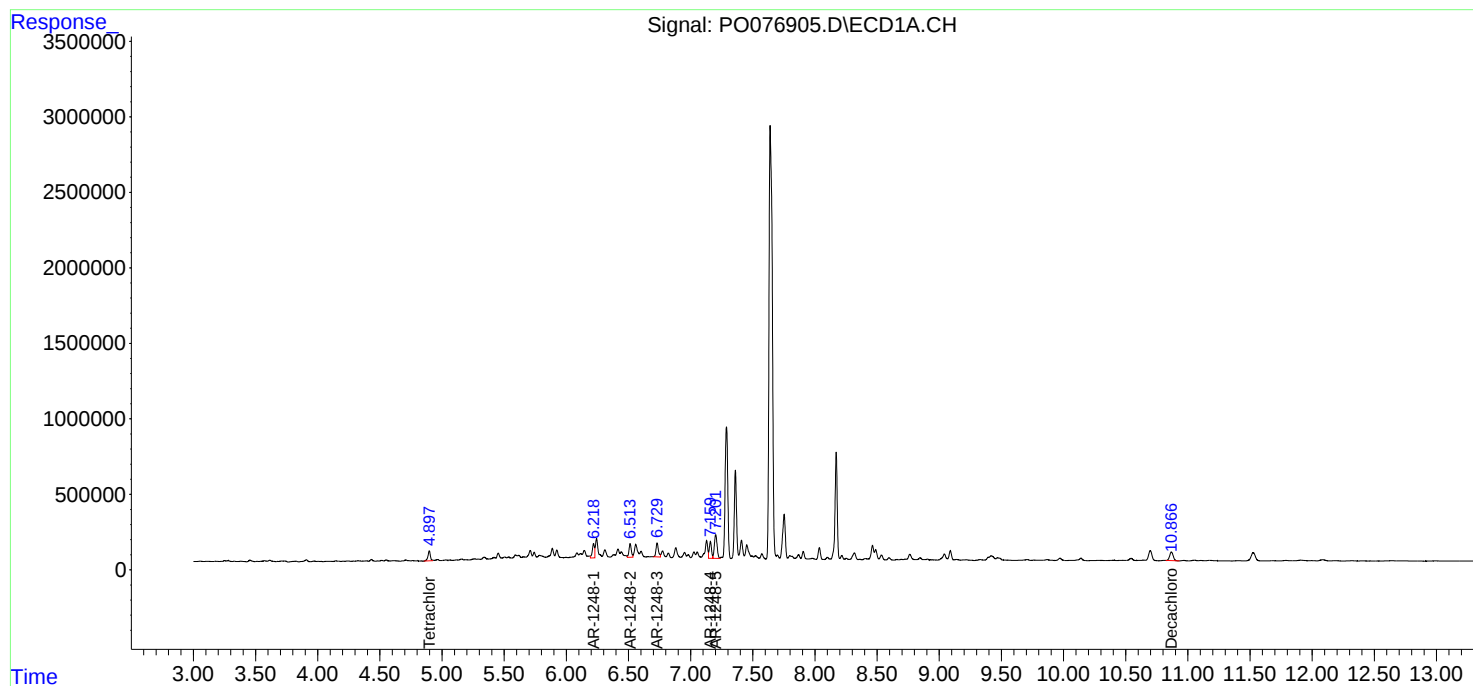

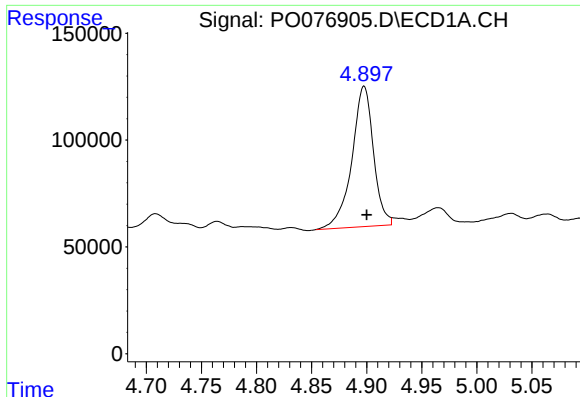


#1 Tetrachloro-m-xylene

R.T.: 4.897 min
Delta R.T.: -0.003 min
Response: 898168
Conc: 9.66 ng/ml m

Instrument :
ECD_O
ClientSampleId :
SB1-ADL


Manual Integrations
APPROVED

Ankita
4/13/2021 1:20:19 PM

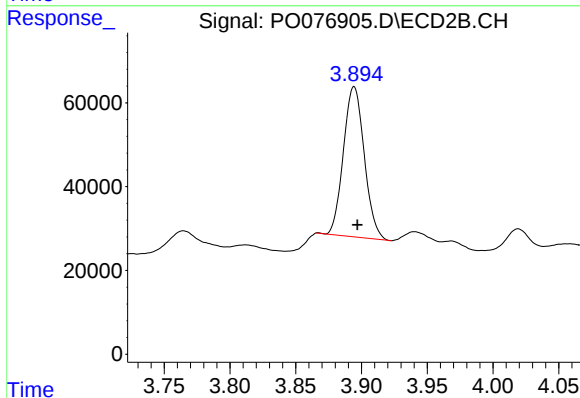


#1 Tetrachloro-m-xylene

R.T.: 3.894 min
Delta R.T.: -0.003 min
Response: 396451
Conc: 7.90 ng/ml

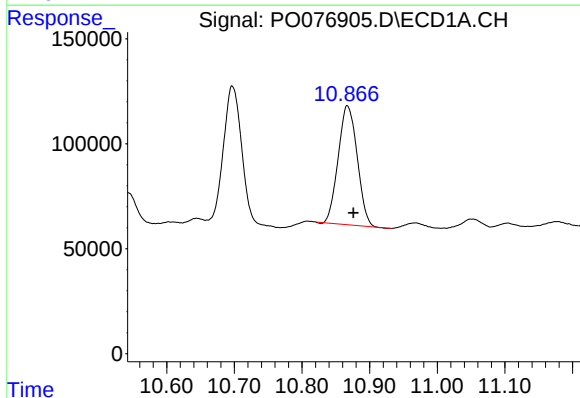


#2 Decachlorobiphenyl

R.T.: 10.867 min
Delta R.T.: -0.009 min
Response: 1106858
Conc: 11.95 ng/ml

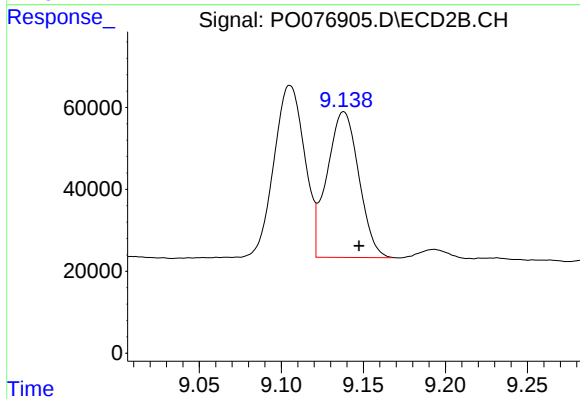

#2 Decachlorobiphenyl

R.T.: 9.138 min
Delta R.T.: -0.010 min
Response: 477349
Conc: 9.84 ng/ml m

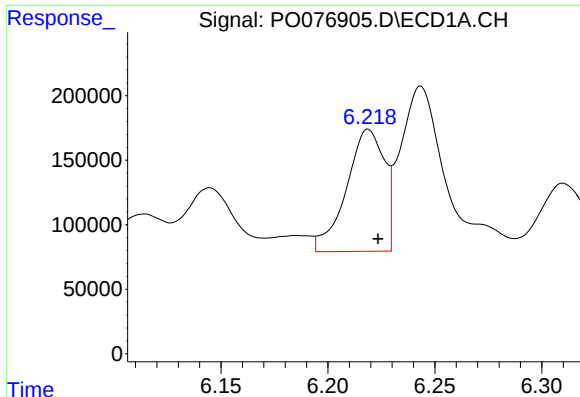


#21 AR-1248-1

R.T.: 6.219 min
Delta R.T.: -0.004 min
Response: 1169227
Conc: 769.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB1-ADL


Manual Integrations
APPROVED

Ankita
4/13/2021 1:20:19 PM

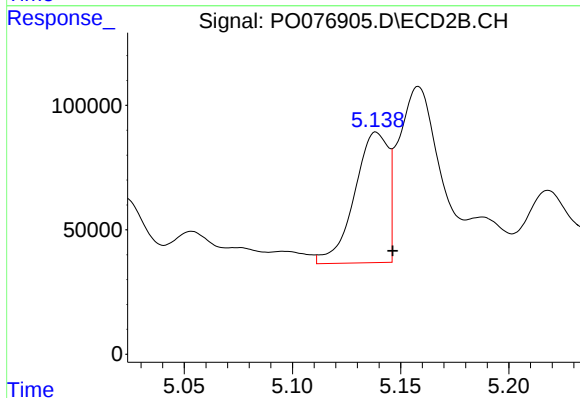


#21 AR-1248-1

R.T.: 5.139 min
Delta R.T.: -0.008 min
Response: 568216
Conc: 754.48 ng/ml

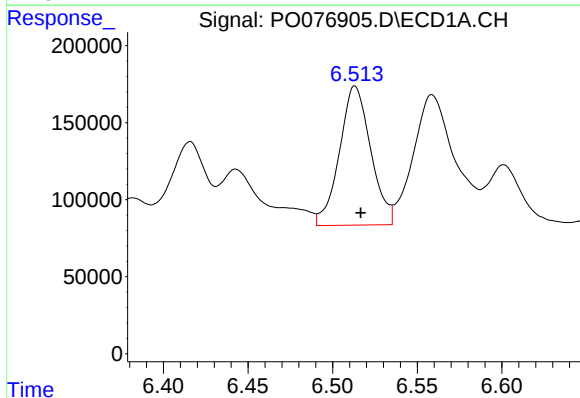


#22 AR-1248-2

R.T.: 6.513 min
Delta R.T.: -0.003 min
Response: 1162793
Conc: 502.35 ng/ml

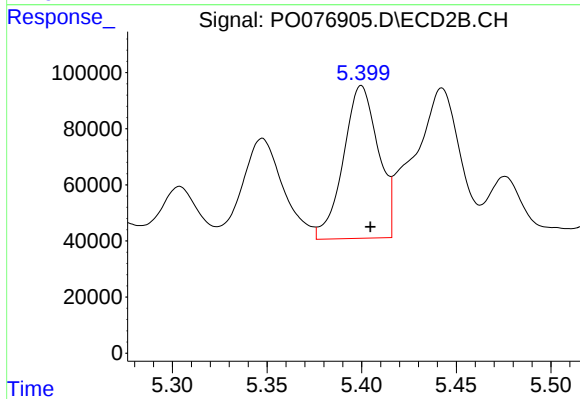

#22 AR-1248-2

R.T.: 5.400 min
Delta R.T.: -0.005 min
Response: 698962
Conc: 481.42 ng/ml

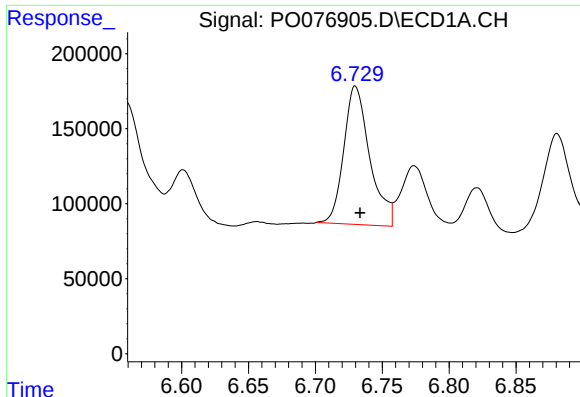


#23 AR-1248-3

R.T.: 6.730 min
Delta R.T.: -0.004 min
Response: 1250557
Conc: 444.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB1-ADL


Manual Integrations
APPROVED

Ankita
4/13/2021 1:20:19 PM

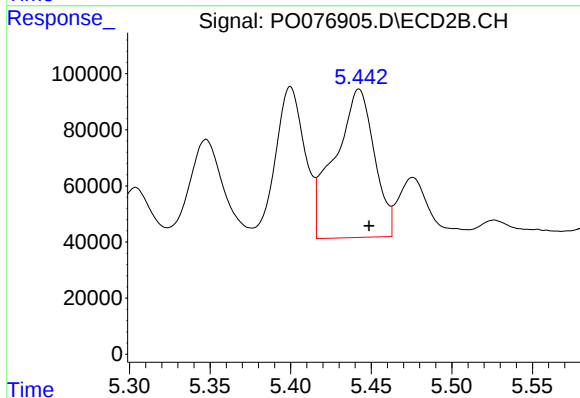


#23 AR-1248-3

R.T.: 5.442 min
Delta R.T.: -0.006 min
Response: 903654
Conc: 620.71 ng/ml

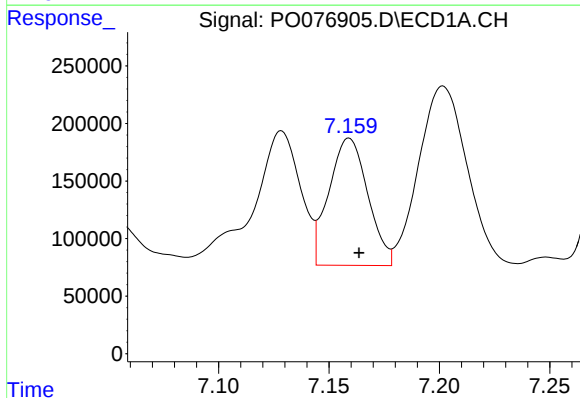


#24 AR-1248-4

R.T.: 7.159 min
Delta R.T.: -0.005 min
Response: 1355219
Conc: 402.02 ng/ml

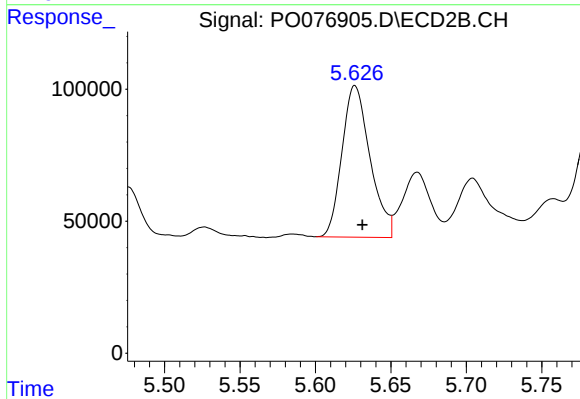

#24 AR-1248-4

R.T.: 5.626 min
Delta R.T.: -0.005 min
Response: 744861
Conc: 436.29 ng/ml

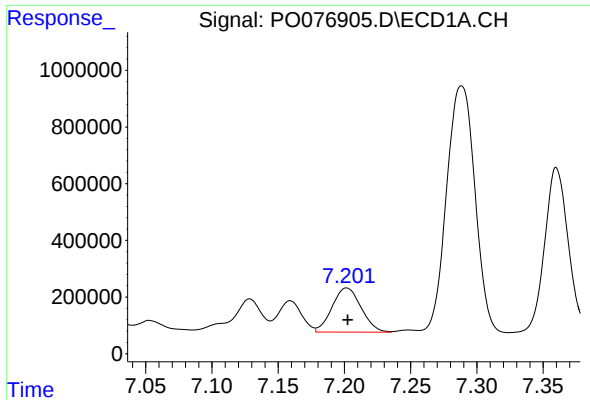


#25 AR-1248-5

R.T.: 7.202 min
Delta R.T.: 0.000 min
Response: 2388050
Conc: 692.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB1-ADL

Manual Integrations
APPROVED

Ankita
4/13/2021 1:20:19 PM

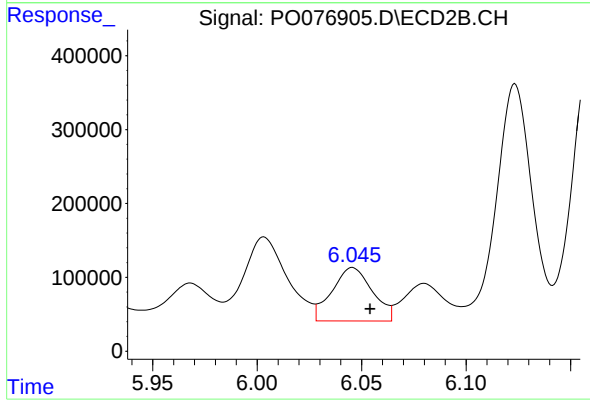

#25 AR-1248-5

R.T.: 6.046 min
Delta R.T.: -0.008 min
Response: 975480
Conc: 485.35 ng/ml