

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041221\
 Data File : P0076923.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Apr 2021 17:43
 Operator : AJ/MA
 Sample : M1983-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 31019

Manual Integrations
 APPROVED

Ankita
 4/14/2021 8:49:52 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 05:58:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.908	3.909	1519313	881695	16.334m	17.570m
2) SA Decachlor...	10.871	9.138	1835167	633339	19.814m	13.052 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041221\
Data File : P0076923.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Apr 2021 17:43
Operator : AJ/MA
Sample : M1983-06
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
31019


Manual Integrations
APPROVED

Ankita
4/14/2021 8:49:52 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 05:58:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

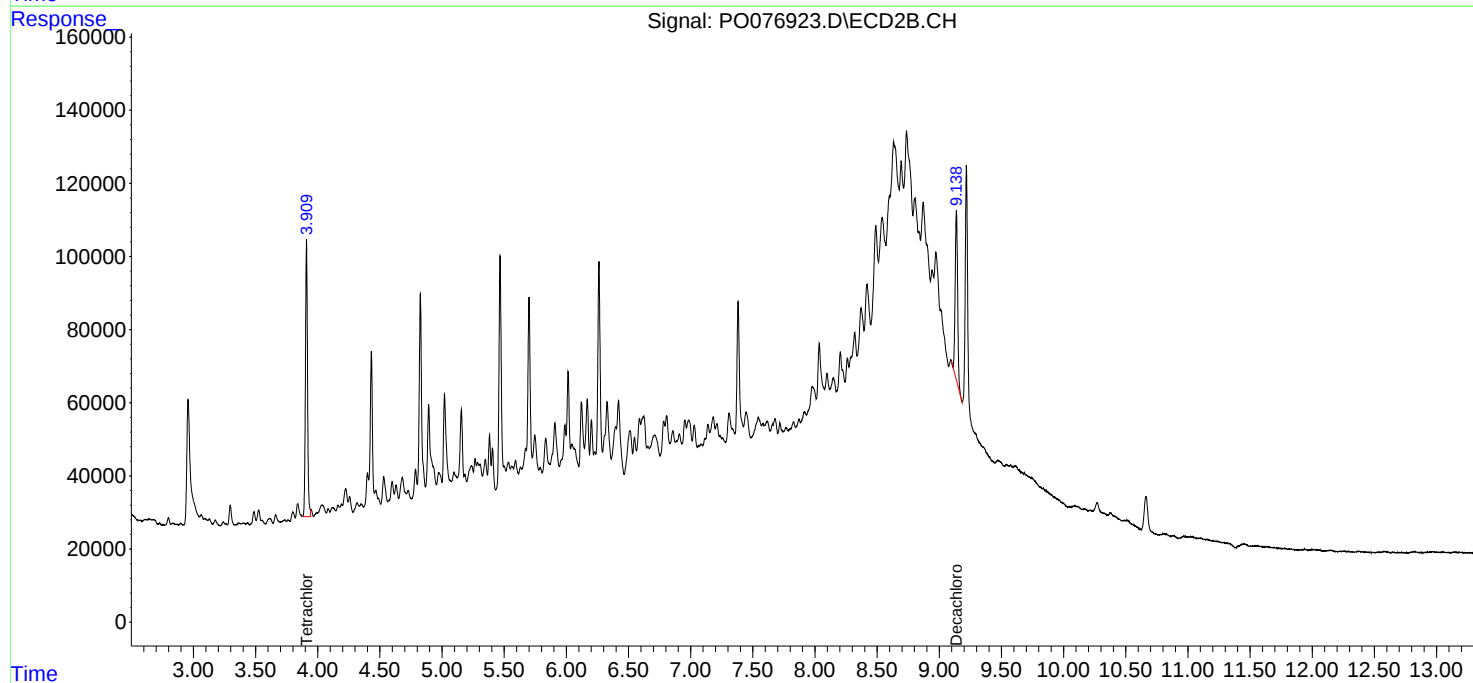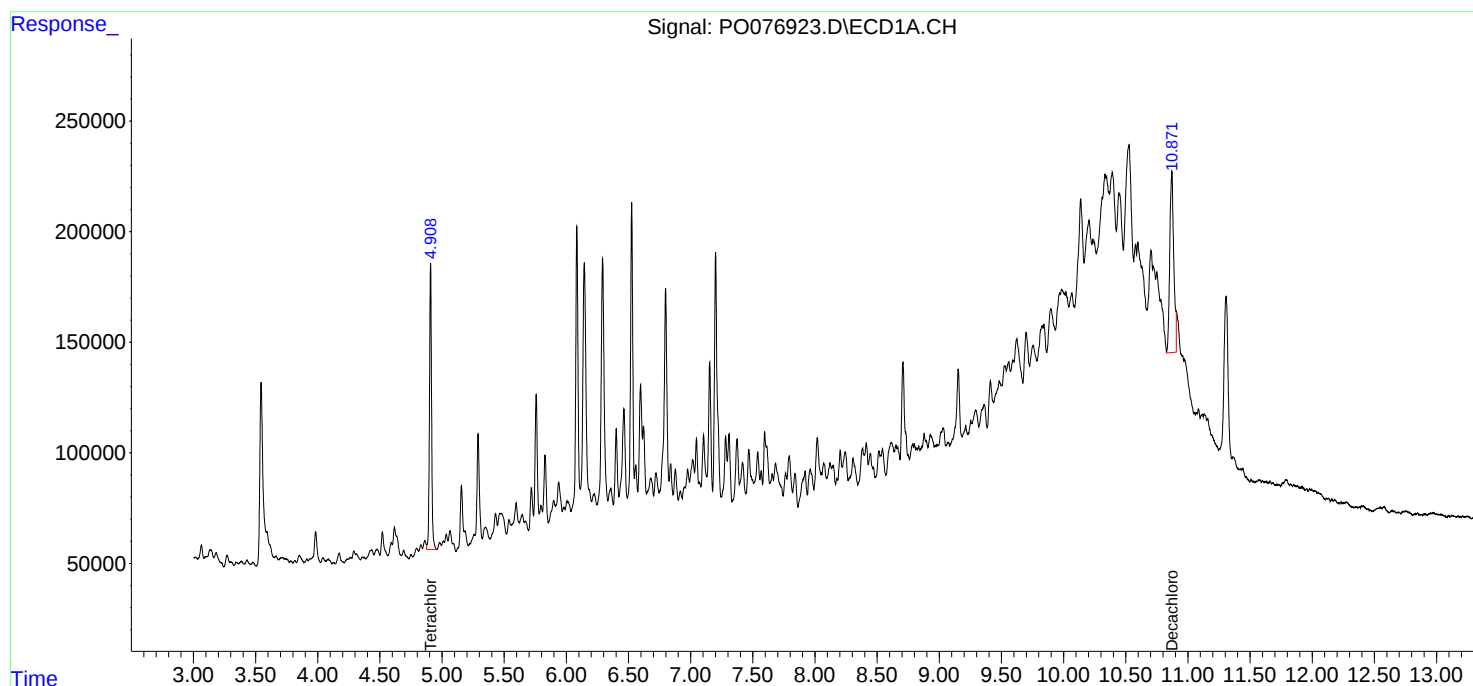

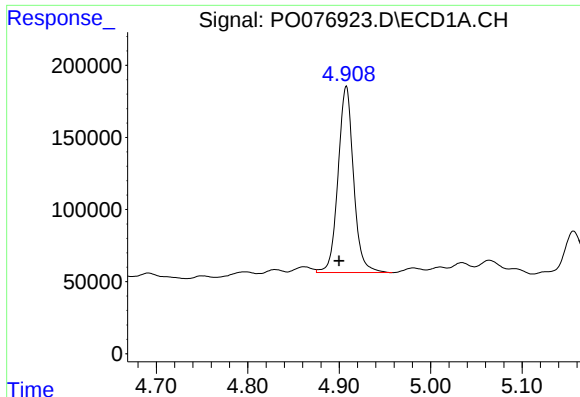


#1 Tetrachloro-m-xylene

R.T.: 4.908 min
Delta R.T.: 0.008 min
Response: 1519313
Conc: 16.33 ng/ml m

Instrument :
ECD_O
ClientSampleId :
31019


Manual Integrations
APPROVED

Ankita
4/14/2021 8:49:52 AM

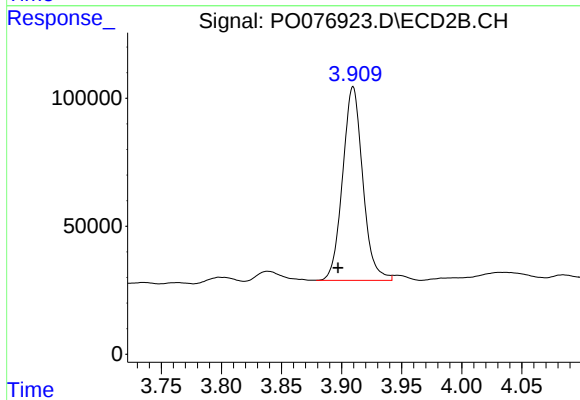


#1 Tetrachloro-m-xylene

R.T.: 3.909 min
Delta R.T.: 0.012 min
Response: 881695
Conc: 17.57 ng/ml m

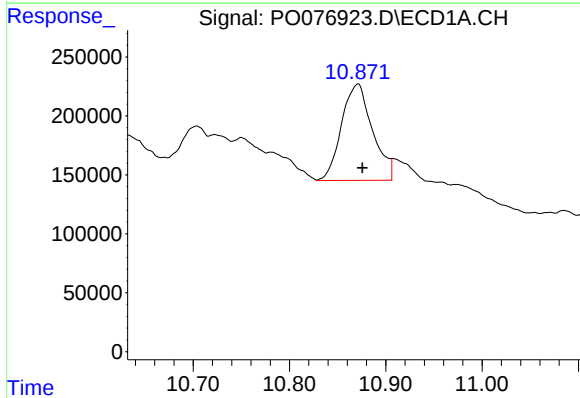

#2 Decachlorobiphenyl

R.T.: 10.871 min
Delta R.T.: -0.005 min
Response: 1835167
Conc: 19.81 ng/ml m

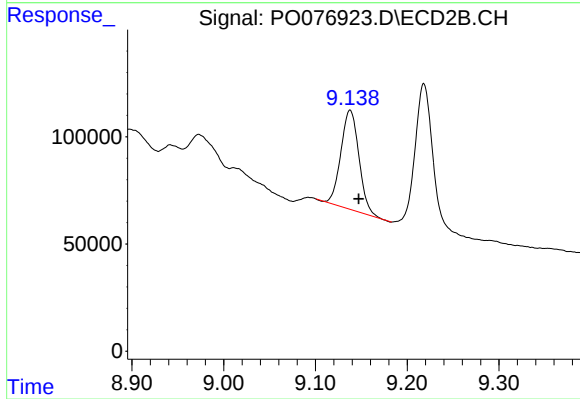

#2 Decachlorobiphenyl

R.T.: 9.138 min
Delta R.T.: -0.010 min
Response: 633339
Conc: 13.05 ng/ml