

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0041221\
 Data File : P0076935.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 Apr 2021 21:09
 Operator : AJ/MA
 Sample : M2001-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 HA-02

Manual Integrations
 APPROVED

Ankita
 4/14/2021 8:50:02 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 06:04:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.900	3.897	2226082	1081845	23.933	21.558
2) SA Decachlor...	10.867	9.137	1968292	1234994	21.251	25.450
Target Compounds						
26) L6 AR-1254-1	7.132	6.004	1044137	716298	328.497m	273.278
27) L6 AR-1254-2	7.359	6.162	1617148	662037	315.623m	289.098
28) L6 AR-1254-3	7.741	6.578	2053986	1282798	372.736	362.958
29) L6 AR-1254-4	8.036	6.817	1740315	844295	442.010	402.297
30) L6 AR-1254-5	8.464	7.243	2712546	5395562	616.751	1655.074 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041221\
Data File : P0076935.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 Apr 2021 21:09
Operator : AJ/MA
Sample : M2001-01
Misc :
ALS Vial : 31 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
HA-02


Manual Integrations
APPROVED

Ankita
4/14/2021 8:50:02 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 06:04:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

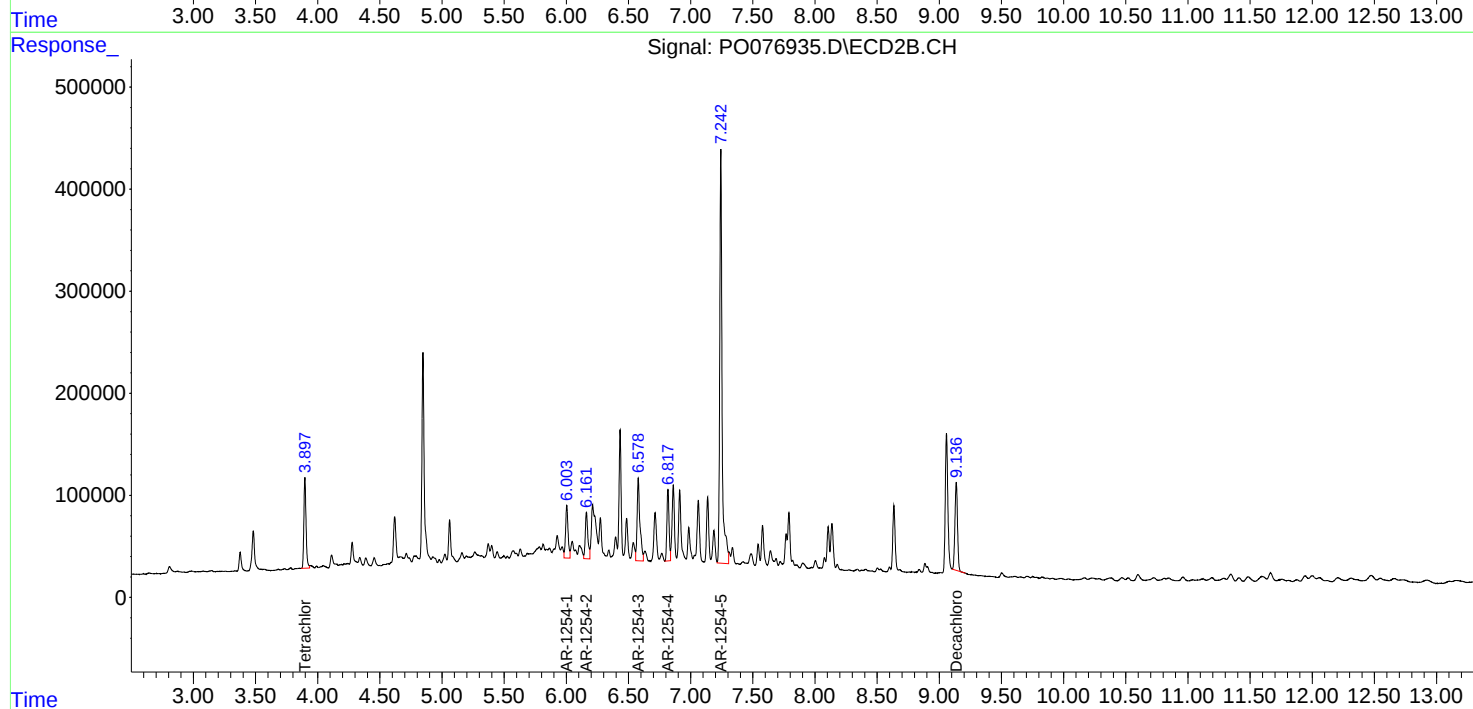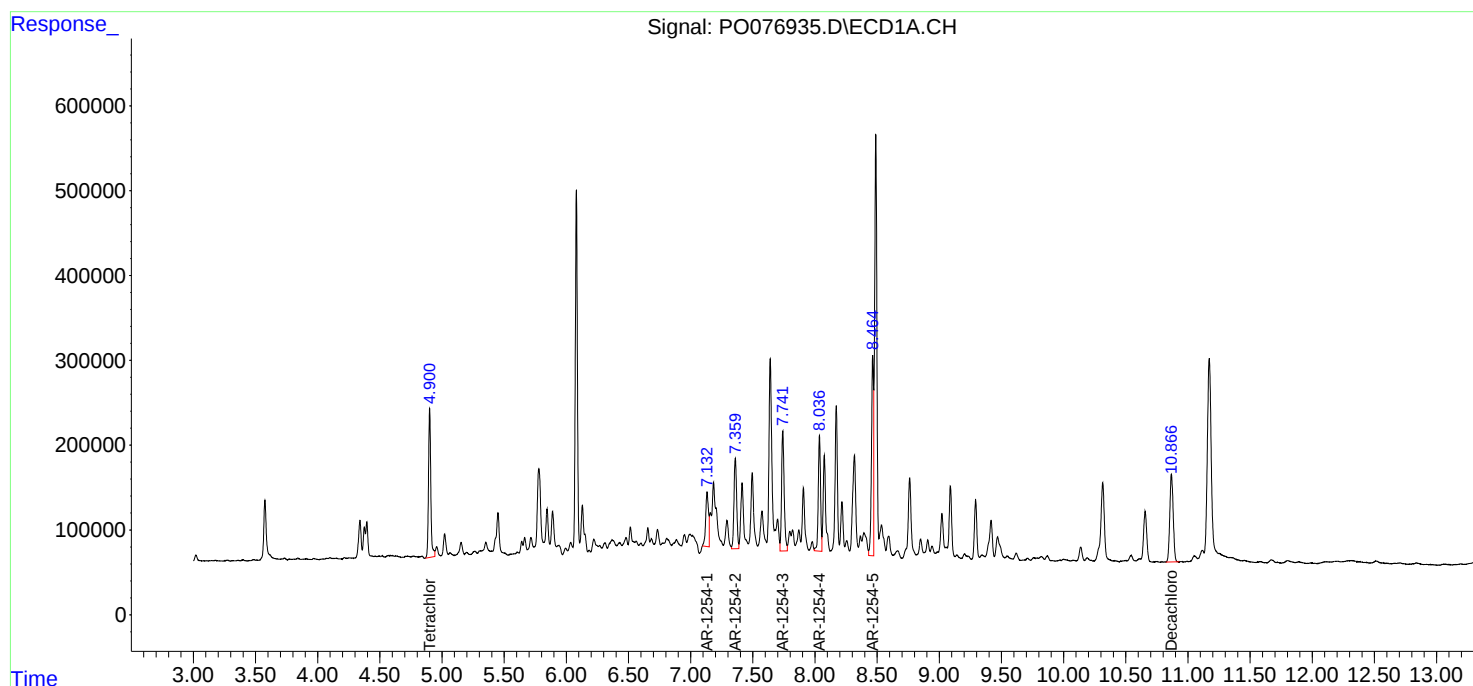

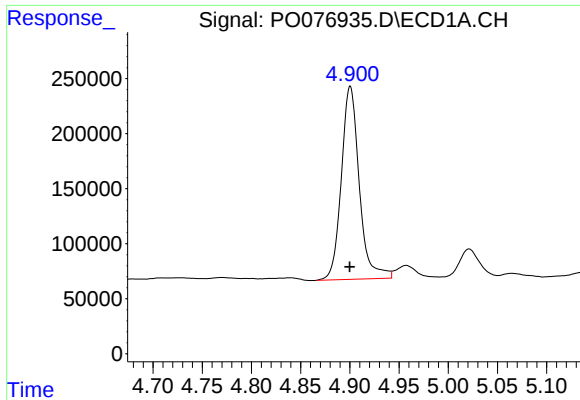


#1 Tetrachloro-m-xylene

R.T.: 4.900 min
Delta R.T.: 0.000 min
Response: 2226082
Conc: 23.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
HA-02


Manual Integrations
APPROVED

Ankita
4/14/2021 8:50:02 AM

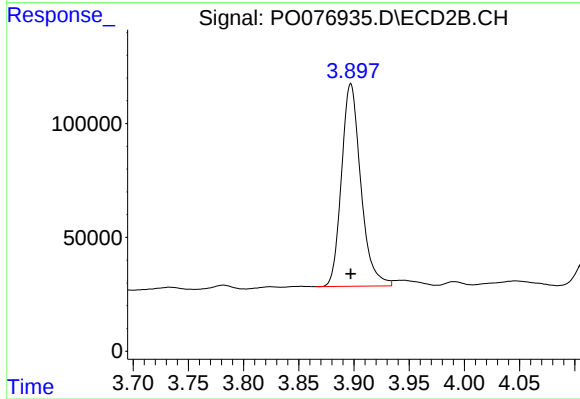


#1 Tetrachloro-m-xylene

R.T.: 3.897 min
Delta R.T.: 0.000 min
Response: 1081845
Conc: 21.56 ng/ml

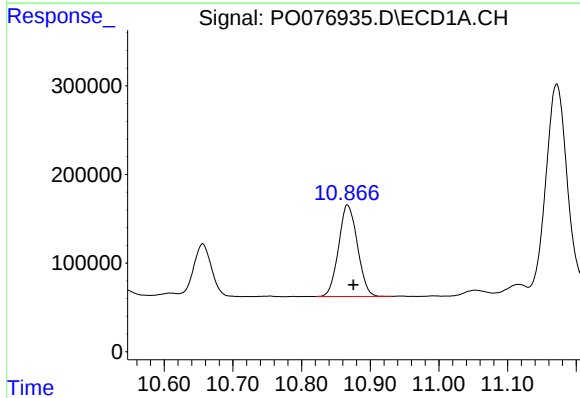


#2 Decachlorobiphenyl

R.T.: 10.867 min
Delta R.T.: -0.009 min
Response: 1968292
Conc: 21.25 ng/ml

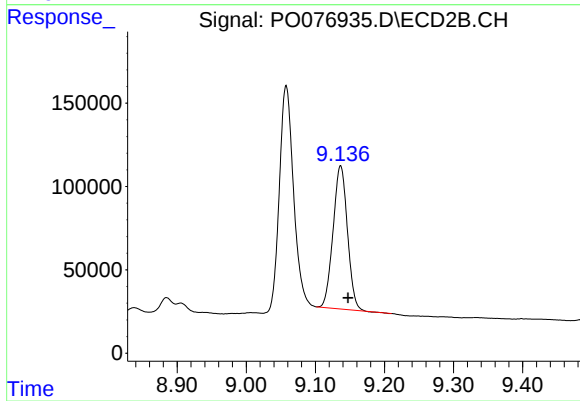

#2 Decachlorobiphenyl

R.T.: 9.137 min
Delta R.T.: -0.011 min
Response: 1234994
Conc: 25.45 ng/ml

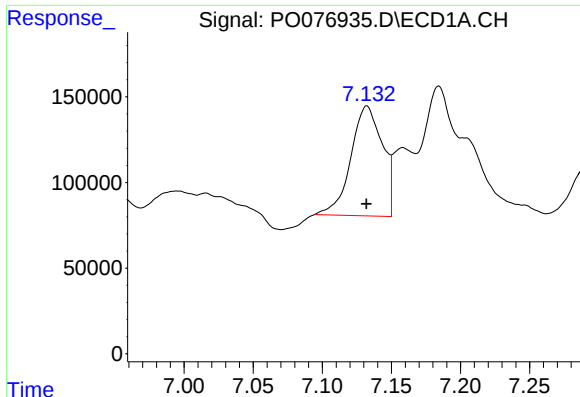


#26 AR-1254-1

R.T.: 7.132 min
Delta R.T.: 0.000 min
Response: 1044137
Conc: 328.50 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HA-02


Manual Integrations
APPROVED

Ankita
4/14/2021 8:50:02 AM

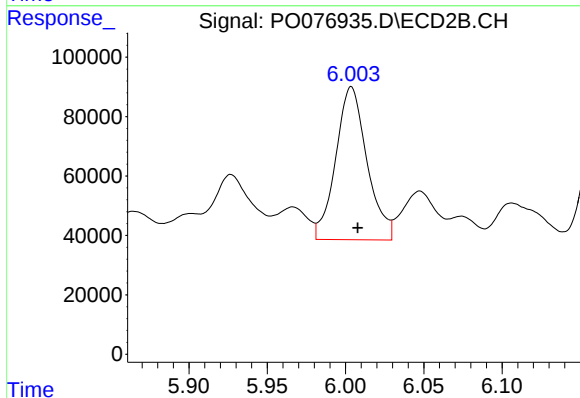


#26 AR-1254-1

R.T.: 6.004 min
Delta R.T.: -0.004 min
Response: 716298
Conc: 273.28 ng/ml

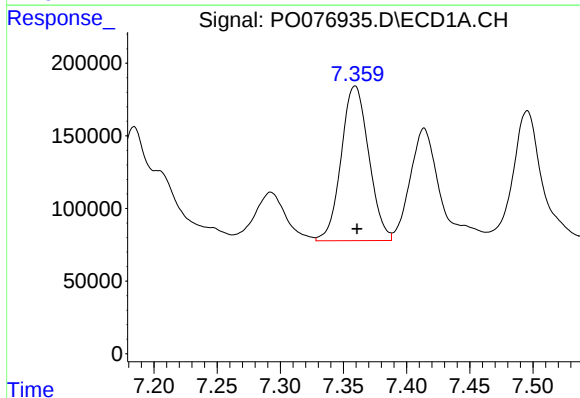


#27 AR-1254-2

R.T.: 7.359 min
Delta R.T.: -0.002 min
Response: 1617148
Conc: 315.62 ng/ml m

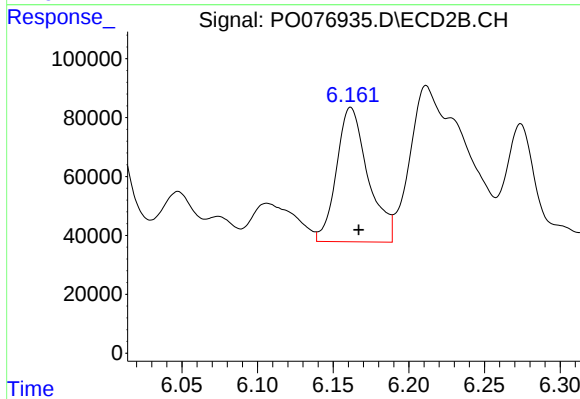

#27 AR-1254-2

R.T.: 6.162 min
Delta R.T.: -0.005 min
Response: 662037
Conc: 289.10 ng/ml

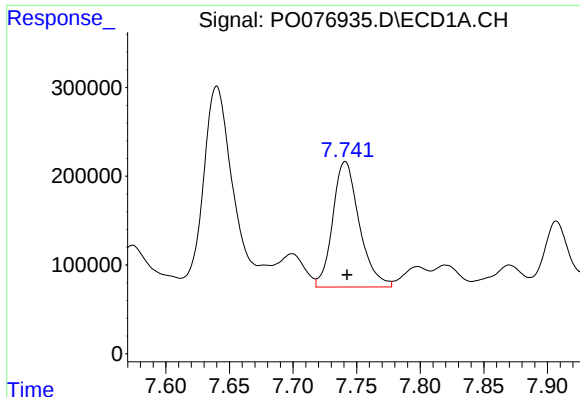


#28 AR-1254-3

R.T.: 7.741 min
Delta R.T.: -0.001 min
Response: 2053986
Conc: 372.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
HA-02


Manual Integrations
APPROVED

Ankita
4/14/2021 8:50:02 AM

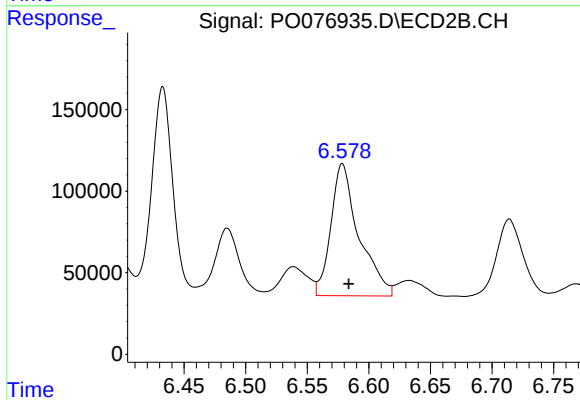


#28 AR-1254-3

R.T.: 6.578 min
Delta R.T.: -0.005 min
Response: 1282798
Conc: 362.96 ng/ml

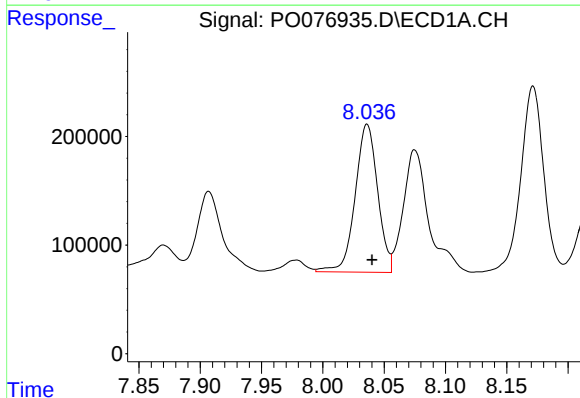


#29 AR-1254-4

R.T.: 8.036 min
Delta R.T.: -0.004 min
Response: 1740315
Conc: 442.01 ng/ml

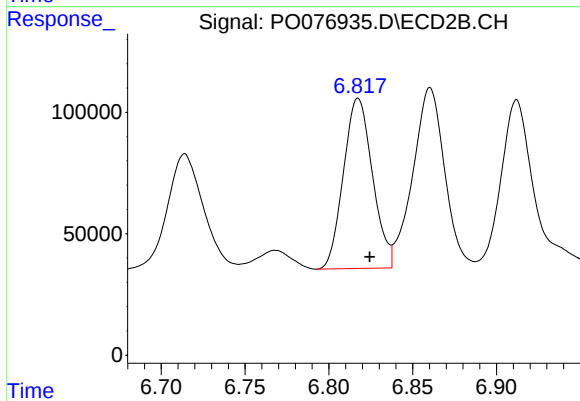

#29 AR-1254-4

R.T.: 6.817 min
Delta R.T.: -0.007 min
Response: 844295
Conc: 402.30 ng/ml

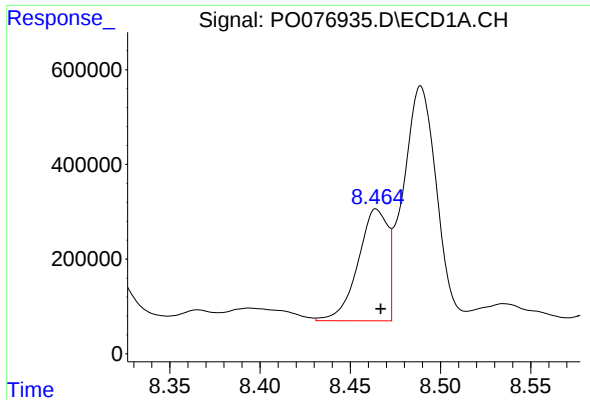


#30 AR-1254-5

R.T.: 8.464 min
Delta R.T.: -0.002 min
Response: 2712546
Conc: 616.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
HA-02

Manual Integrations
APPROVED

Ankita
4/14/2021 8:50:02 AM

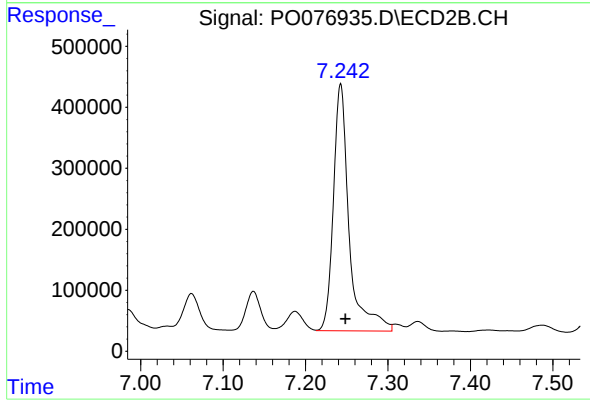

#30 AR-1254-5

R.T.: 7.243 min
Delta R.T.: -0.006 min
Response: 5395562
Conc: 1655.07 ng/ml