

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041223\
 Data File : P0094149.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Apr 2023 17:36
 Operator : YP/AJ
 Sample : 02283-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 20230328-COMP-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 12 22:25:42 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.421	3.624	67416203	25699032	18.034	20.181
2) SA Decachlor...	10.247	8.647	40959072	18960142	18.310	18.964

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041223\
Data File : PO094149.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Apr 2023 17:36
Operator : YP/AJ
Sample : 02283-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20230328-COMP-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 12 22:25:42 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

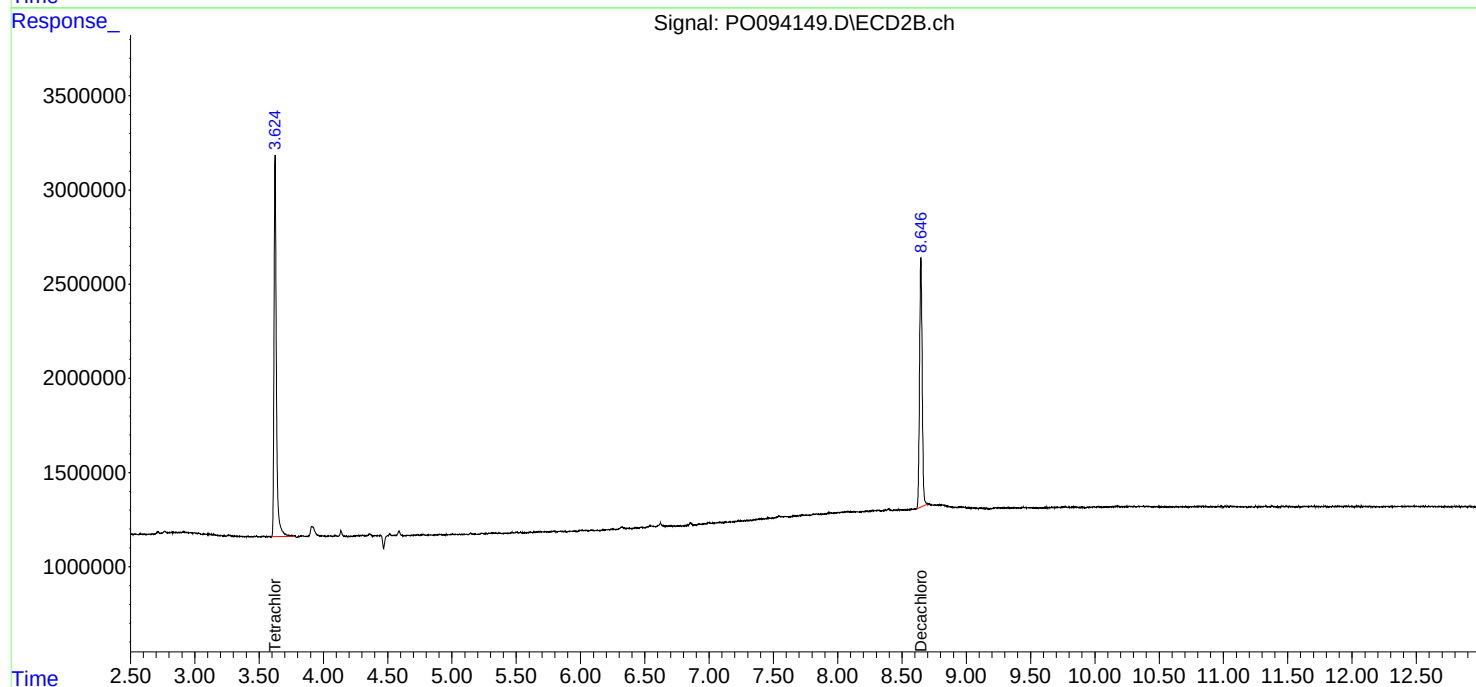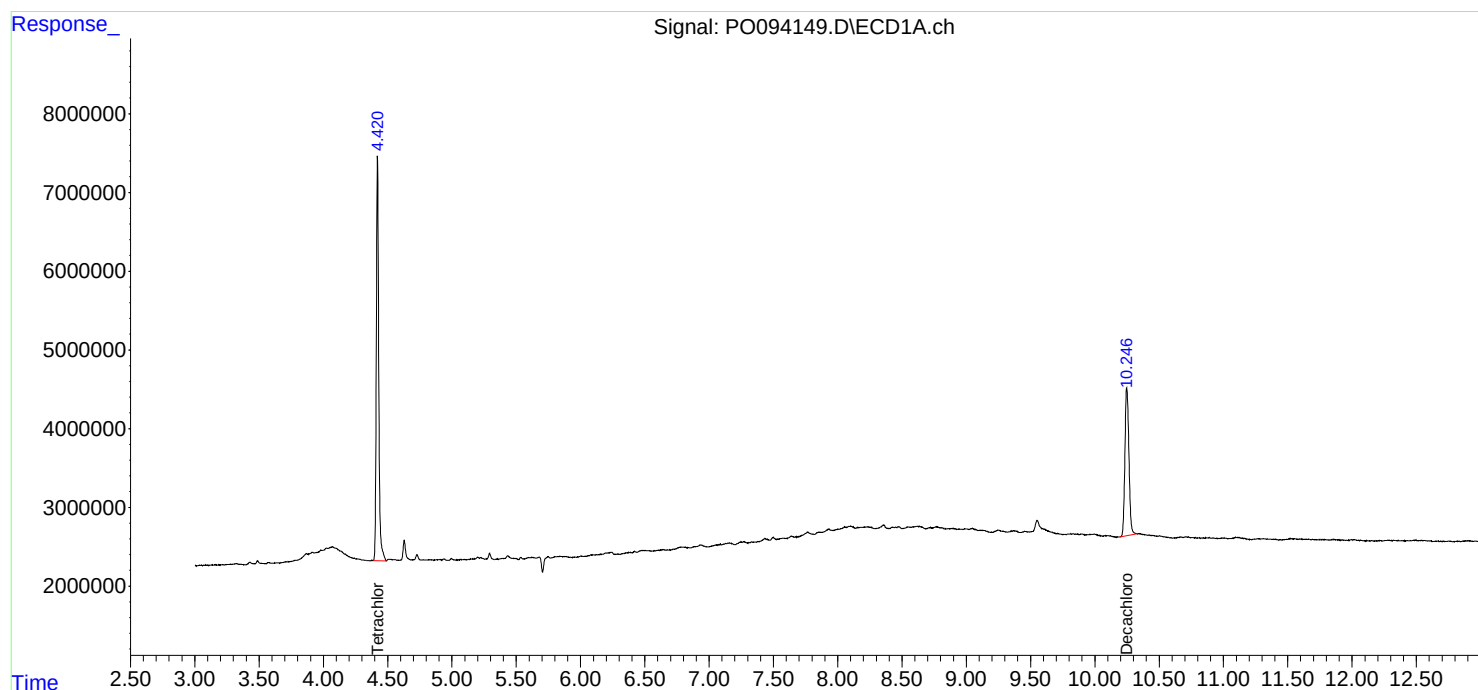


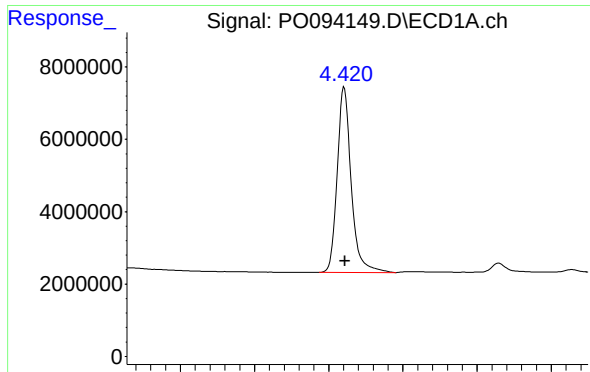

#1 Tetrachloro-m-xylene


R.T.: 4.421 min
Delta R.T.: -0.001 min
Response: 67416203
Conc: 18.03 ng/ml

Instrument :
ECD_O
ClientSampleId :
20230328-COMP-6

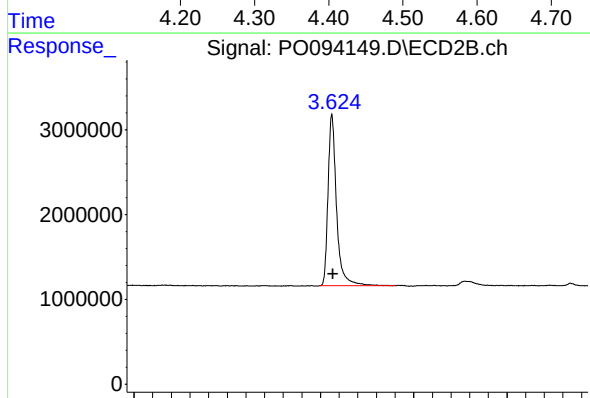


#1 Tetrachloro-m-xylene

R.T.: 3.624 min
Delta R.T.: -0.002 min
Response: 25699032
Conc: 20.18 ng/ml

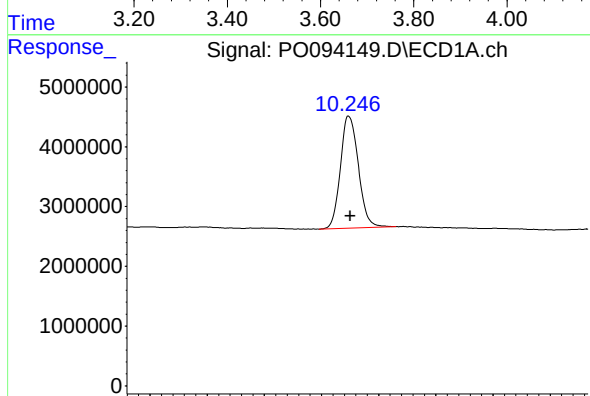

#2 Decachlorobiphenyl

R.T.: 10.247 min
Delta R.T.: -0.003 min
Response: 40959072
Conc: 18.31 ng/ml

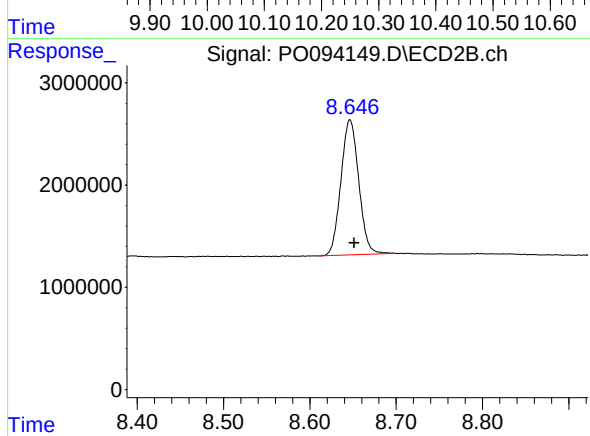

#2 Decachlorobiphenyl

R.T.: 8.647 min
Delta R.T.: -0.005 min
Response: 18960142
Conc: 18.96 ng/ml