

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041223\
 Data File : P0094175.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2023 02:02
 Operator : YP/AJ
 Sample : 02286-03 10X
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 3134

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/13/2023
 Supervised By :Ankita Jodhani 04/13/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 05:43:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Apr 04 06:20:55 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.419	3.622	6429561	1607768	1.720m	1.263 #
2) SA Decachlor...	10.247	8.645	7071448	2716010	3.161	2.717

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041223\
Data File : PO094175.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2023 02:02
Operator : YP/AJ
Sample : 02286-03 10X
Misc :
ALS Vial : 38 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
3134


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/13/2023
Supervised By :Ankita Jodhani 04/13/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 05:43:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040323.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Apr 04 06:20:55 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

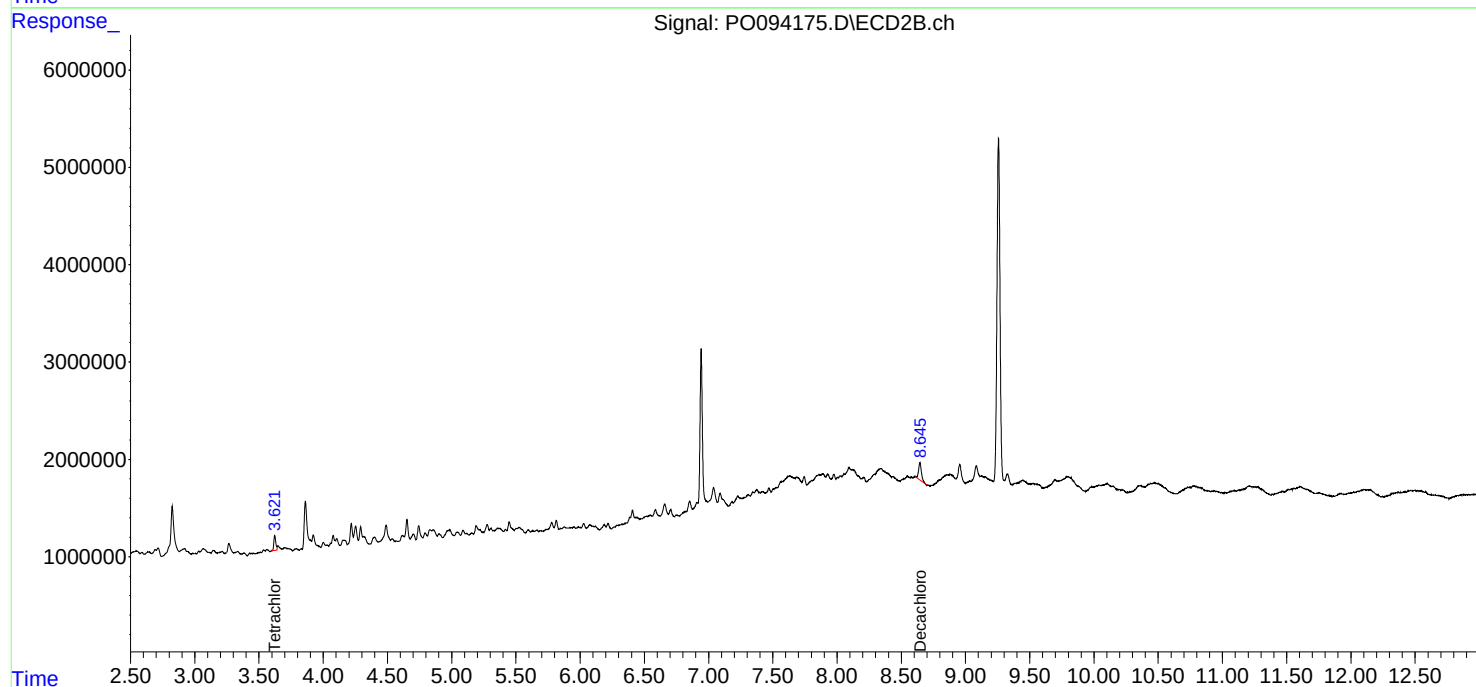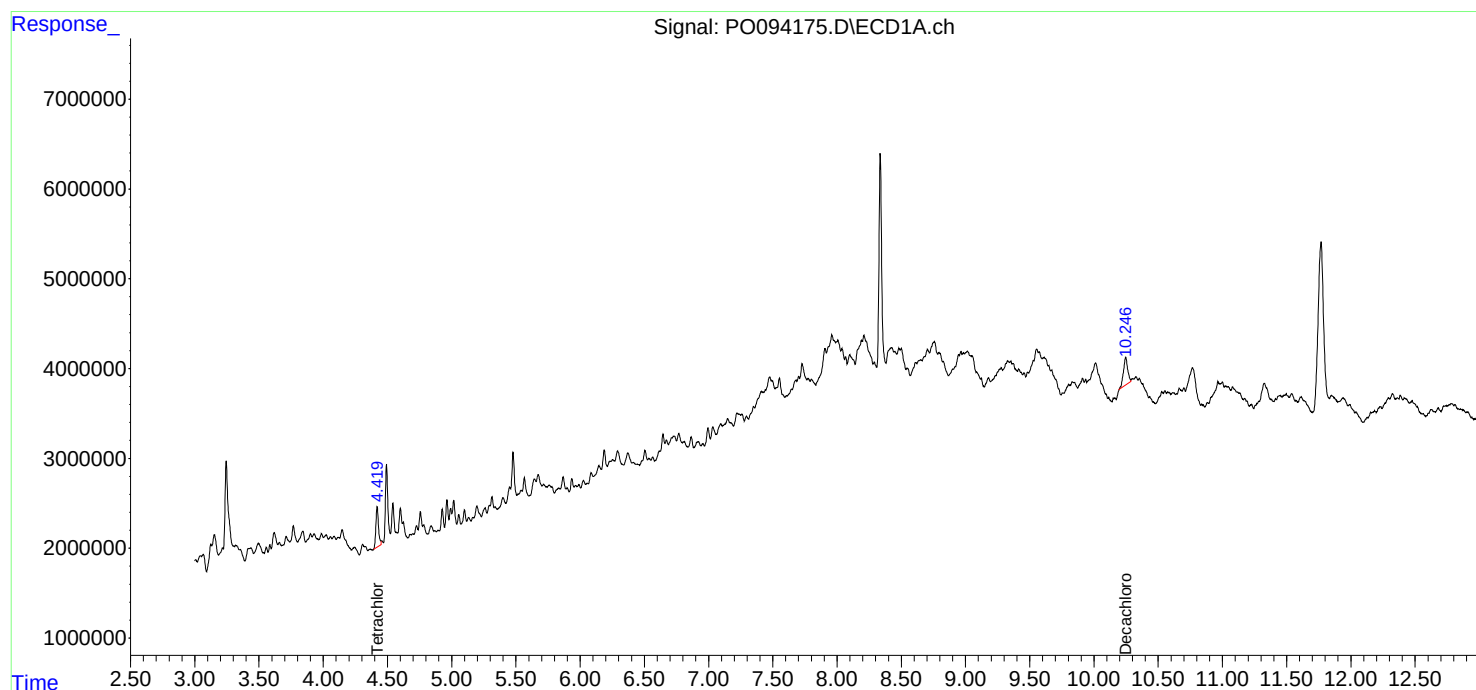

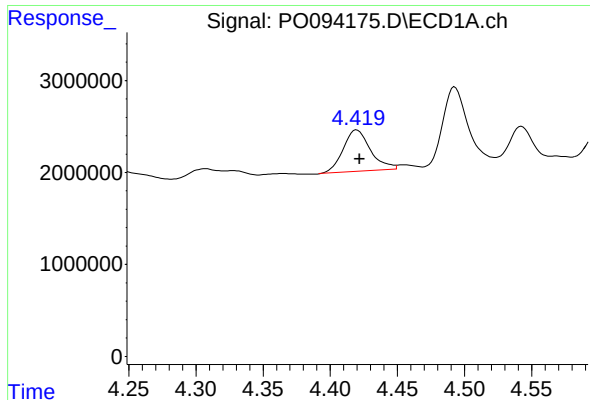


#1 Tetrachloro-m-xylene

R.T.: 4.419 min
Delta R.T.: -0.003 min
Response: 6429561
Conc: 1.72 ng/ml

Instrument :
ECD_O
ClientSampleId :
3134


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/13/2023
Supervised By :Ankita Jodhani 04/13/2023

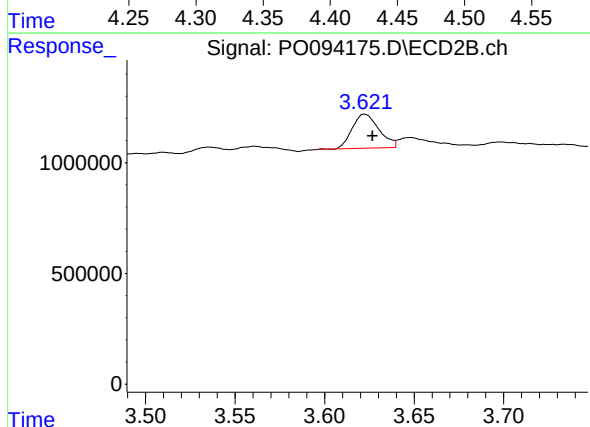


#1 Tetrachloro-m-xylene

R.T.: 3.622 min
Delta R.T.: -0.004 min
Response: 1607768
Conc: 1.26 ng/ml

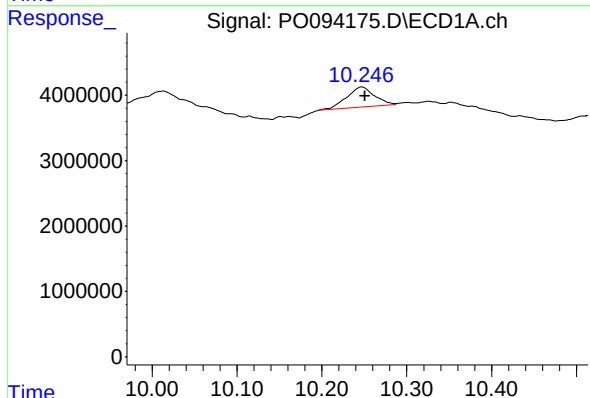

#2 Decachlorobiphenyl

R.T.: 10.247 min
Delta R.T.: -0.004 min
Response: 7071448
Conc: 3.16 ng/ml

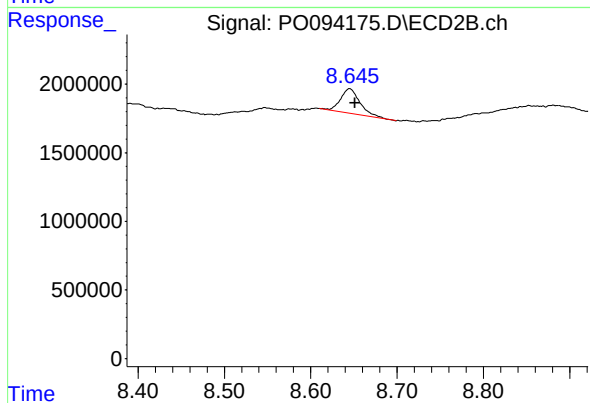

#2 Decachlorobiphenyl

R.T.: 8.645 min
Delta R.T.: -0.006 min
Response: 2716010
Conc: 2.72 ng/ml