

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR032119\
 Data File : PR036457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 21 Mar 2019 11:39
 Operator : SM\SJ
 Sample : K1971-04 10X (Sig #1); K1971-04DL 10X (Sig #2)
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 15 04:29:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR032019.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 20 15:19:33 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.403	3.476	3166788	8054811	2.092	1.964
2) SA Decachlor...	10.055	8.340	2398836	6748802	1.369	1.220

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_R\Data\PR032119\
Data File : PR036457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 21 Mar 2019 11:39
Operator : SM\SJ
Sample : K1971-04 10X (Sig #1); K1971-04DL 10X (Sig #2)
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 15 04:29:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_R\Method\PR032019.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 20 15:19:33 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

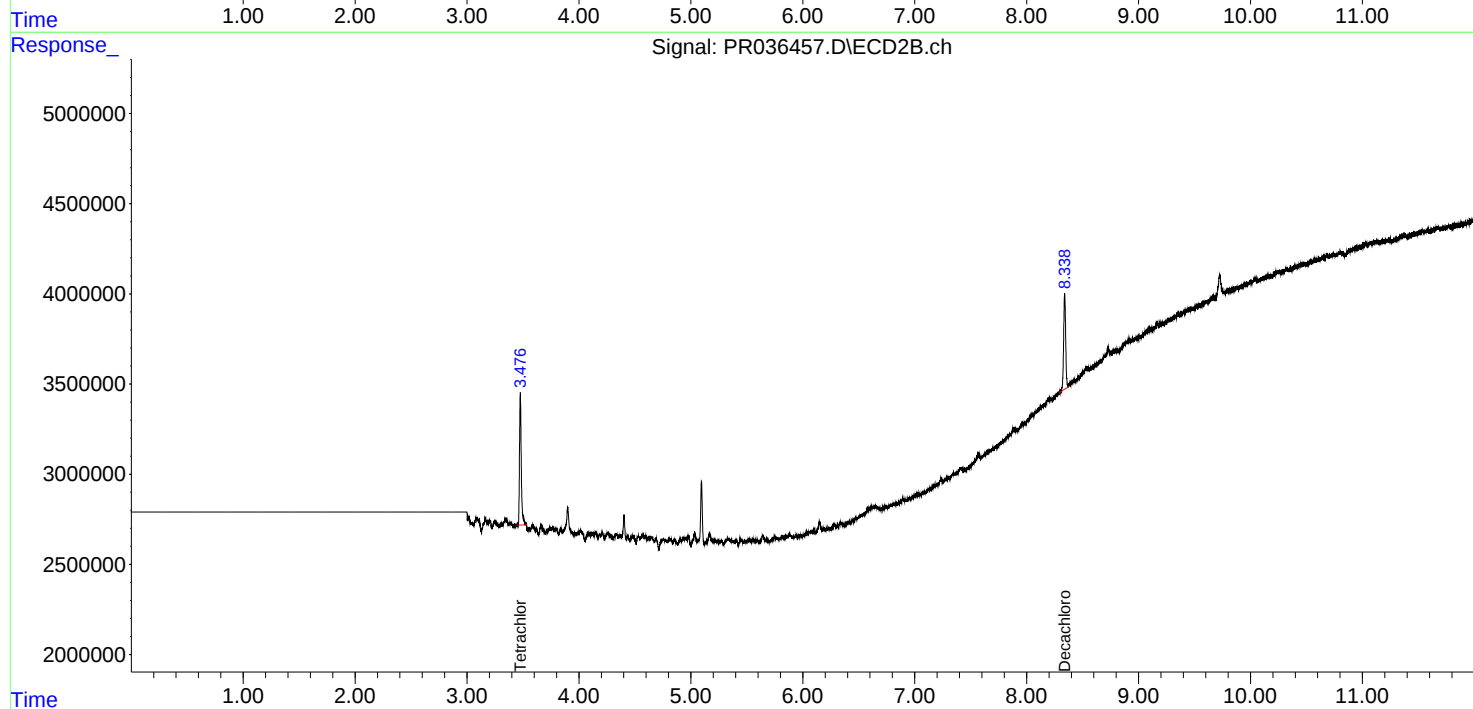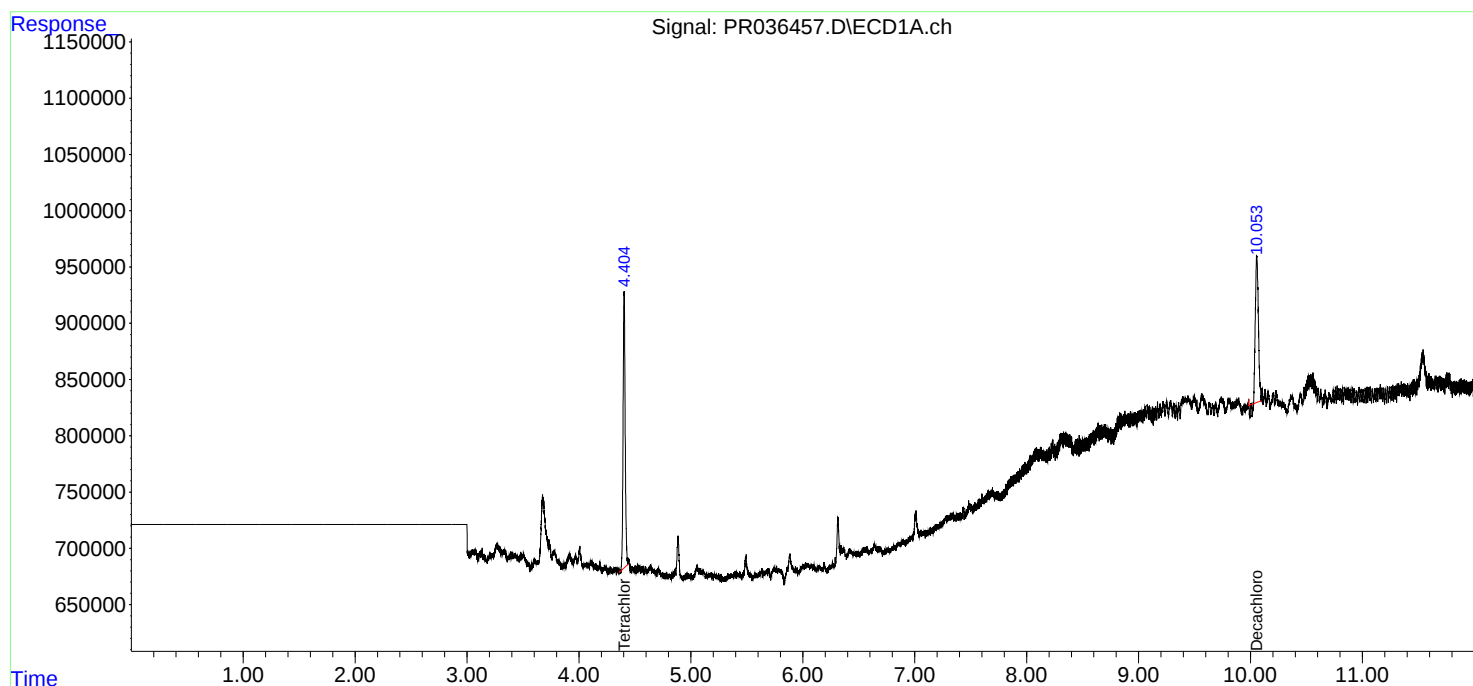


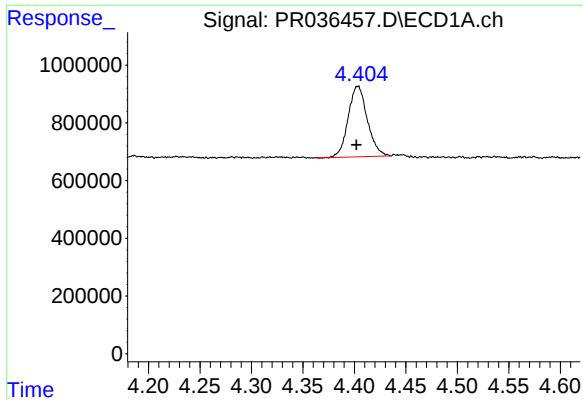

#1 Tetrachloro-m-xylene


R.T.: 4.403 min
Delta R.T.: 0.001 min
Response: 3166788
Conc: 2.09 ng/ml

Instrument :
ECD_O
ClientSampleId :

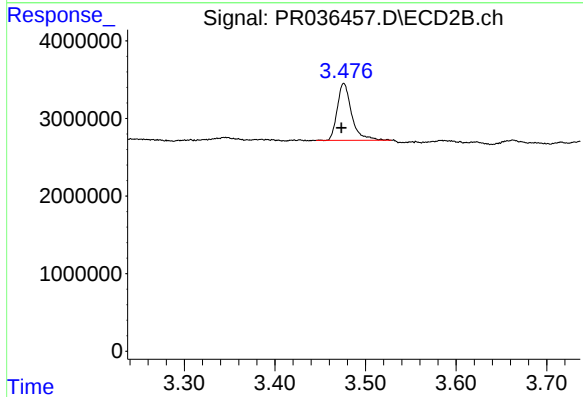


#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: 0.003 min
Response: 8054811
Conc: 1.96 ng/ml

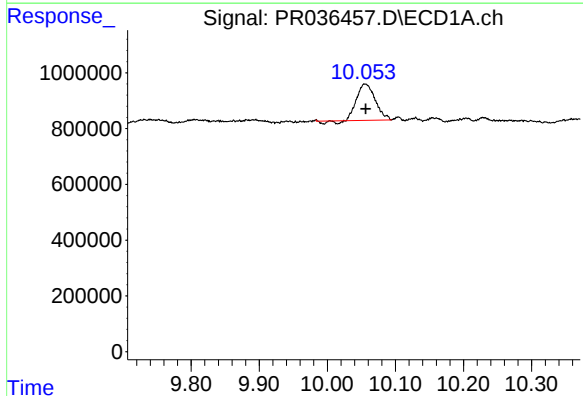

#2 Decachlorobiphenyl

R.T.: 10.055 min
Delta R.T.: -0.001 min
Response: 2398836
Conc: 1.37 ng/ml

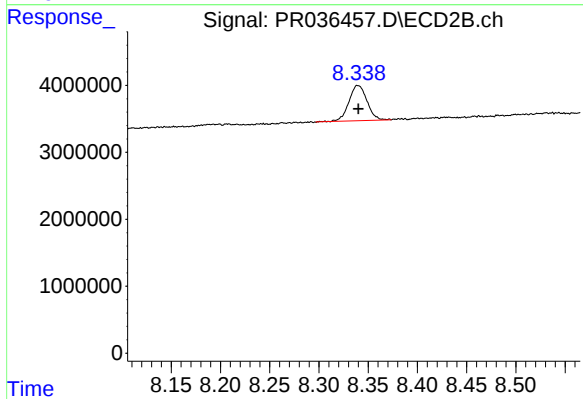

#2 Decachlorobiphenyl

R.T.: 8.340 min
Delta R.T.: 0.000 min
Response: 6748802
Conc: 1.22 ng/ml