

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041321\
 Data File : PL066071.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2021 10:00
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 08:47:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041321.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 08:43:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds



Target Compounds							
2) A	alpha-BHC	3.873	0.000	3655762	0	0.887	N.D. #
4) MA	Heptachlor	0.000	5.351f	0	2478579	N.D.	0.450 #
6) B	beta-BHC	4.408	5.033	3056695	7283029	1.769	2.667 #
14) MA	Endrin	5.975	0.000	1456541	0	0.435	N.D. #
15) B	Endosulfa...	6.266f	7.133	2311096	2586398	0.707	0.752
21) B	Endrin ke...	0.000	7.971	0	973843	N.D.	0.265 #
22)	Mirex	0.000	8.447f	0	522298	N.D.	0.188 #
23)	Chlordane-1	0.000	5.201f	0	8001894	N.D.	46.052 #
24)	Chlordane-2	0.000	5.648	0	6404389	N.D.	34.791 #
27)	Chlordane-5	6.266	0.000	2311096	0	15.516	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041321\
Data File : PL066071.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2021 10:00
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 08:47:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041321.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 08:43:04 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

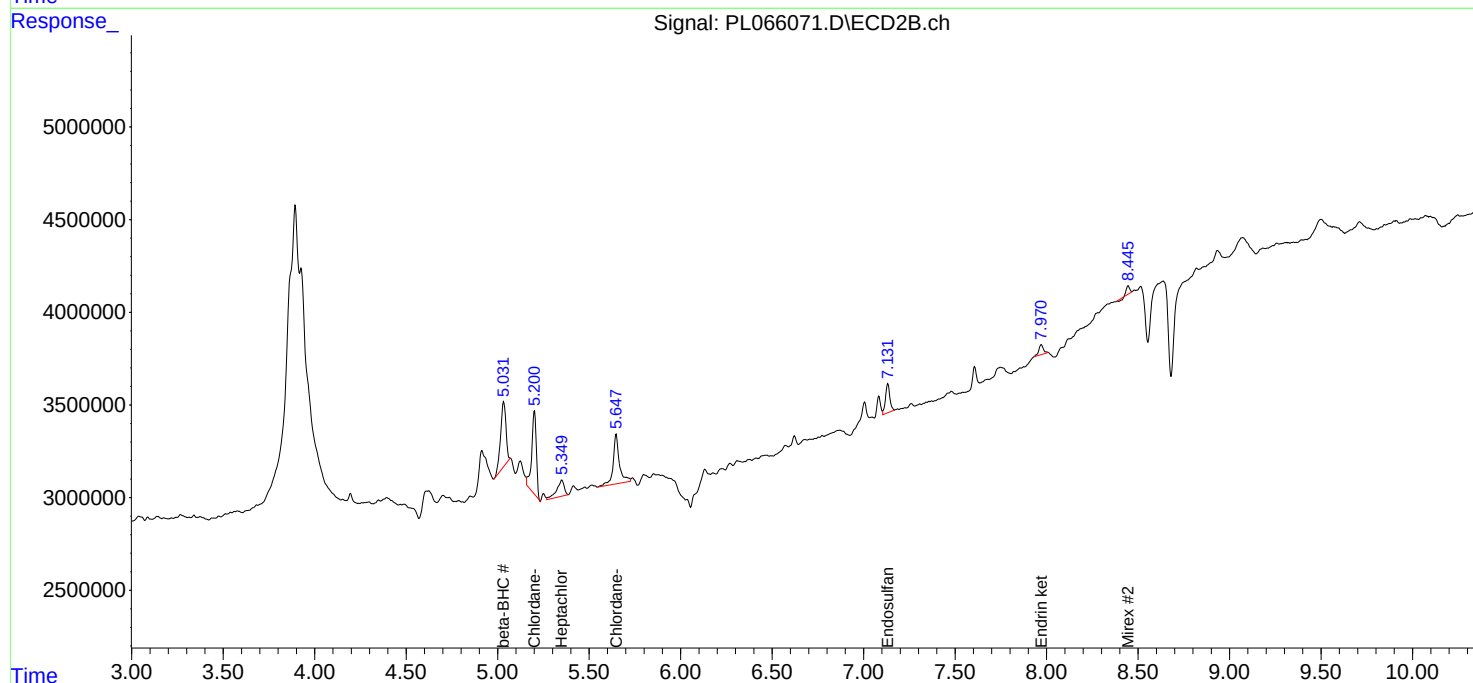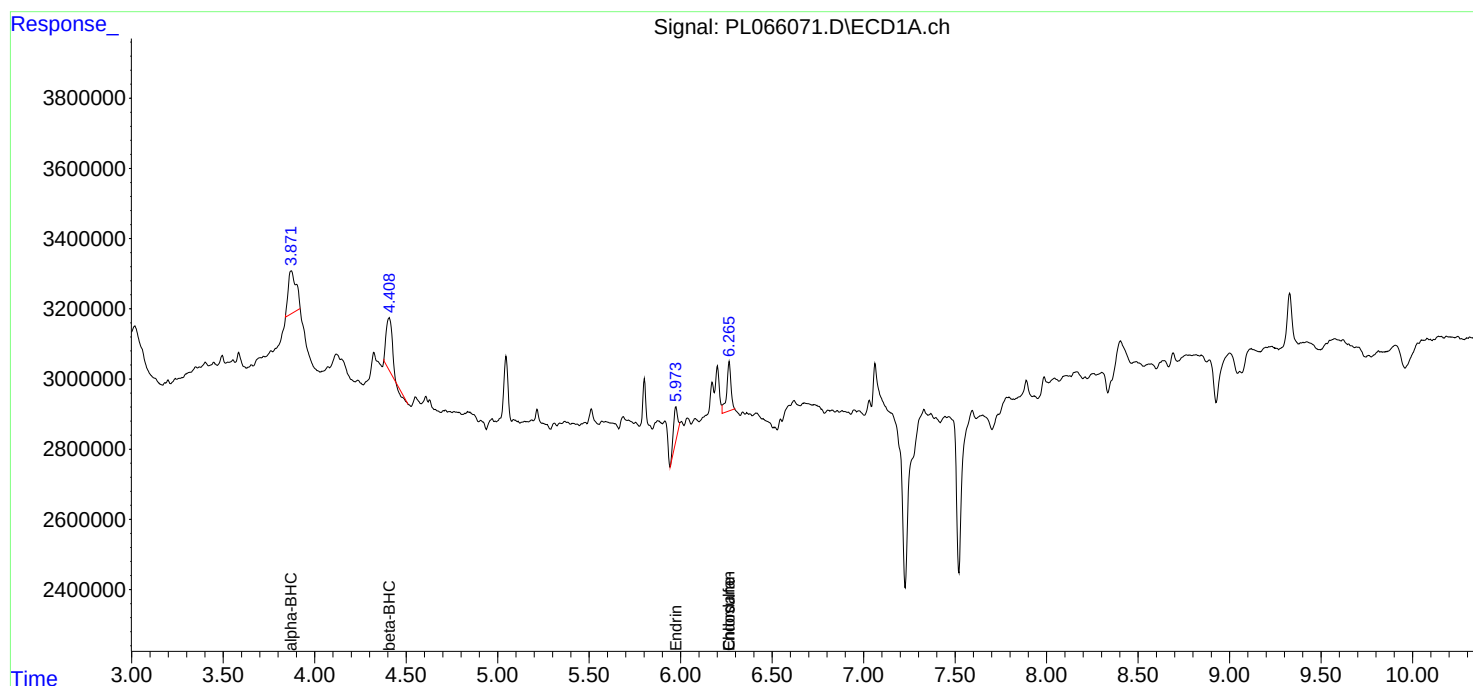

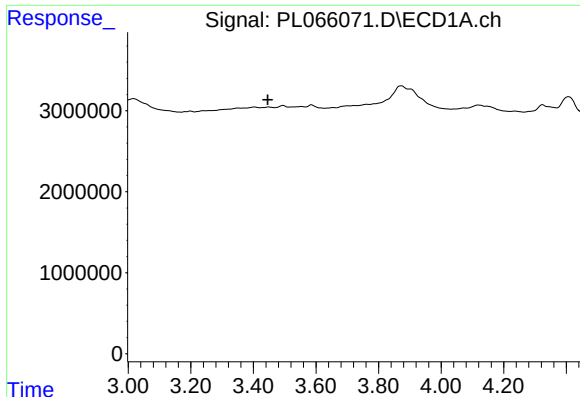


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.446 min
Response: 0
Conc: N.D.

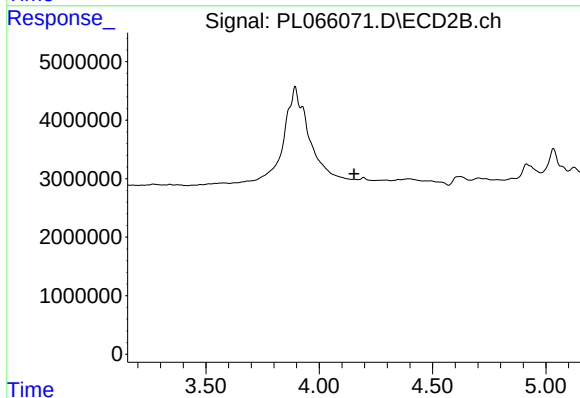


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.153 min
Response: 0
Conc: N.D.

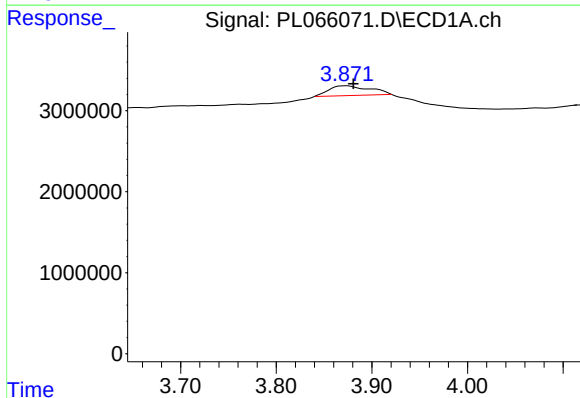


#2 alpha-BHC

R.T.: 3.873 min
Delta R.T.: -0.008 min
Response: 3655762
Conc: 0.89 ng/ml

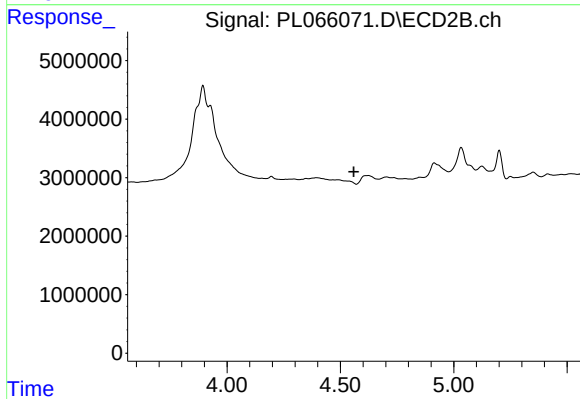


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 4.559 min
Response: 0
Conc: N.D.

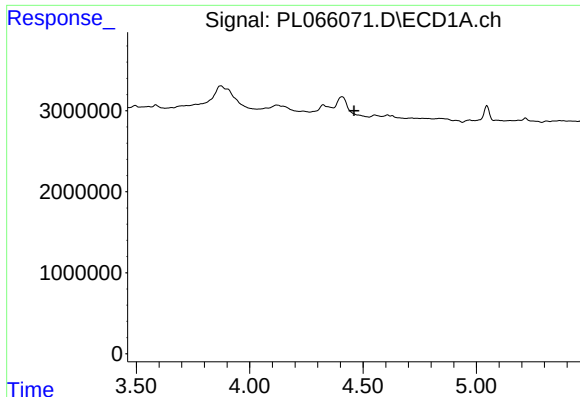


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 4.460 min
Response: 0
Conc: N.D.

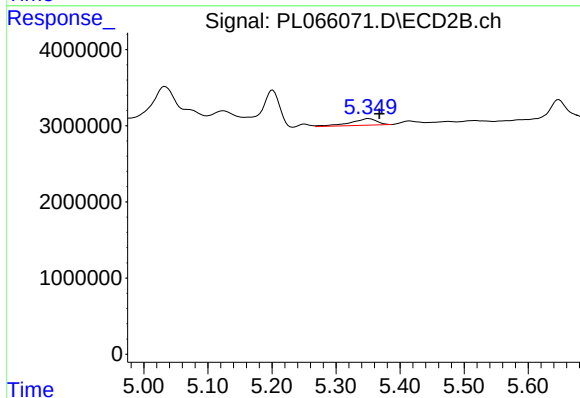


#4 Heptachlor

R.T.: 5.351 min
Delta R.T.: -0.017 min
Response: 2478579
Conc: 0.45 ng/ml

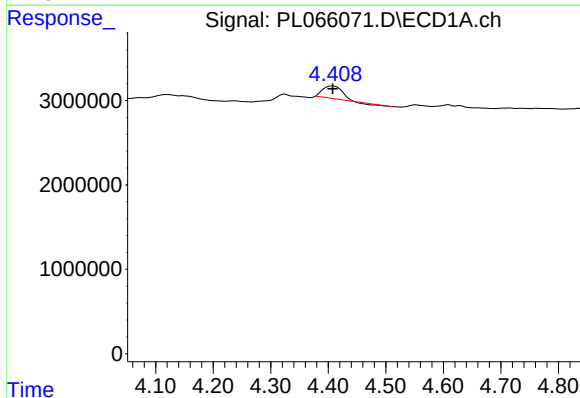


#6 beta-BHC

R.T.: 4.408 min
Delta R.T.: 0.000 min
Response: 3056695
Conc: 1.77 ng/ml

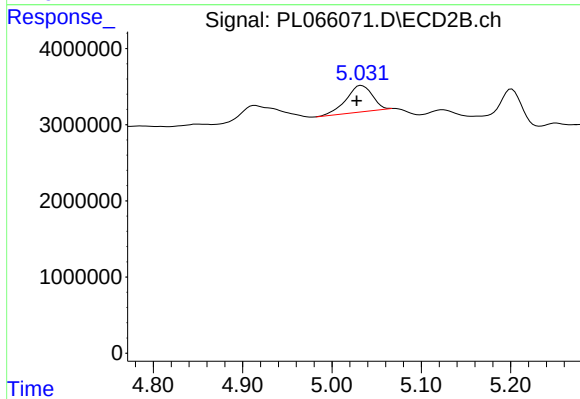


#6 beta-BHC

R.T.: 5.033 min
Delta R.T.: 0.005 min
Response: 7283029
Conc: 2.67 ng/ml

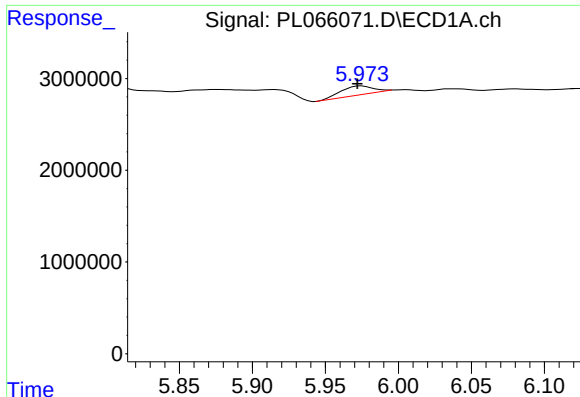


#14 Endrin

R.T.: 5.975 min
Delta R.T.: 0.003 min
Response: 1456541
Conc: 0.44 ng/ml

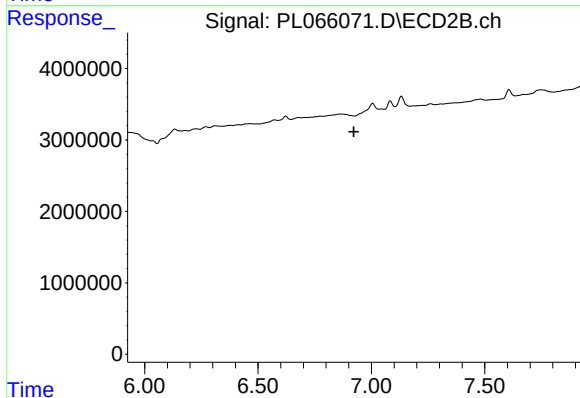


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.922 min
Response: 0
Conc: N.D.

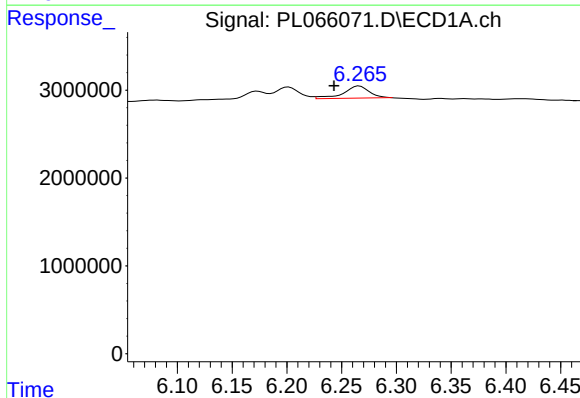


#15 Endosulfan II

R.T.: 6.266 min
Delta R.T.: 0.023 min
Response: 2311096
Conc: 0.71 ng/ml

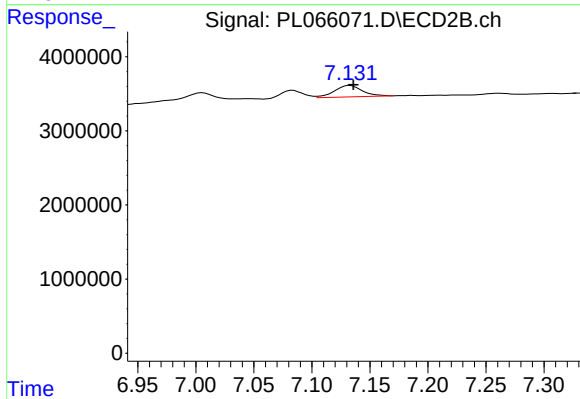


#15 Endosulfan II

R.T.: 7.133 min
Delta R.T.: -0.003 min
Response: 2586398
Conc: 0.75 ng/ml

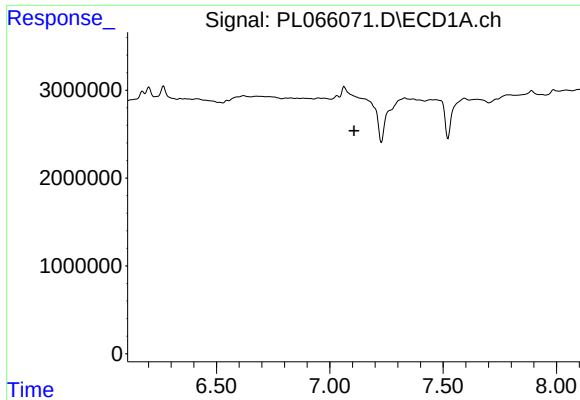


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.107 min
Response: 0
Conc: N.D.

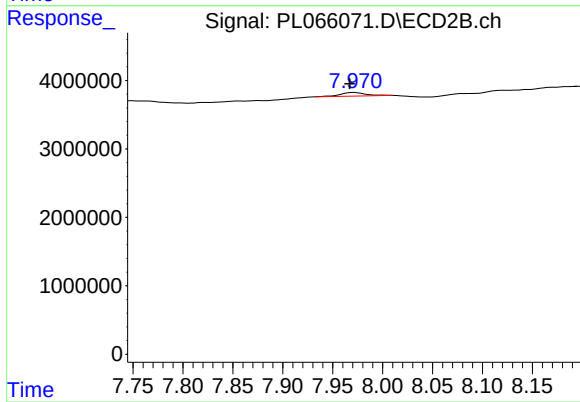


#21 Endrin ketone

R.T.: 7.971 min
Delta R.T.: 0.004 min
Response: 973843
Conc: 0.27 ng/ml

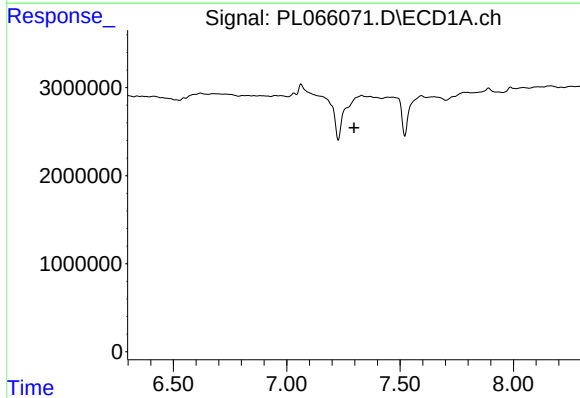


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.297 min
Response: 0
Conc: N.D.

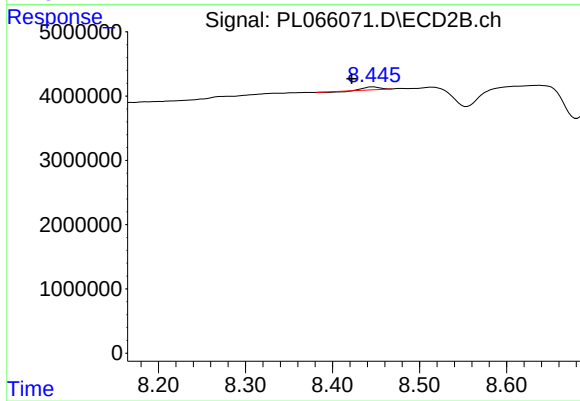


#22 Mirex

R.T.: 8.447 min
Delta R.T.: 0.024 min
Response: 522298
Conc: 0.19 ng/ml

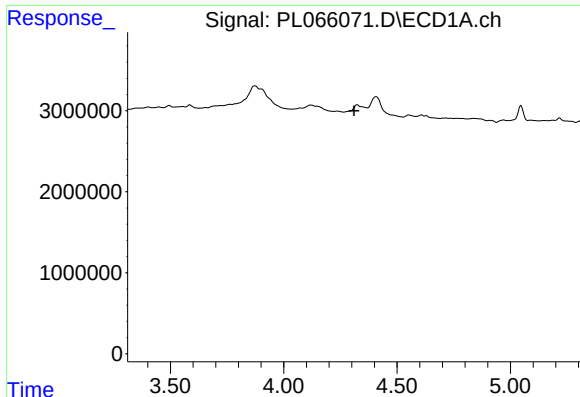


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.310 min
Response: 0
Conc: N.D.

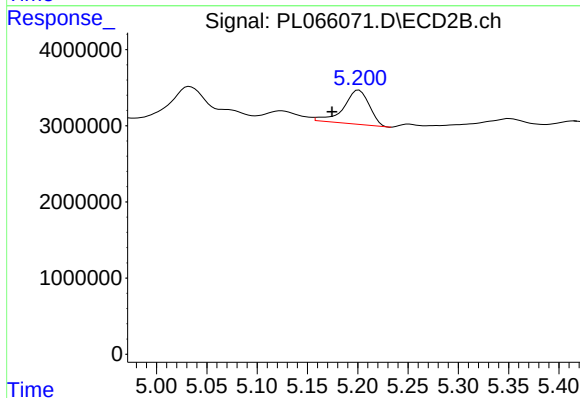


#23 Chlordane-1

R.T.: 5.201 min
Delta R.T.: 0.027 min
Response: 8001894
Conc: 46.05 ng/ml

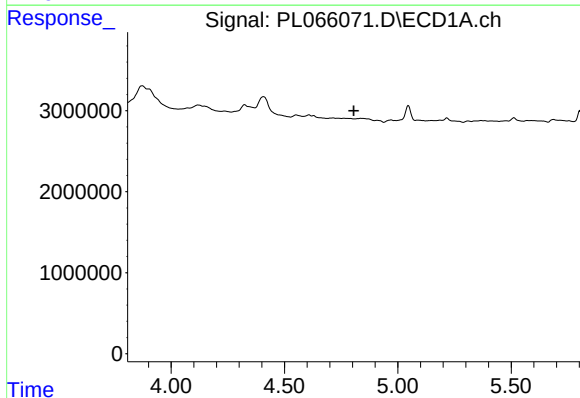


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.806 min
Response: 0
Conc: N.D.

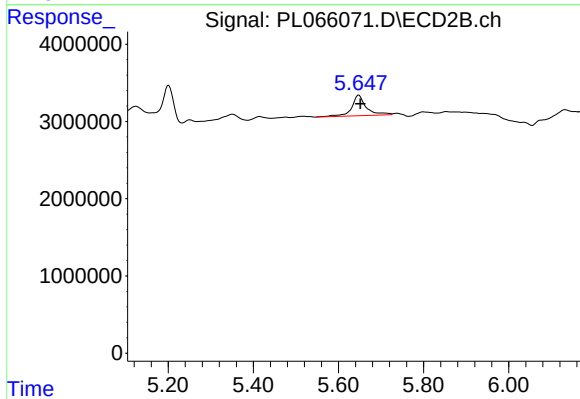


#24 Chlordane-2

R.T.: 5.648 min
Delta R.T.: -0.004 min
Response: 6404389
Conc: 34.79 ng/ml

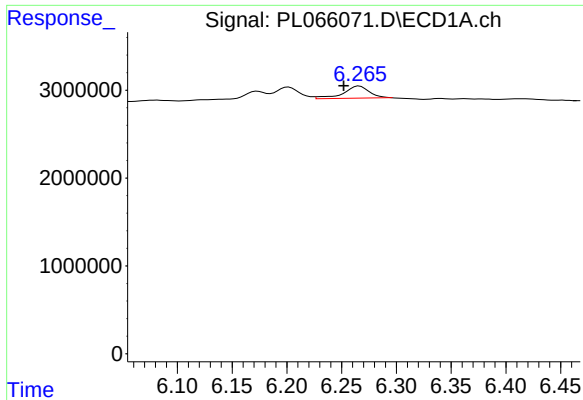


#27 Chlordane-5

R.T.: 6.266 min
Delta R.T.: 0.014 min
Response: 2311096
Conc: 15.52 ng/ml

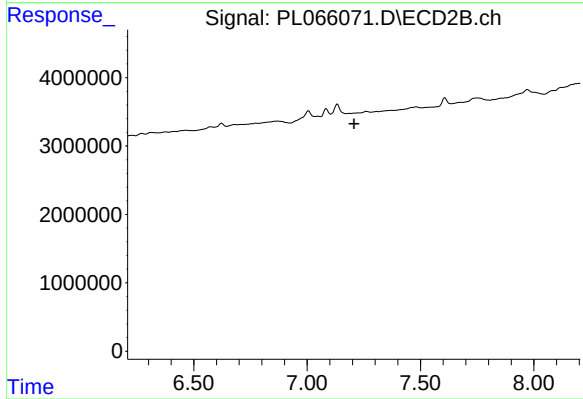


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.207 min
Response: 0
Conc: N.D.

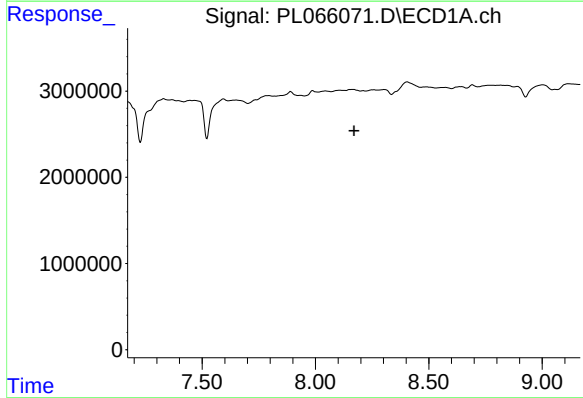

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.171 min
Response: 0
Conc: N.D.

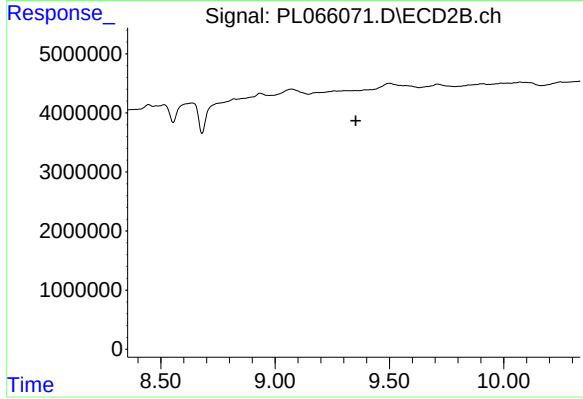

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.353 min
Response: 0
Conc: N.D.