

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041321\
 Data File : PL066076.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Apr 2021 15:42
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 08:48:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041321.M
 Quant Title : GC Extractables
 QLast Update : Wed Apr 14 08:43:04 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.445	4.153	47210100	75865031	19.095	19.154
28)	SA Decachlor...	8.170	9.351	47578554	64524293	20.214	20.014
Target Compounds							
2)	A alpha-BHC	3.869	0.000	4389993	0	1.065	N.D. #
6)	B beta-BHC	0.000	5.034	0	9971780	N.D.	3.652 #
8)	B Heptachlo...	0.000	6.067	0	4971482	N.D.	1.086 #
14)	MA Endrin	5.975	0.000	2217110	0	0.662	N.D. #
15)	B Endosulfa...	0.000	7.128	0	1505059	N.D.	0.437 #
17)	MA 4,4'-DDT	0.000	7.343	0	573512	N.D.	0.174 #
18)	B Endrin al...	0.000	7.258	0	888737	N.D.	0.320 #
21)	B Endrin ke...	7.091f	7.971	8111211	1594686	2.248	0.435 #
22)	Mirex	0.000	8.442f	0	509280	N.D.	0.183 #
23)	Chlordane-1	4.330f	0.000	2539143	0	21.177	N.D. #
24)	Chlordane-2	0.000	5.646	0	1302193	N.D.	7.074 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL041321\
Data File : PL066076.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Apr 2021 15:42
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 08:48:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL041321.M
Quant Title : GC Extractables
QLast Update : Wed Apr 14 08:43:04 2021
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

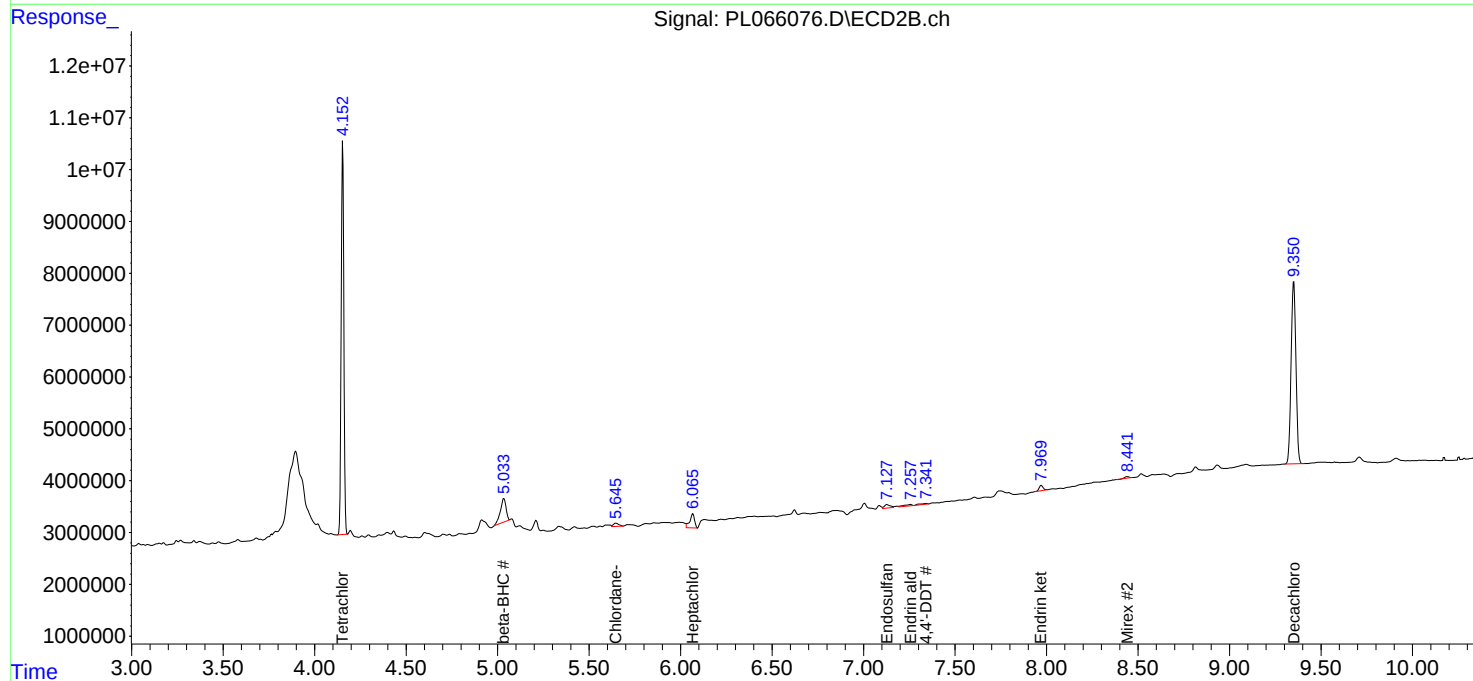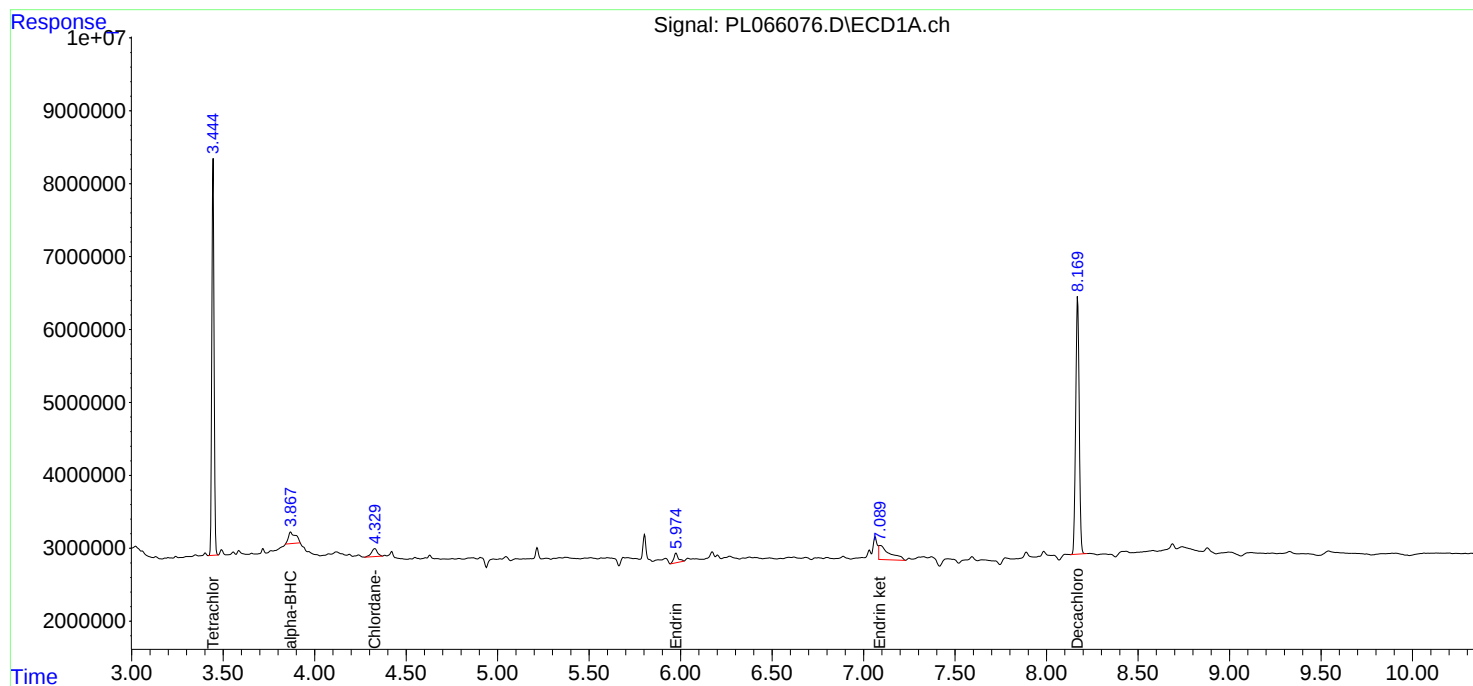

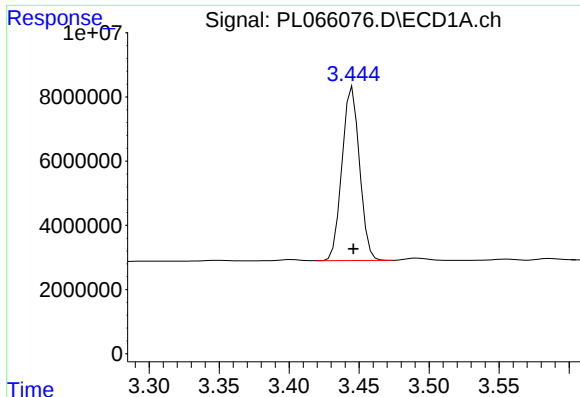


#1 Tetrachloro-m-xylene

R.T.: 3.445 min
Delta R.T.: 0.000 min
Response: 47210100
Conc: 19.10 ng/ml

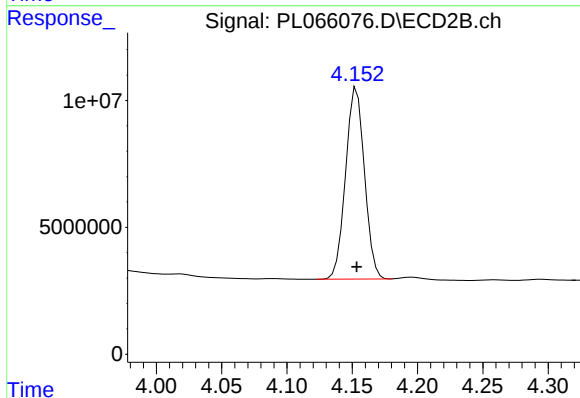


#1 Tetrachloro-m-xylene

R.T.: 4.153 min
Delta R.T.: 0.000 min
Response: 75865031
Conc: 19.15 ng/ml

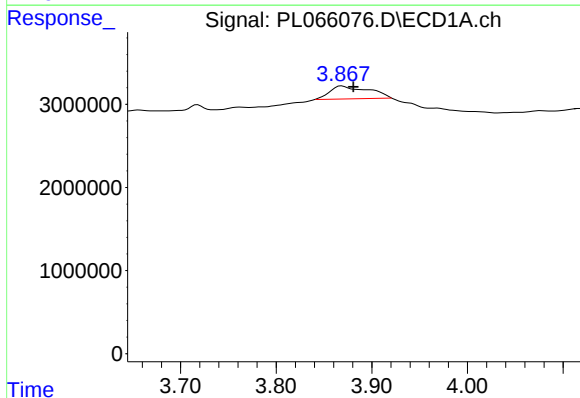


#2 alpha-BHC

R.T.: 3.869 min
Delta R.T.: -0.012 min
Response: 4389993
Conc: 1.07 ng/ml

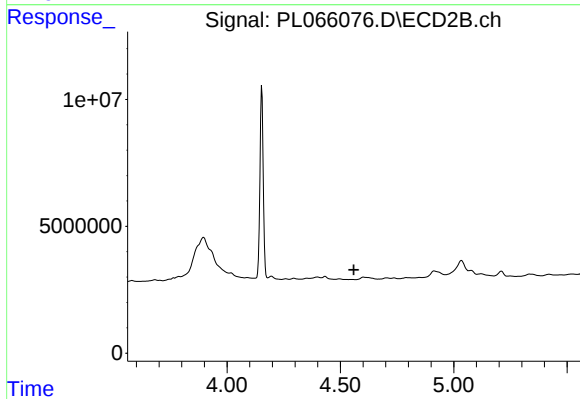


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T.: 4.559 min
Response: 0
Conc: N.D.

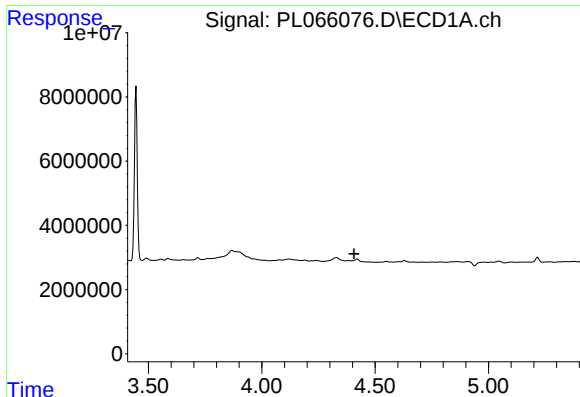


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.408 min
Response: 0
Conc: N.D.

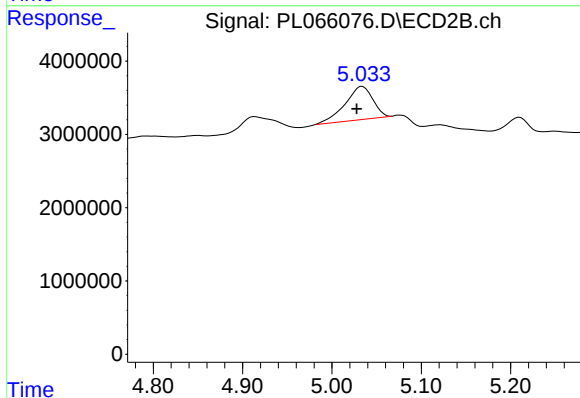


#6 beta-BHC

R.T.: 5.034 min
Delta R.T.: 0.006 min
Response: 9971780
Conc: 3.65 ng/ml

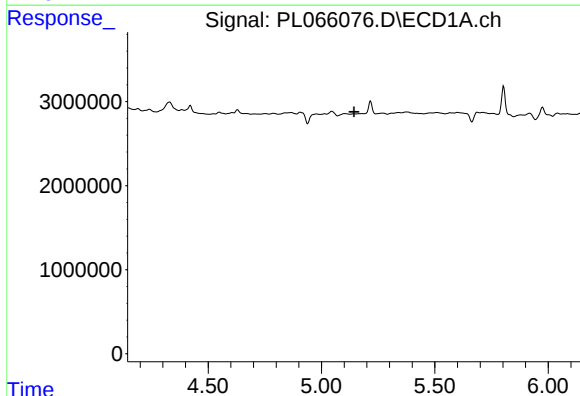


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.144 min
Response: 0
Conc: N.D.

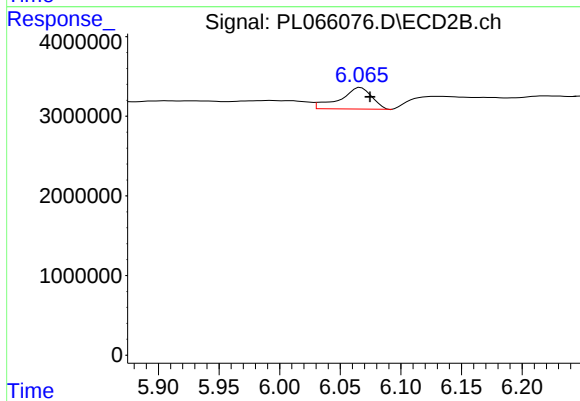


#8 Heptachlor epoxide

R.T.: 6.067 min
Delta R.T.: -0.008 min
Response: 4971482
Conc: 1.09 ng/ml

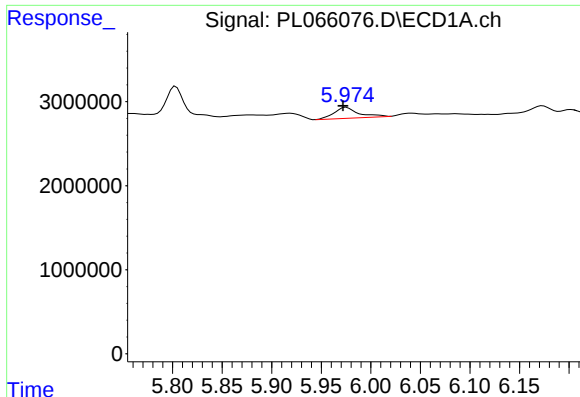


#14 Endrin

R.T.: 5.975 min
Delta R.T.: 0.003 min
Response: 2217110
Conc: 0.66 ng/ml

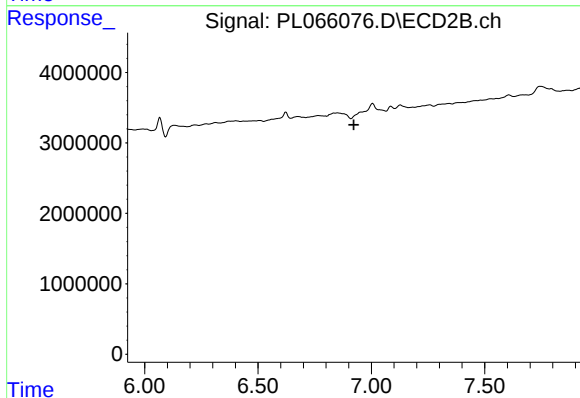


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.922 min
Response: 0
Conc: N.D.

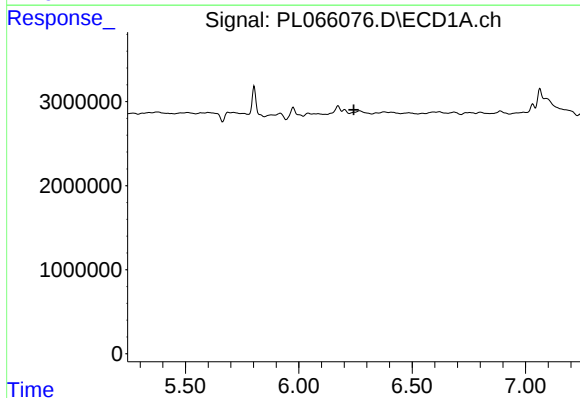


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.243 min
Response: 0
Conc: N.D.

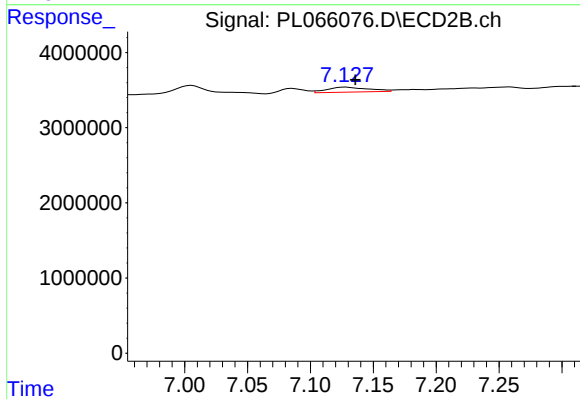


#15 Endosulfan II

R.T.: 7.128 min
Delta R.T.: -0.008 min
Response: 1505059
Conc: 0.44 ng/ml

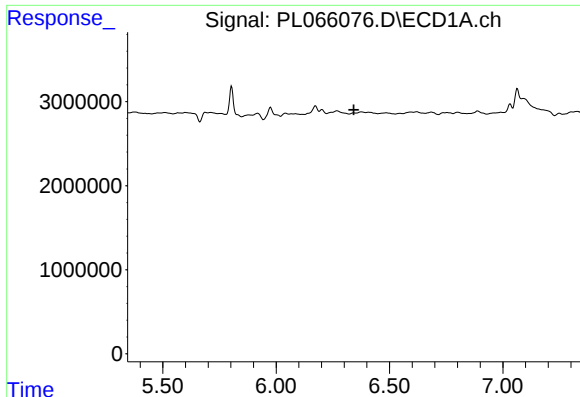


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 6.342 min
Response: 0
Conc: N.D.

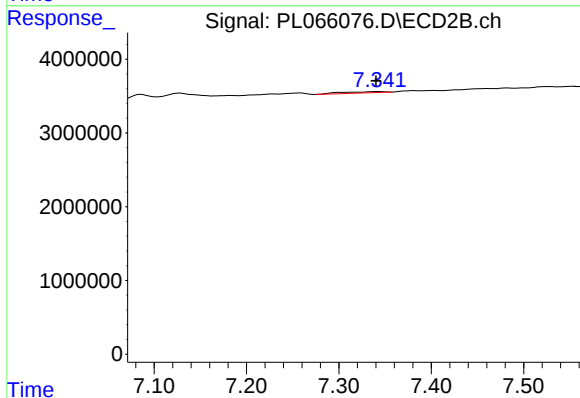


#17 4,4'-DDT

R.T.: 7.343 min
Delta R.T.: 0.003 min
Response: 573512
Conc: 0.17 ng/ml

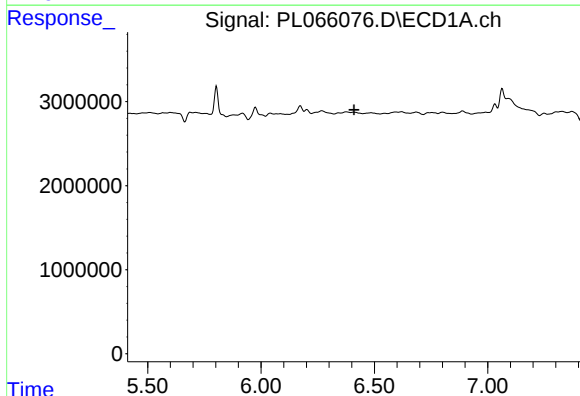


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.411 min
Response: 0
Conc: N.D.

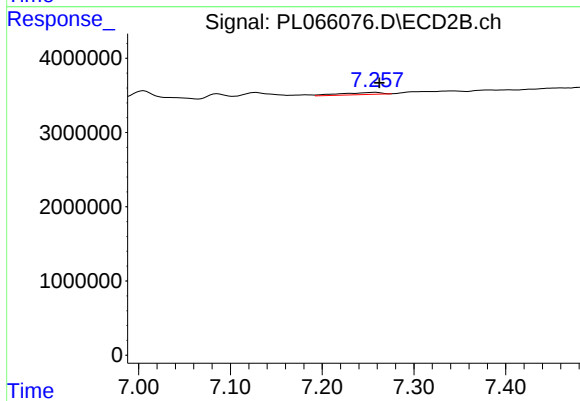


#18 Endrin aldehyde

R.T.: 7.258 min
Delta R.T.: -0.004 min
Response: 888737
Conc: 0.32 ng/ml

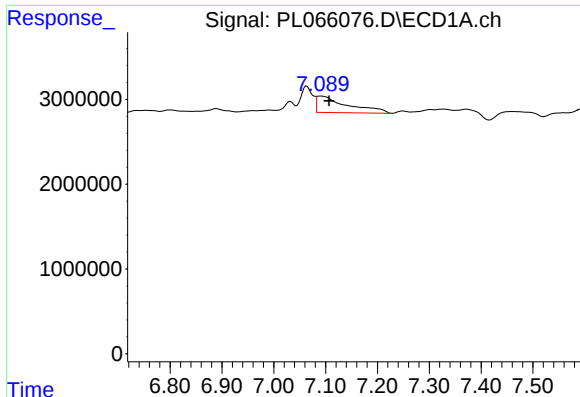


#21 Endrin ketone

R.T.: 7.091 min
Delta R.T.: -0.016 min
Response: 8111211
Conc: 2.25 ng/ml

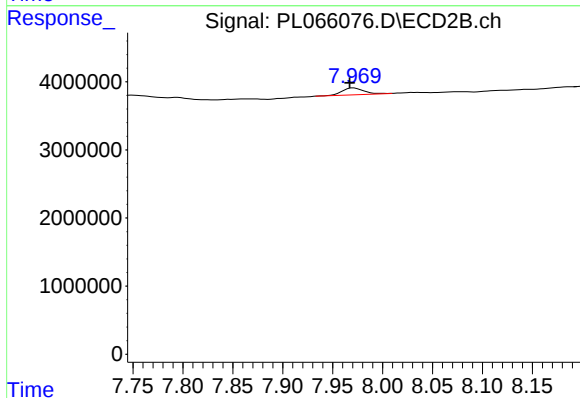


#21 Endrin ketone

R.T.: 7.971 min
Delta R.T.: 0.004 min
Response: 1594686
Conc: 0.43 ng/ml

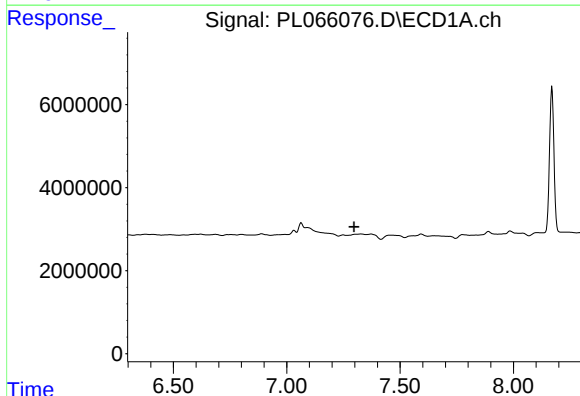


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 7.297 min
Response: 0
Conc: N.D.

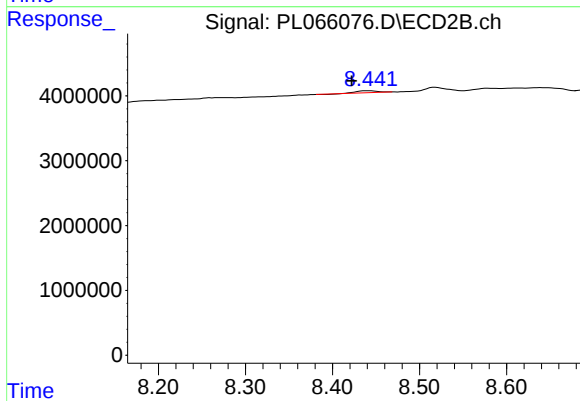


#22 Mirex

R.T.: 8.442 min
Delta R.T.: 0.020 min
Response: 509280
Conc: 0.18 ng/ml

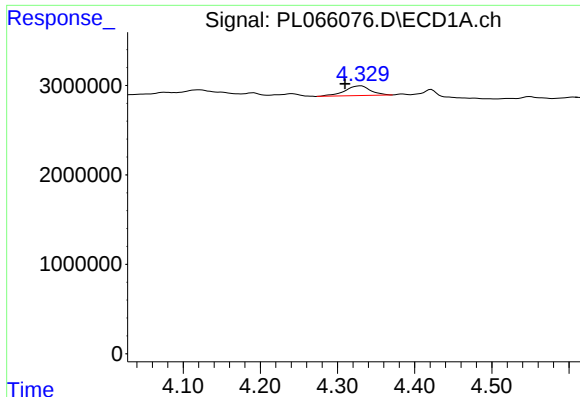


#23 Chlordane-1

R.T.: 4.330 min
Delta R.T.: 0.020 min
Response: 2539143
Conc: 21.18 ng/ml

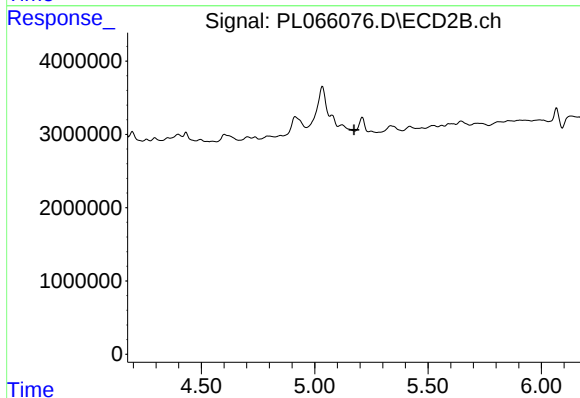


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.175 min
Response: 0
Conc: N.D.

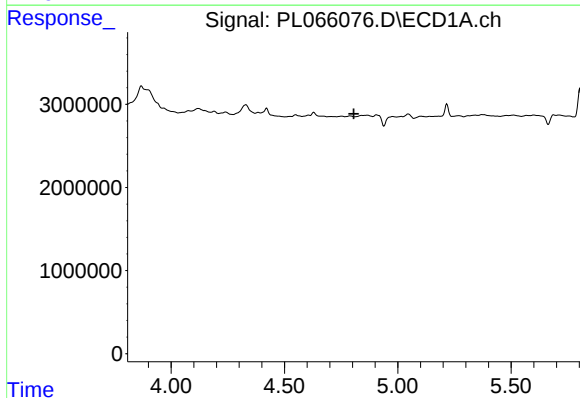


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.806 min
Response: 0
Conc: N.D.

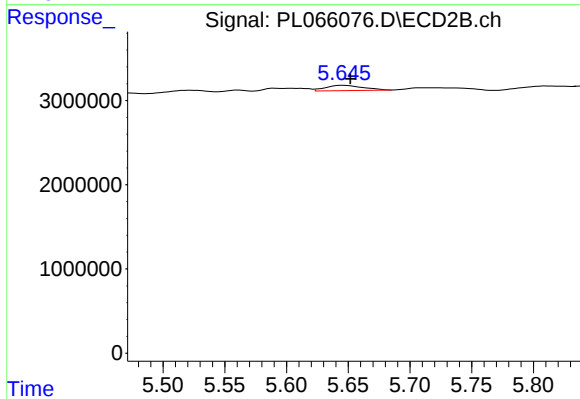


#24 Chlordane-2

R.T.: 5.646 min
Delta R.T.: -0.005 min
Response: 1302193
Conc: 7.07 ng/ml

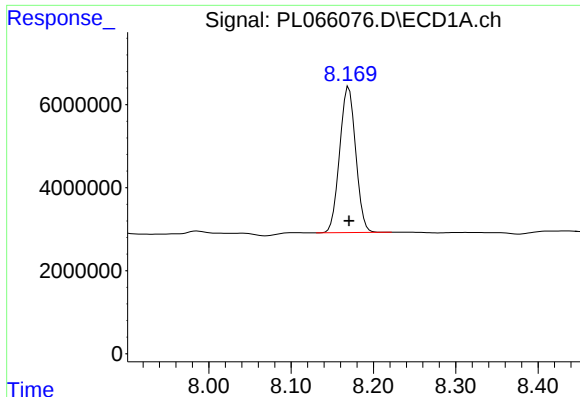

#28 Decachlorobiphenyl

R.T.: 8.170 min
Delta R.T.: 0.000 min
Response: 47578554
Conc: 20.21 ng/ml

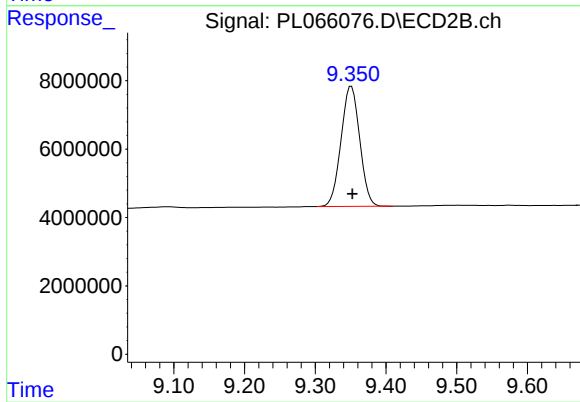

#28 Decachlorobiphenyl

R.T.: 9.351 min
Delta R.T.: -0.002 min
Response: 64524293
Conc: 20.01 ng/ml