

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0041321\
 Data File : P0076976.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Apr 2021 21:09
 Operator : AJ/MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 03:54:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	4.898	3.895	1956307	1063646	21.032	21.196
2)	SA Decachlor...	10.867	9.137	1643853	729268	17.748	15.028
Target Compounds							
9)	L2 AR-1221-2	0.000	4.244	0	12174	N.D.	34.521 #
28)	L6 AR-1254-3	7.759f	0.000	74073	0	13.442	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041321\
Data File : P0076976.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Apr 2021 21:09
Operator : AJ/MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 03:54:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped


Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

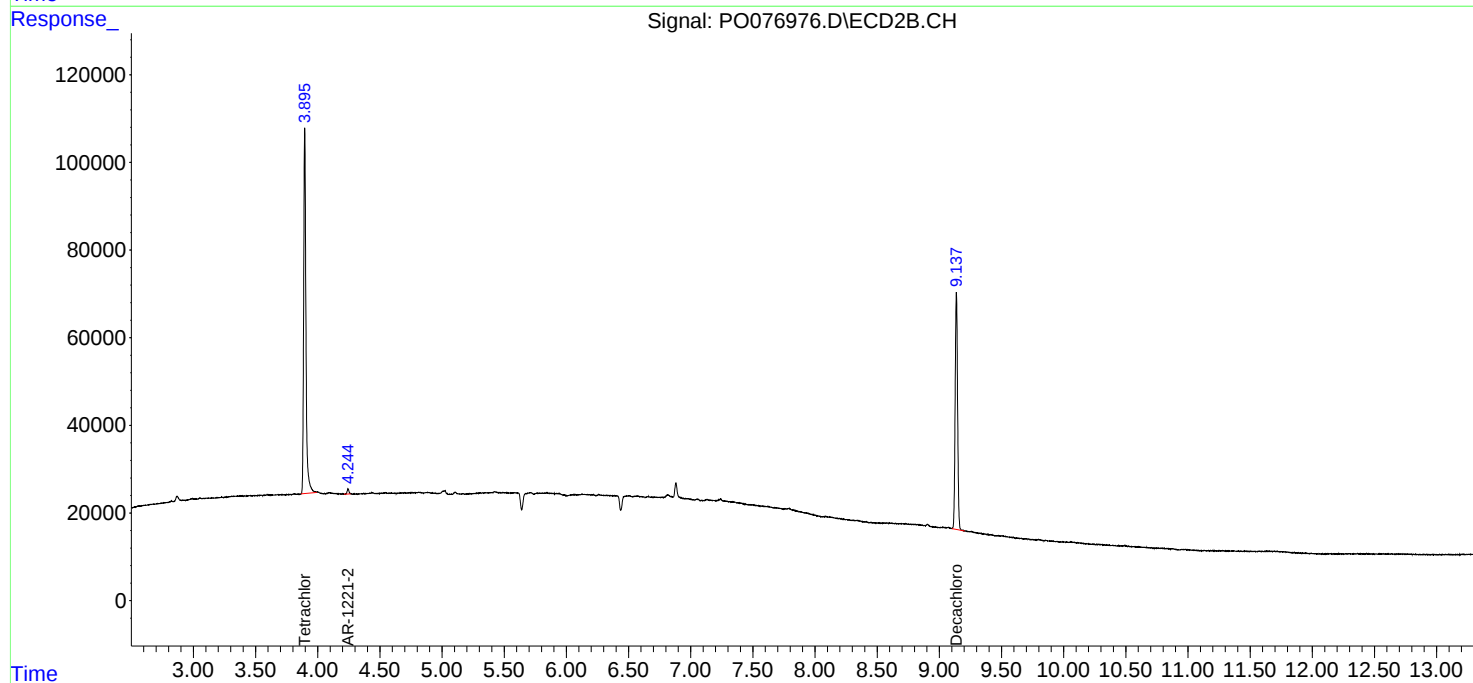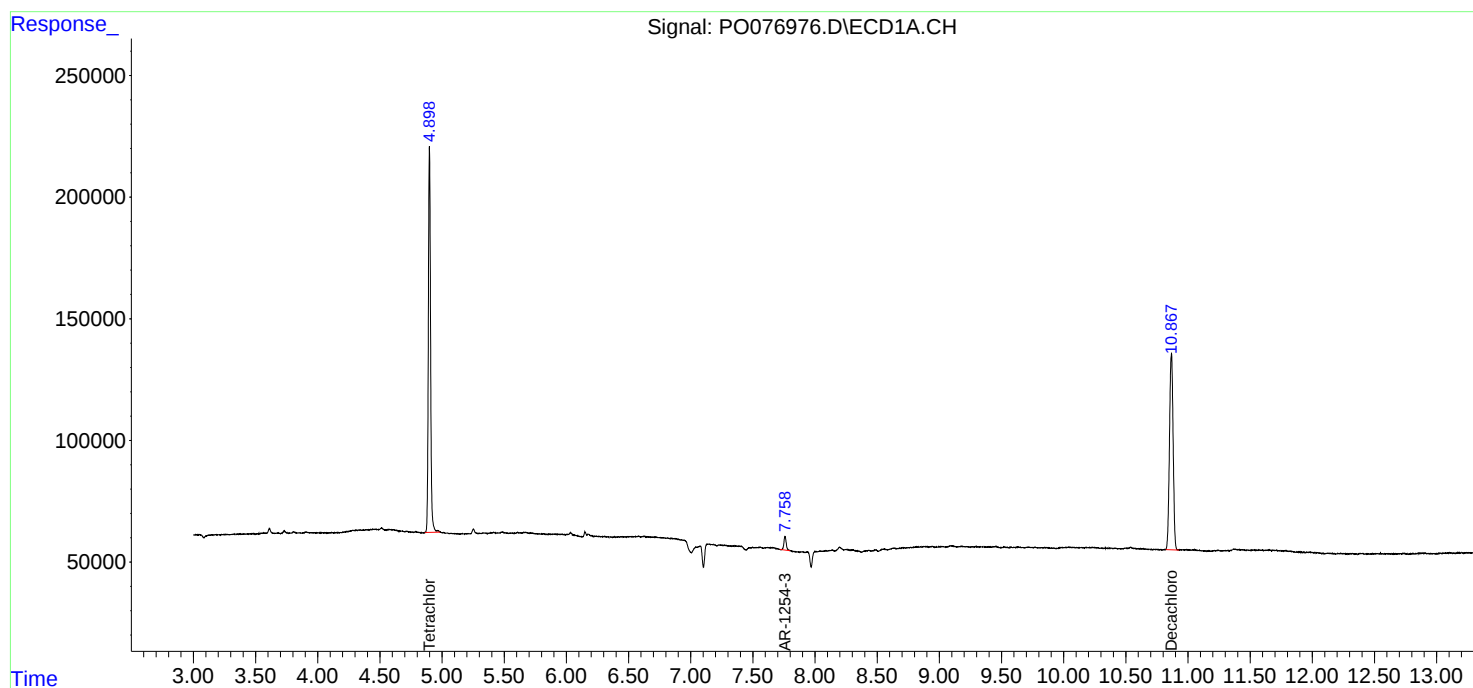

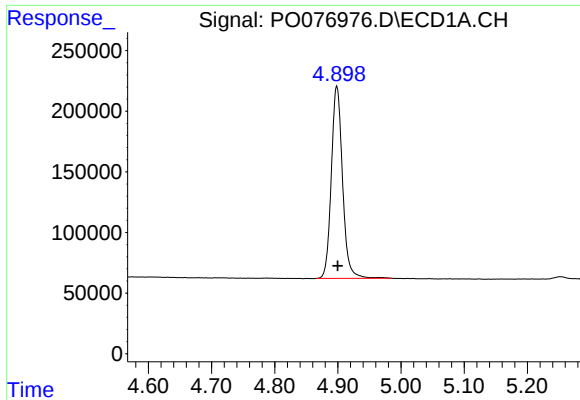


#1 Tetrachloro-m-xylene

R.T.: 4.898 min
Delta R.T.: -0.002 min
Response: 1956307
Conc: 21.03 ng/ml

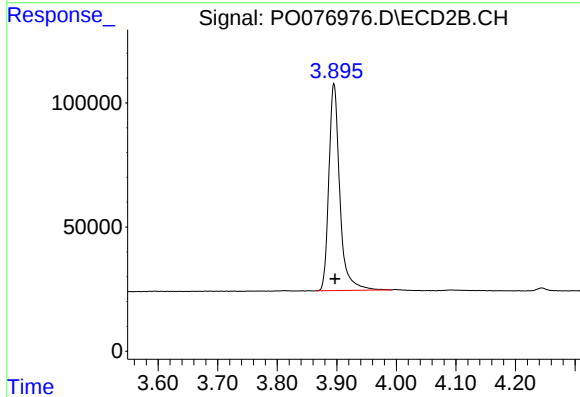


#1 Tetrachloro-m-xylene

R.T.: 3.895 min
Delta R.T.: -0.002 min
Response: 1063646
Conc: 21.20 ng/ml

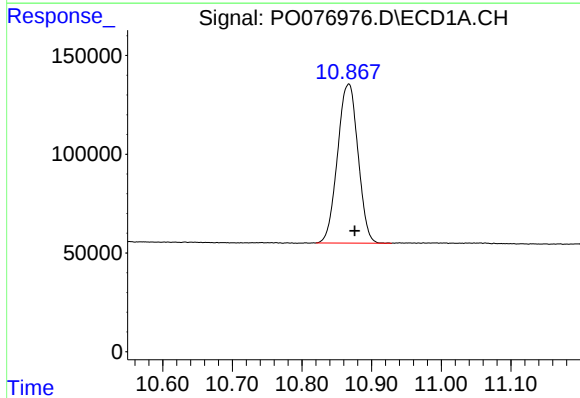


#2 Decachlorobiphenyl

R.T.: 10.867 min
Delta R.T.: -0.008 min
Response: 1643853
Conc: 17.75 ng/ml

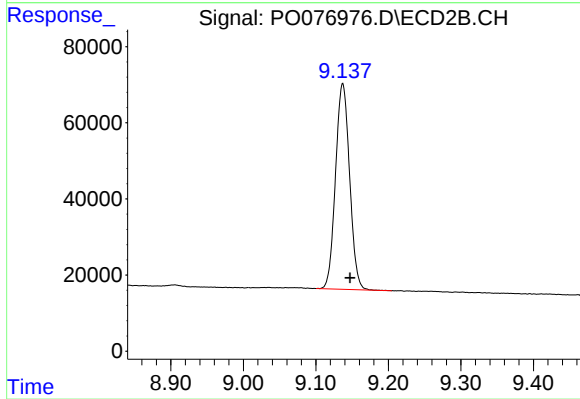


#2 Decachlorobiphenyl

R.T.: 9.137 min
Delta R.T.: -0.010 min
Response: 729268
Conc: 15.03 ng/ml

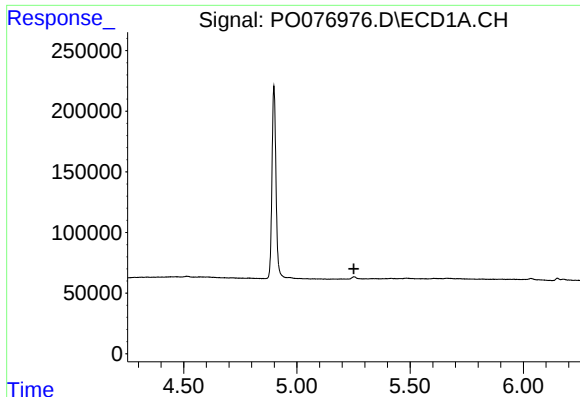


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 5.251 min
Response: 0
Conc: N.D.

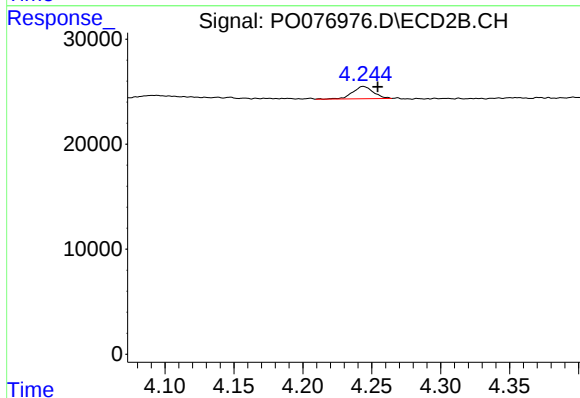


#9 AR-1221-2

R.T.: 4.244 min
Delta R.T.: -0.011 min
Response: 12174
Conc: 34.52 ng/ml

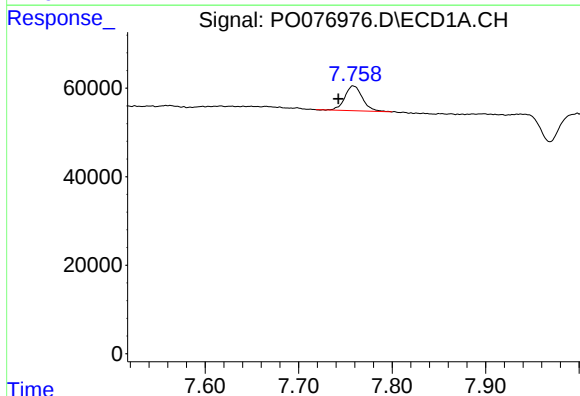

#28 AR-1254-3

R.T.: 7.759 min
Delta R.T.: 0.016 min
Response: 74073
Conc: 13.44 ng/ml

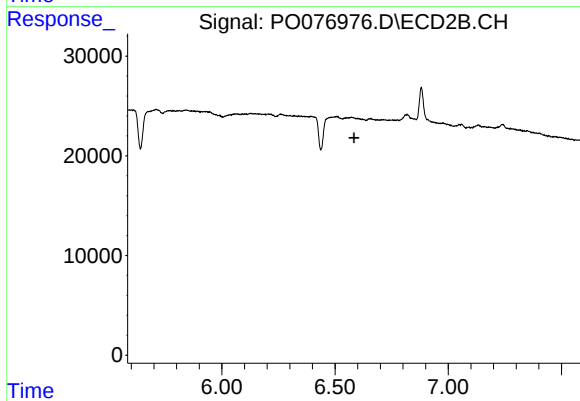

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T.: 6.584 min
Response: 0
Conc: N.D.