

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041321\
 Data File : P0076946.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Apr 2021 11:07
 Operator : AJ/MA
 Sample : M2001-02RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 HA-03RE

Manual Integrations
 APPROVED

Ankita
 4/14/2021 1:53:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 09:01:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.897	3.894	3183955	1789072	34.231	35.651
2) SA Decachlor...	10.856	9.134	5530566	2105934	59.712	43.398m#
Target Compounds						
26) L6 AR-1254-1	7.130	6.001	1874256	418868	589.661	159.804 #
27) L6 AR-1254-2	7.368	6.159	2526888	400601	493.179	174.934 #
28) L6 AR-1254-3	7.740	6.576	723567	531173	131.305	150.292
29) L6 AR-1254-4	8.030	6.814	996254	262480	253.032m	125.069 #
30) L6 AR-1254-5	8.462	7.242	772768	2109189	175.704m	646.988 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO041321\
Data File : PO076946.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Apr 2021 11:07
Operator : AJ/MA
Sample : M2001-02RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
HA-03RE


Manual Integrations
APPROVED

Ankita
4/14/2021 1:53:28 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 09:01:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

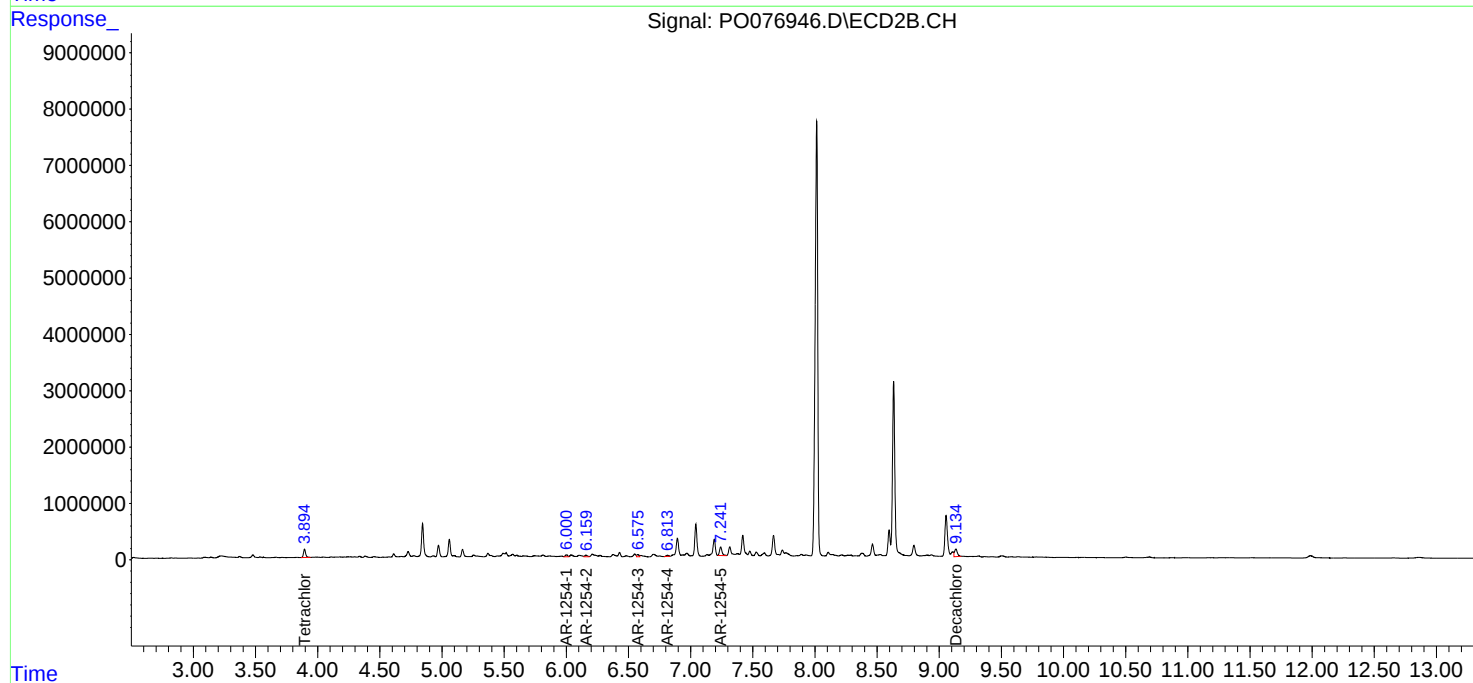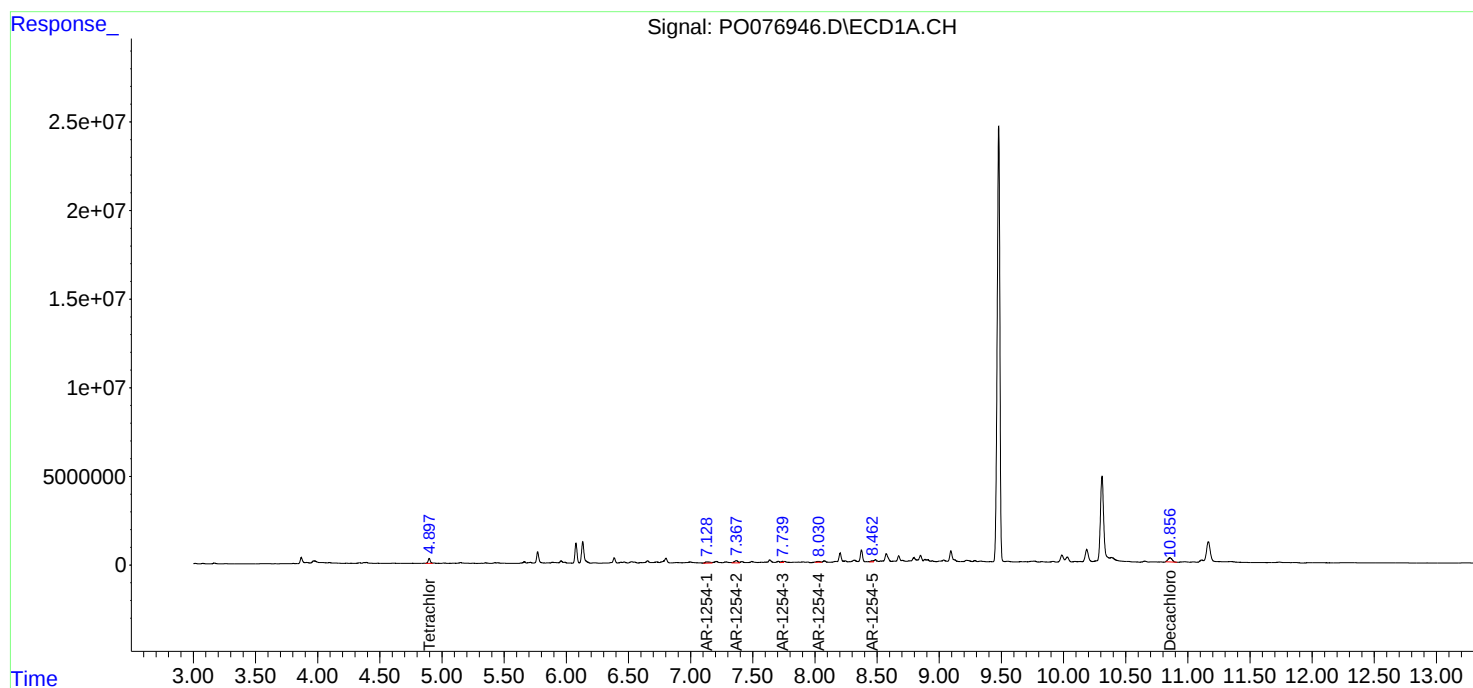

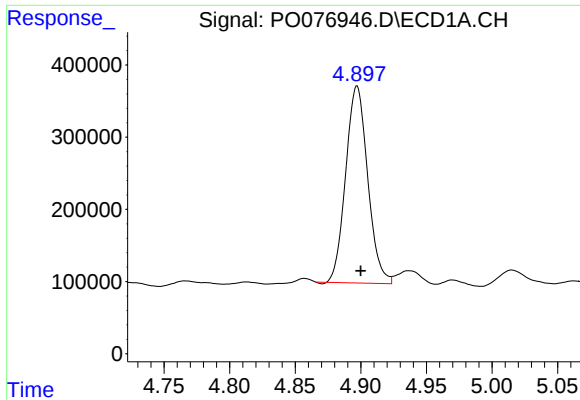


#1 Tetrachloro-m-xylene

R.T.: 4.897 min
Delta R.T.: -0.003 min
Response: 3183955
Conc: 34.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
HA-03RE


Manual Integrations
APPROVED

Ankita
4/14/2021 1:53:28 PM

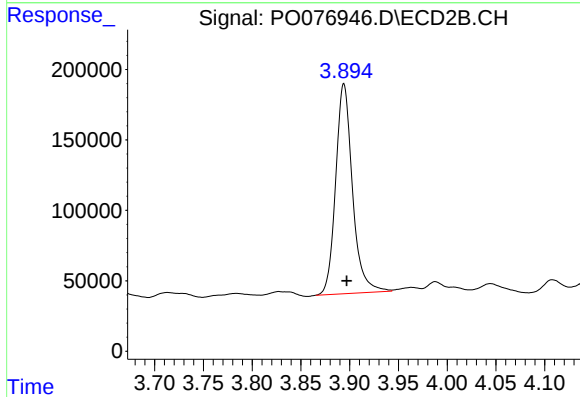


#1 Tetrachloro-m-xylene

R.T.: 3.894 min
Delta R.T.: -0.003 min
Response: 1789072
Conc: 35.65 ng/ml

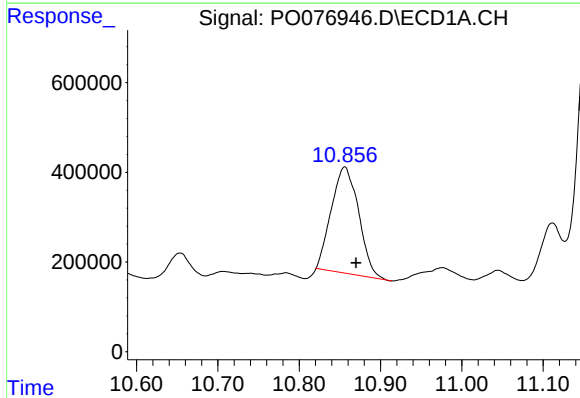


#2 Decachlorobiphenyl

R.T.: 10.856 min
Delta R.T.: -0.014 min
Response: 5530566
Conc: 59.71 ng/ml

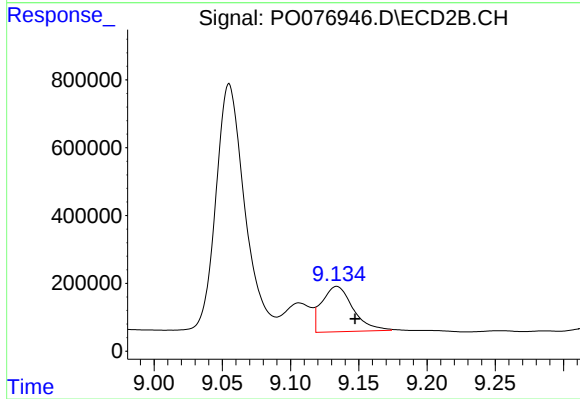

#2 Decachlorobiphenyl

R.T.: 9.134 min
Delta R.T.: -0.014 min
Response: 2105934
Conc: 43.40 ng/ml m

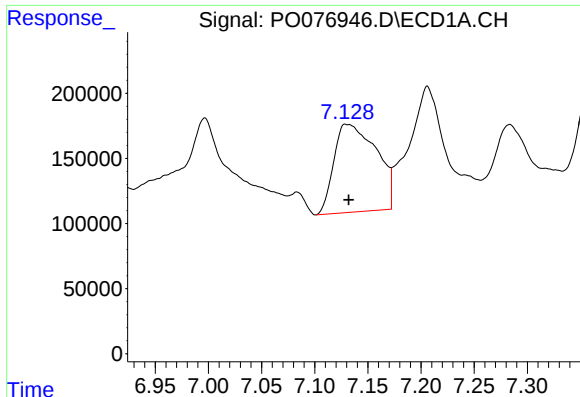


#26 AR-1254-1

R.T.: 7.130 min
Delta R.T.: -0.002 min
Response: 1874256
Conc: 589.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
HA-03RE


Manual Integrations
APPROVED

Ankita
4/14/2021 1:53:28 PM

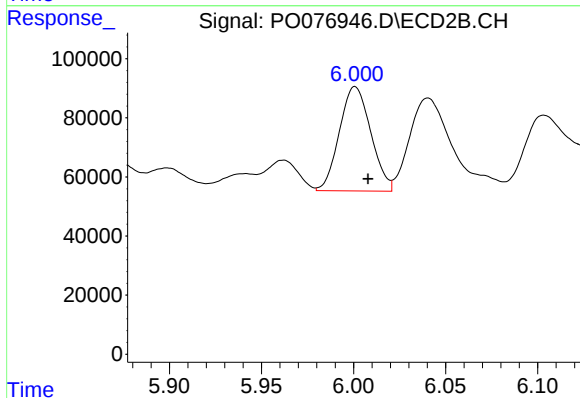


#26 AR-1254-1

R.T.: 6.001 min
Delta R.T.: -0.007 min
Response: 418868
Conc: 159.80 ng/ml

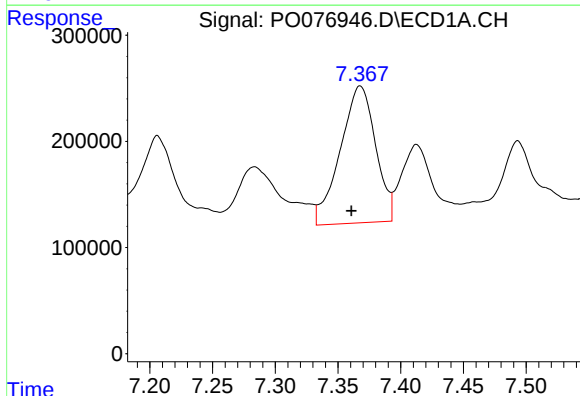


#27 AR-1254-2

R.T.: 7.368 min
Delta R.T.: 0.007 min
Response: 2526888
Conc: 493.18 ng/ml

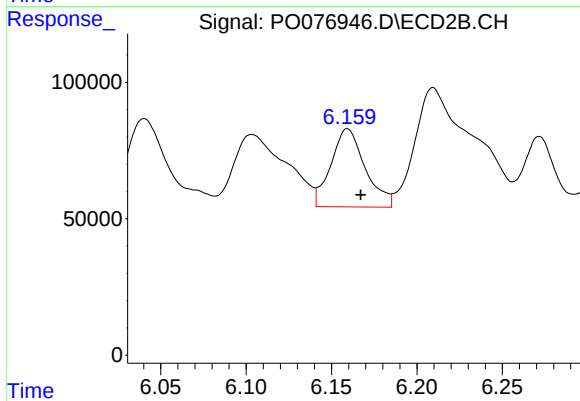

#27 AR-1254-2

R.T.: 6.159 min
Delta R.T.: -0.008 min
Response: 400601
Conc: 174.93 ng/ml

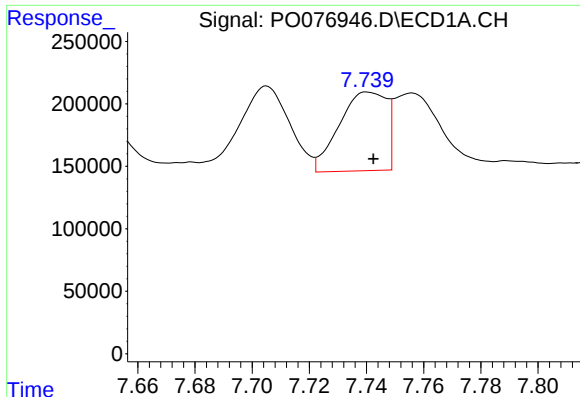


#28 AR-1254-3

R.T.: 7.740 min
Delta R.T.: -0.002 min
Response: 723567
Conc: 131.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
HA-03RE


Manual Integrations
APPROVED

Ankita
4/14/2021 1:53:28 PM

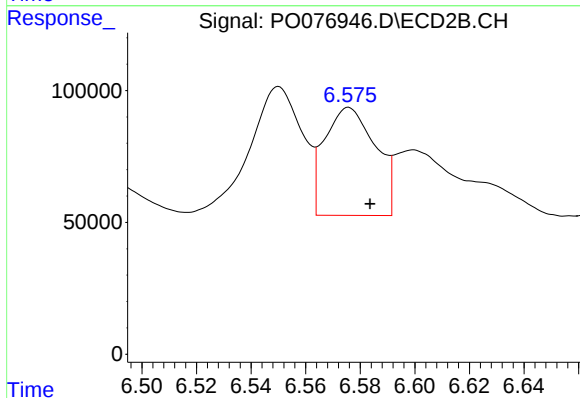


#28 AR-1254-3

R.T.: 6.576 min
Delta R.T.: -0.008 min
Response: 531173
Conc: 150.29 ng/ml

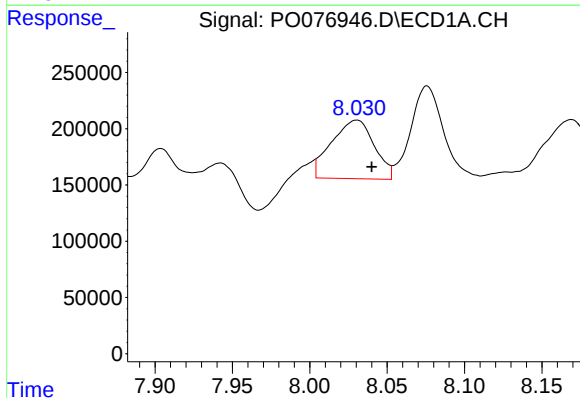


#29 AR-1254-4

R.T.: 8.030 min
Delta R.T.: -0.010 min
Response: 996254
Conc: 253.03 ng/ml m

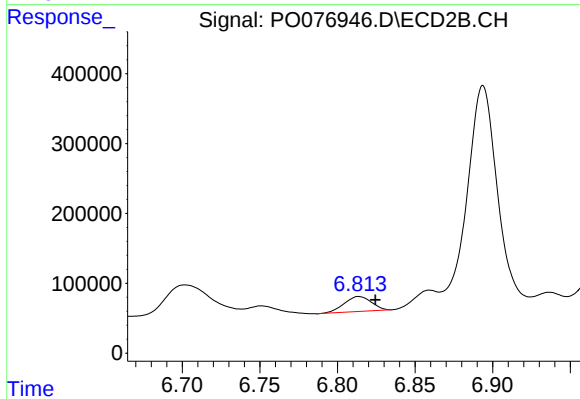

#29 AR-1254-4

R.T.: 6.814 min
Delta R.T.: -0.011 min
Response: 262480
Conc: 125.07 ng/ml

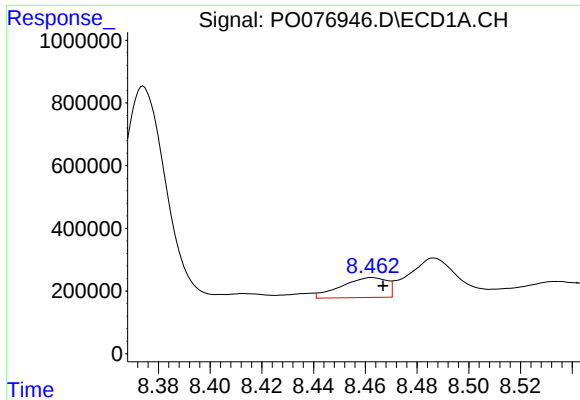


#30 AR-1254-5

R.T.: 8.462 min
Delta R.T.: -0.005 min
Response: 772768
Conc: 175.70 ng/ml m

Instrument :
ECD_O
ClientSampleId :
HA-03RE

Manual Integrations
APPROVED

Ankita
4/14/2021 1:53:28 PM

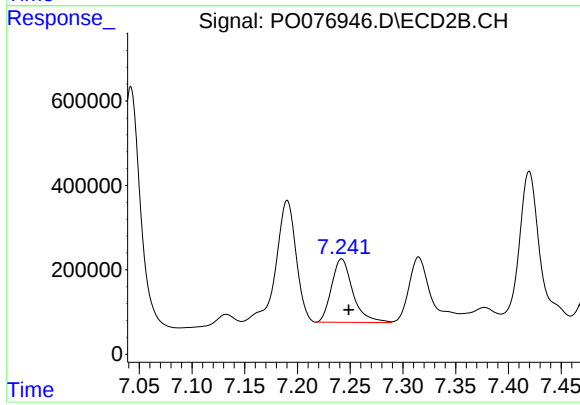

#30 AR-1254-5

R.T.: 7.242 min
Delta R.T.: -0.007 min
Response: 2109189
Conc: 646.99 ng/ml