

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041321\
 Data File : P0076958.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Apr 2021 14:53
 Operator : AJ/MA
 Sample : M2008-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NANUET-ST-041221

Manual Integrations
 APPROVED

Ankita
 4/14/2021 1:53:33 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 13 18:12:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.896	3.893	2198865	1155773	23.640	23.031
2) SA Decachlor...	10.863	9.135	1709258	776338	18.455	15.998m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041321\
Data File : P0076958.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Apr 2021 14:53
Operator : AJ/MA
Sample : M2008-02
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NANUET-ST-041221


Manual Integrations
APPROVED

Ankita
4/14/2021 1:53:33 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 13 18:12:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

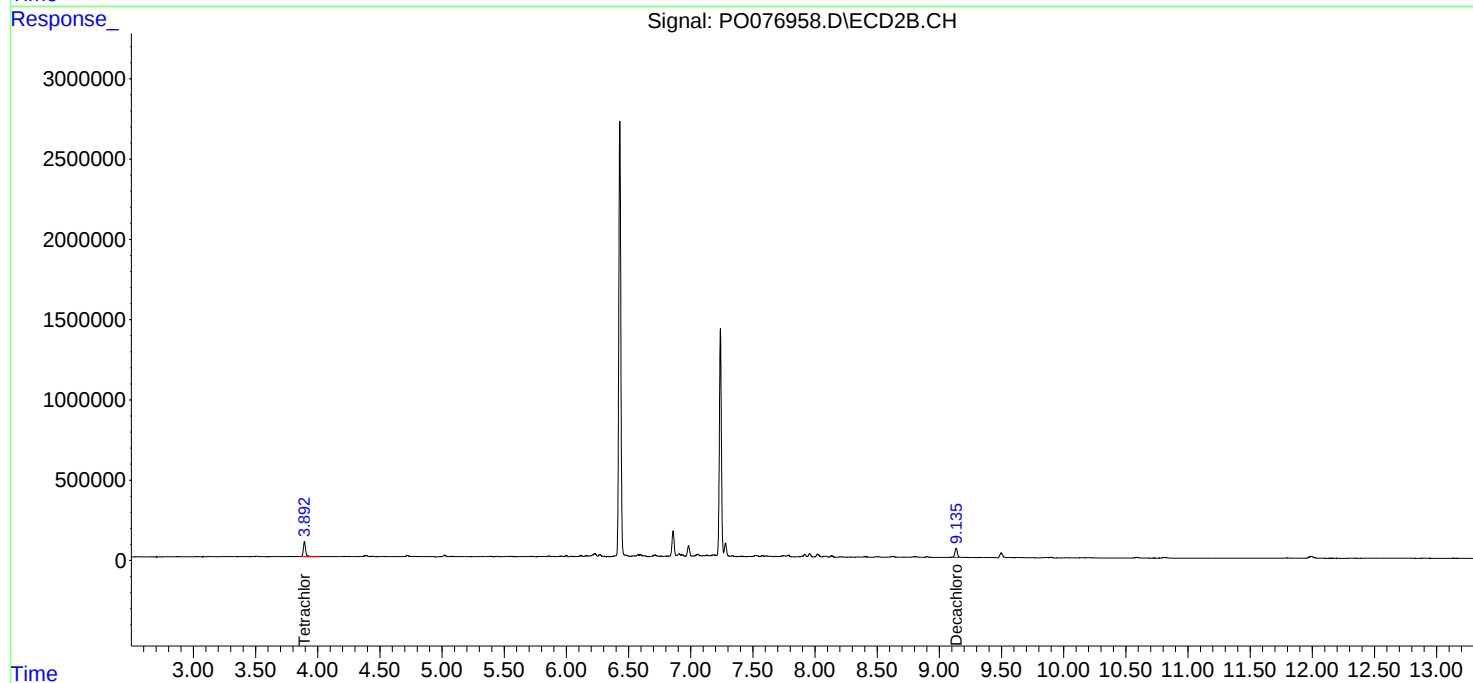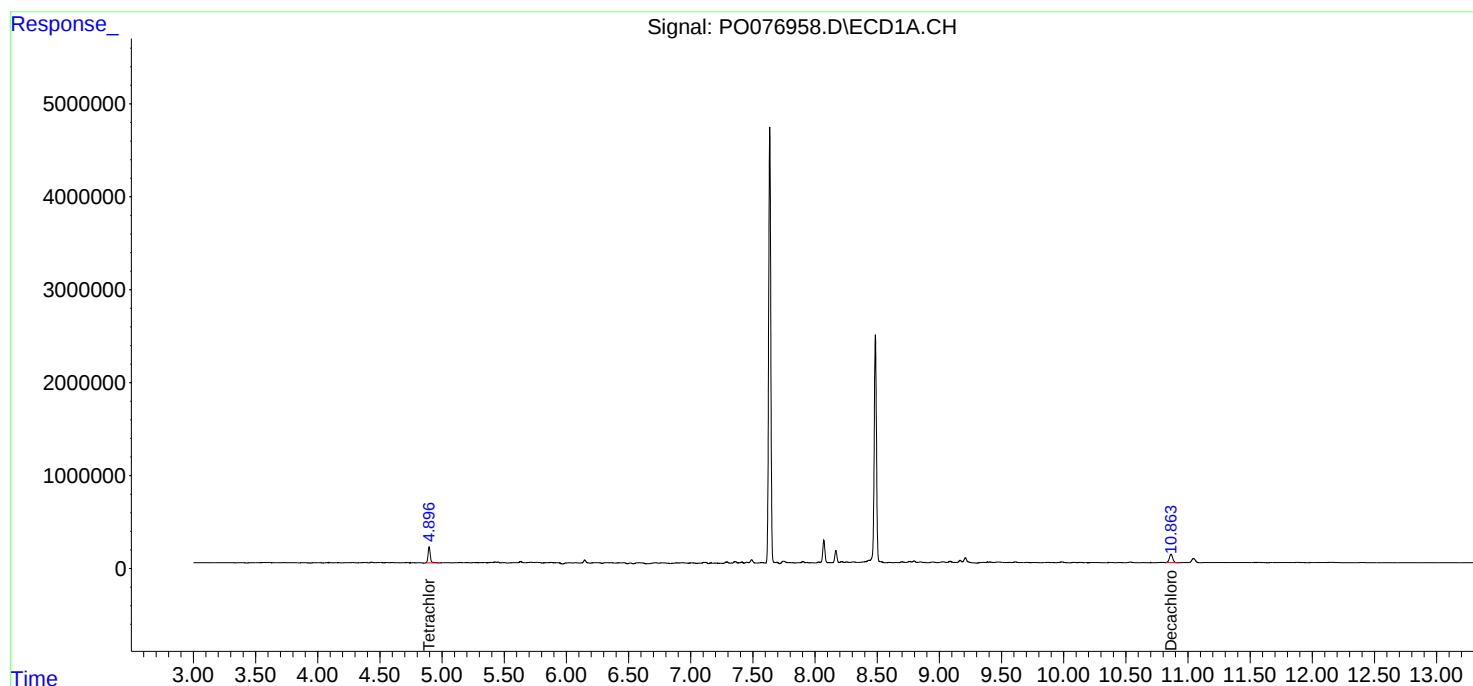

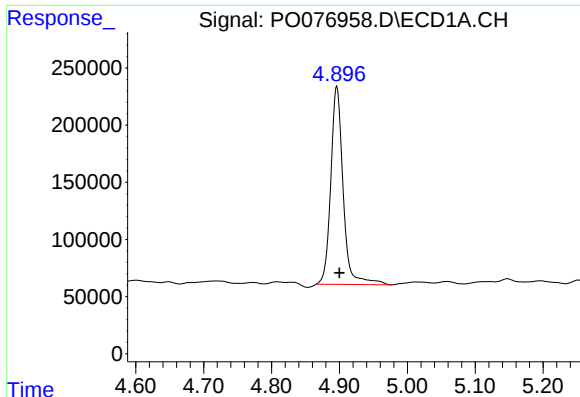


#1 Tetrachloro-m-xylene

R.T.: 4.896 min
Delta R.T.: -0.004 min
Response: 2198865
Conc: 23.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
NANUET-ST-041221


Manual Integrations
APPROVED

Ankita
4/14/2021 1:53:33 PM

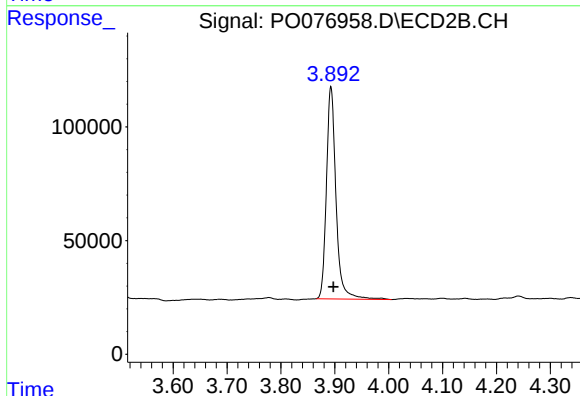


#1 Tetrachloro-m-xylene

R.T.: 3.893 min
Delta R.T.: -0.004 min
Response: 1155773
Conc: 23.03 ng/ml

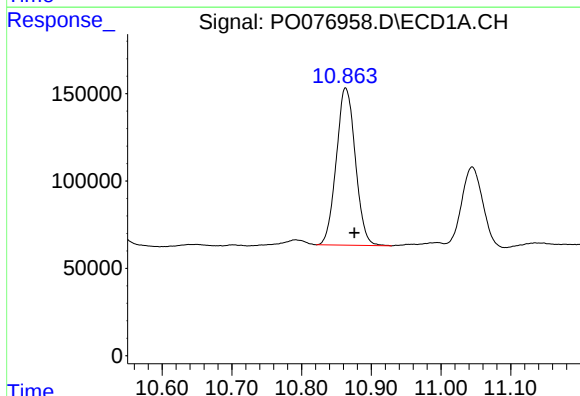

#2 Decachlorobiphenyl

R.T.: 10.863 min
Delta R.T.: -0.012 min
Response: 1709258
Conc: 18.45 ng/ml

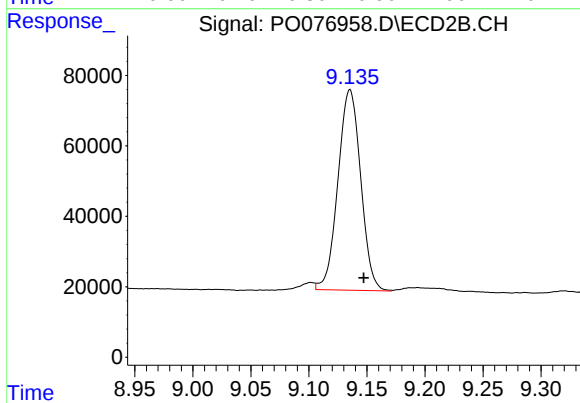

#2 Decachlorobiphenyl

R.T.: 9.135 min
Delta R.T.: -0.012 min
Response: 776338
Conc: 16.00 ng/ml m