

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041321\
 Data File : P0076962.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Apr 2021 16:18
 Operator : AJ/MA
 Sample : M2009-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OR-02-041221

Manual Integrations
 APPROVED

Ankita
 4/14/2021 1:53:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 14 03:47:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Apr 02 05:20:17 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.897	3.894	1988985	1117256	21.384m	22.264
2) SA Decachlor...	10.866	9.136	1647253	733625	17.785	15.118

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0041321\
Data File : P0076962.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Apr 2021 16:18
Operator : AJ/MA
Sample : M2009-01
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OR-02-041221


Manual Integrations
APPROVED

Ankita
4/14/2021 1:53:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 14 03:47:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0040121.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Apr 02 05:20:17 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

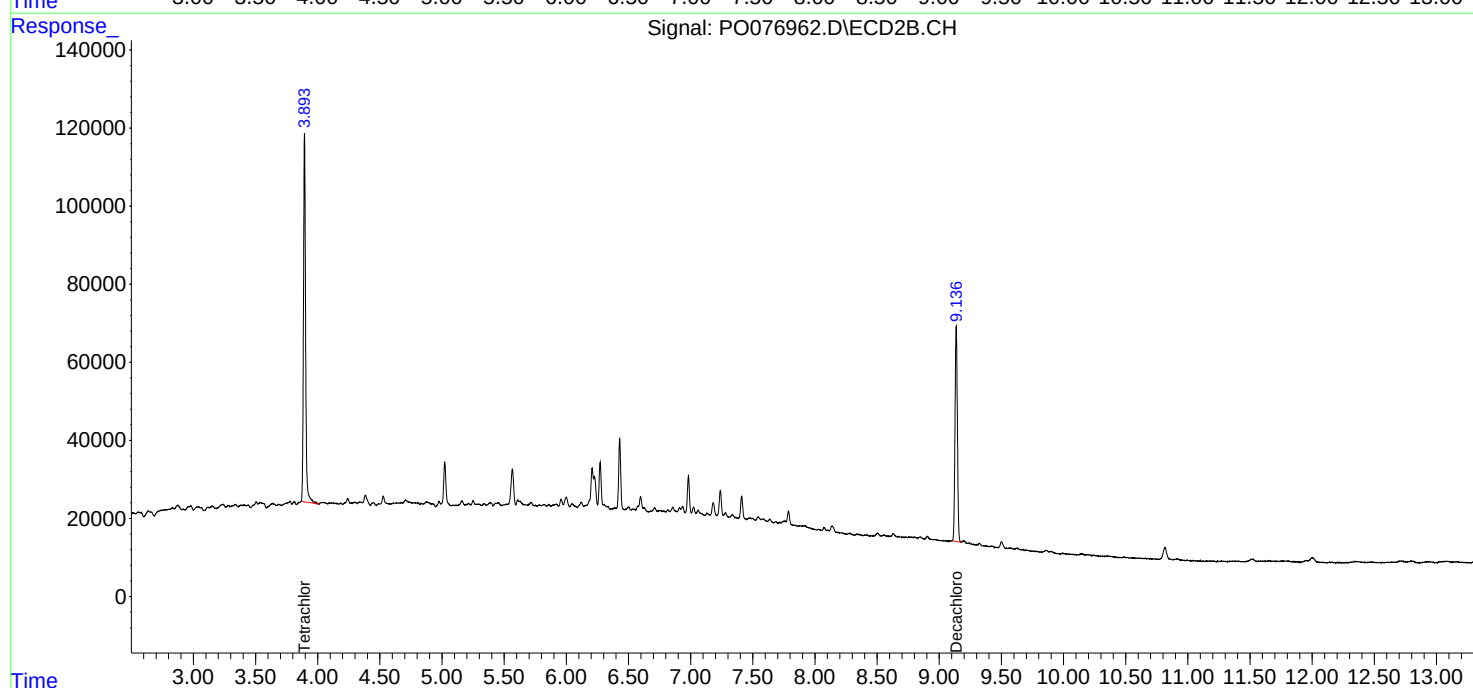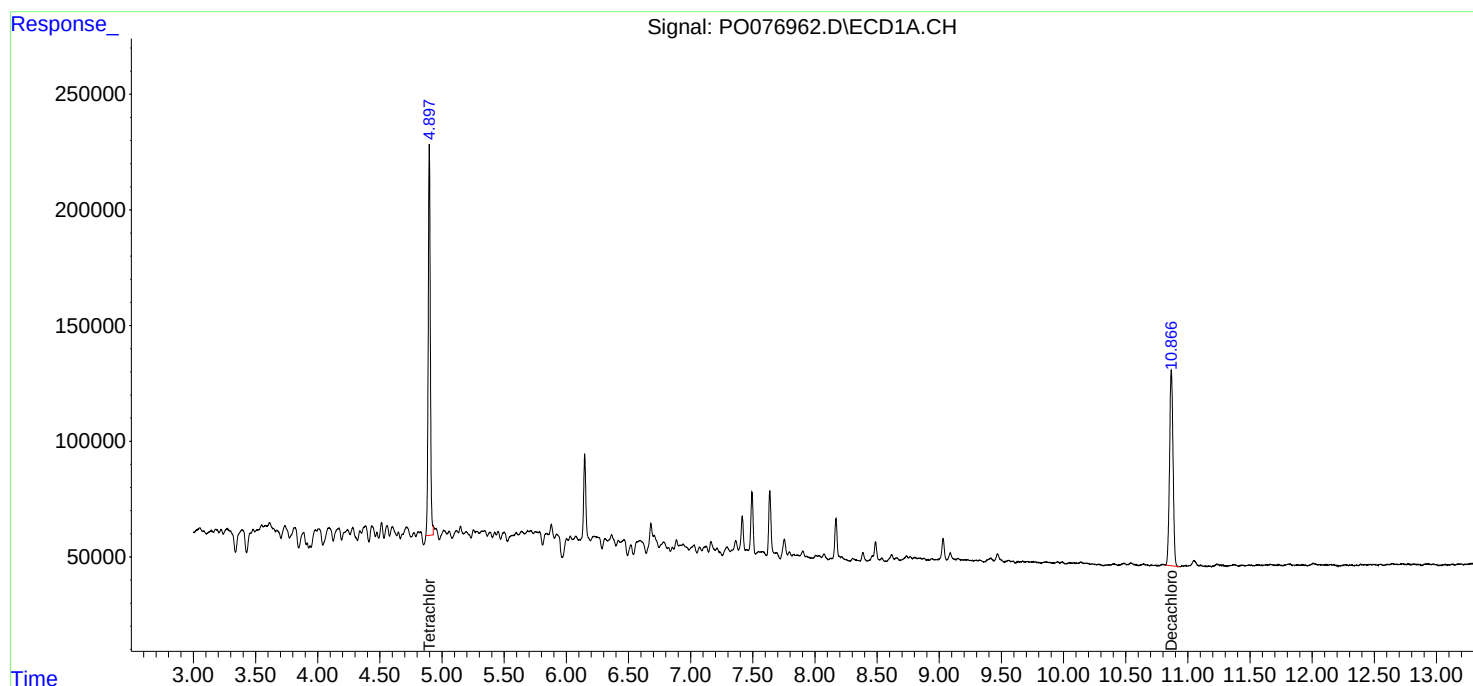

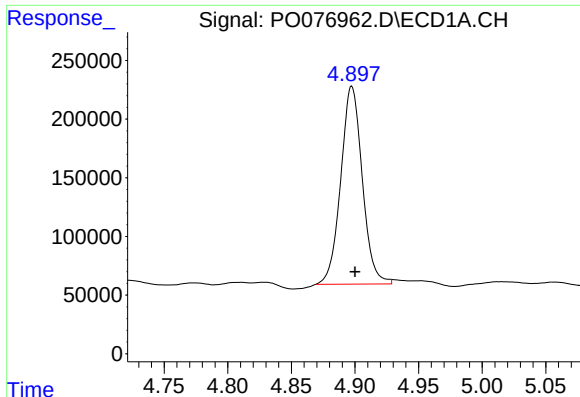


#1 Tetrachloro-m-xylene

R.T.: 4.897 min
Delta R.T.: -0.003 min
Response: 1988985
Conc: 21.38 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OR-02-041221


Manual Integrations
APPROVED

Ankita
4/14/2021 1:53:35 PM

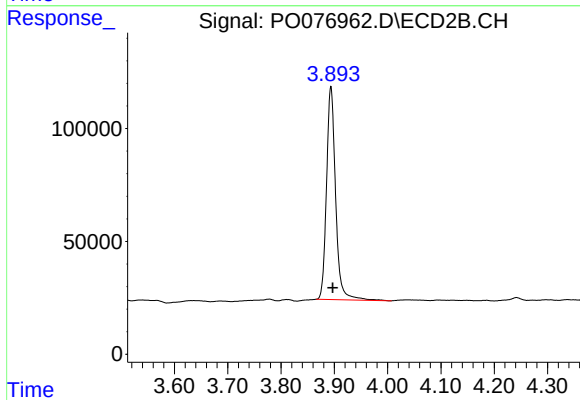


#1 Tetrachloro-m-xylene

R.T.: 3.894 min
Delta R.T.: -0.003 min
Response: 1117256
Conc: 22.26 ng/ml

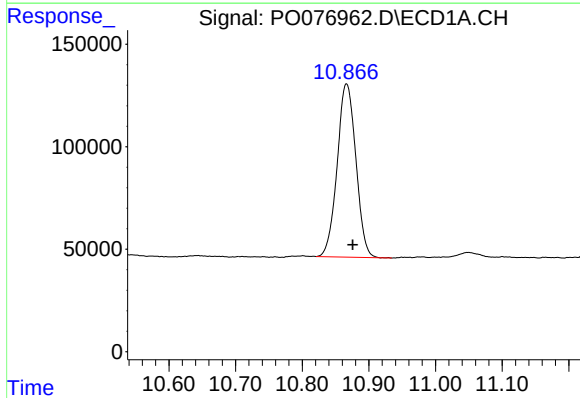

#2 Decachlorobiphenyl

R.T.: 10.866 min
Delta R.T.: -0.009 min
Response: 1647253
Conc: 17.79 ng/ml

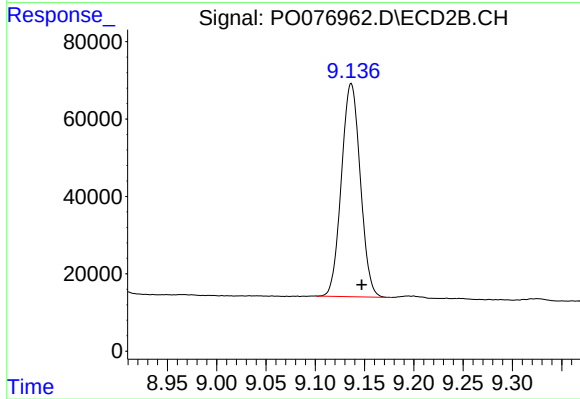

#2 Decachlorobiphenyl

R.T.: 9.136 min
Delta R.T.: -0.011 min
Response: 733625
Conc: 15.12 ng/ml